


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120822\
 Data File : VV029459.D
 Acq On : 08 Dec 2022 08:56
 Operator : SY/MD
 Sample : BFB352
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB352

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis
 Last Update : Thu Dec 08 01:48:46 2022

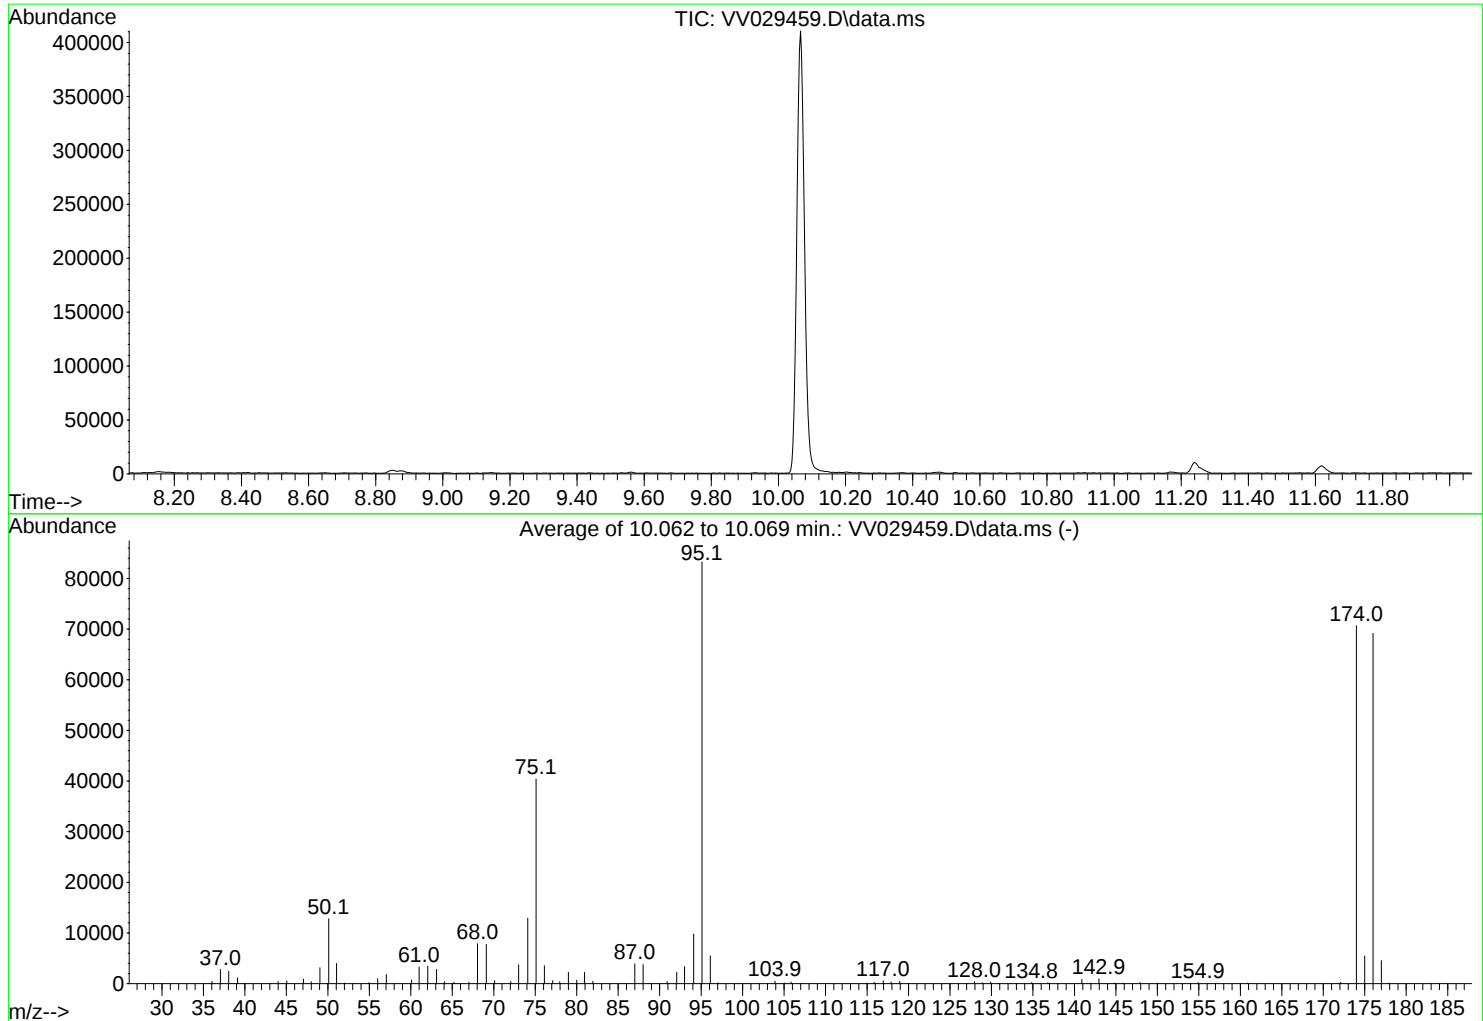

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	12819	PASS
75	95	30	80	48.5	40421	PASS
95	95	100	100	100.0	83280	PASS
96	95	5	9	6.6	5496	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.9	70680	PASS
175	174	5	9	7.7	5453	PASS
176	174	95	105	97.9	69168	PASS
177	176	5	10	6.6	4543	PASS

m/z	Abundance
39.90	192.0
44.00	383.0
207.10	124.0

Instrument :
MSVOA_V
ClientSampleId :
BFB352

m/z	Abundance
36.10	439.0
37.00	2951.0
38.10	2512.0
39.10	1168.0
40.10	252.0
43.10	108.0
44.00	861.0
45.00	586.0
47.00	958.0
48.00	377.0
49.10	3114.0
50.10	12736.0
51.10	4112.0
52.00	159.0
55.00	192.0
56.00	962.0
57.10	1820.0
60.10	746.0
61.00	3423.0
62.10	3465.0
63.10	2899.0
64.00	354.0
65.20	245.0
67.00	240.0
68.10	7870.0
69.10	7745.0
70.10	633.0
72.00	387.0
73.00	3768.0
74.10	12990.0
75.10	40368.0
76.10	3549.0
77.10	631.0
78.00	373.0
79.00	2272.0
80.00	677.0
81.00	2157.0
82.00	535.0
87.00	4044.0
88.00	3838.0
90.90	381.0
92.10	2153.0
93.00	3462.0
94.10	10028.0
95.10	82304.0
96.10	5411.0
97.00	128.0
103.90	426.0
105.00	100.0
105.80	364.0
114.90	133.0
115.80	224.0
116.90	560.0
117.90	313.0
118.90	483.0
128.00	286.0
128.90	186.0
129.90	344.0
131.00	104.0
134.90	198.0
136.80	171.0
140.90	805.0
142.00	130.0
142.90	919.0
144.80	126.0
145.80	100.0
147.90	193.0
150.00	124.0
154.90	271.0
160.90	112.0
171.90	295.0
174.00	68920.0
175.00	5388.0
176.00	66248.0
177.00	4465.0
177.90	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB352

m/z	Abundance
36.00	440.0
37.10	2874.0
38.00	2489.0
39.10	1178.0
40.10	265.0
43.10	116.0
44.00	831.0
45.10	565.0
47.00	908.0
48.00	397.0
49.00	3301.0
50.10	13232.0
51.10	4095.0
52.00	138.0
54.90	194.0
56.00	1003.0
57.10	1831.0
58.10	106.0
60.10	763.0
61.00	3399.0
62.00	3555.0
63.10	2845.0
64.10	396.0
65.20	308.0
67.00	298.0
68.00	8184.0
69.10	8005.0
70.10	600.0
72.00	403.0
73.00	3863.0
74.10	13334.0
75.10	41664.0
76.10	3643.0
77.10	643.0
77.90	399.0
79.00	2283.0
80.00	684.0
80.90	2325.0
82.00	486.0
87.00	4108.0
88.00	3957.0
90.90	428.0
92.10	2304.0
93.00	3464.0
94.10	10080.0
95.10	86008.0
96.10	5677.0
97.10	152.0
103.90	535.0
105.00	133.0
105.90	321.0
114.90	125.0
115.90	254.0
117.00	589.0
117.90	337.0
118.90	490.0
127.90	380.0
128.90	205.0
129.90	330.0
134.80	182.0
136.80	157.0
140.90	879.0
141.90	115.0
142.90	979.0
144.80	144.0
145.80	114.0
147.90	242.0
150.00	136.0
154.90	219.0
160.90	141.0
172.10	370.0
174.00	72976.0
175.00	5616.0
176.00	71488.0
177.00	4767.0
177.90	140.0
207.00	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB352

m/z	Abundance
36.00	428.0
37.10	2582.0
38.00	2317.0
39.10	1054.0
40.10	235.0
44.00	708.0
45.10	488.0
47.10	845.0
48.00	401.0
49.00	3061.0
50.10	12489.0
51.00	3747.0
52.00	130.0
55.00	194.0
56.00	970.0
57.00	1774.0
60.10	703.0
61.00	3045.0
62.00	3279.0
63.10	2662.0
64.10	386.0
65.20	337.0
67.00	294.0
68.00	7510.0
69.10	7444.0
70.10	532.0
72.10	416.0
73.00	3556.0
74.10	12421.0
75.10	39232.0
76.10	3391.0
77.10	563.0
77.90	389.0
79.00	2200.0
80.00	622.0
80.90	2250.0
81.90	429.0
86.00	161.0
87.00	3650.0
88.00	3490.0
88.80	155.0
90.90	388.0
92.00	2363.0
93.00	3158.0
94.10	9292.0
95.10	81528.0
96.10	5399.0
97.10	165.0
103.90	538.0
105.10	146.0
105.90	282.0
115.90	263.0
117.00	524.0
117.90	304.0
119.00	399.0
127.90	413.0
128.90	190.0
129.90	285.0
130.80	114.0
134.80	161.0
136.80	169.0
140.90	900.0
143.00	942.0
144.80	143.0
145.80	113.0
147.90	270.0
155.00	143.0
157.00	106.0
160.90	131.0
172.10	444.0
174.00	70144.0
175.00	5355.0
176.00	69768.0
177.00	4398.0
177.90	132.0
207.00	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB352