

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120823\
 Data File : VW033197.D
 Acq On : 08 Dec 2023 17:49
 Operator : SY/MD
 Sample : 05689-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 08 22:02:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	267034	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	265208	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	135212	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	67054	42.005	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	84.020%		
7) Chloroethane-d5	1.532	69	51638	46.426	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.860%		
11) 1,1-Dichloroethene-d2	2.060	65	27556	45.376	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.760%		
21) 2-Butanone-d5	3.783	46	79537	100.316	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	100.320%		
24) Chloroform-d	4.249	84	159404	47.054	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.100%		
26) 1,2-Dichloroethane-d4	4.940	65	106077	50.363	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.720%		
32) Benzene-d6	4.960	84	297309	47.933	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.860%		
36) 1,2-Dichloropropane-d6	5.989	67	79567	47.710	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.420%		
41) Toluene-d8	7.246	98	276700	46.764	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.520%		
43) trans-1,3-Dichloroprop...	7.555	79	47033	44.599	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.200%		
47) 2-Hexanone-d5	8.024	63	64432	96.169	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	96.170%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84	115005	48.510	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	97.020%		
66) 1,2-Dichlorobenzene-d4	11.561	152	131001	54.454	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.900%		
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	11.185	75	11943	7.084	ug/L #	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033197.D
Acq On : 08 Dec 2023 17:49
Operator : SY/MD
Sample : 05689-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 08 22:02:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration

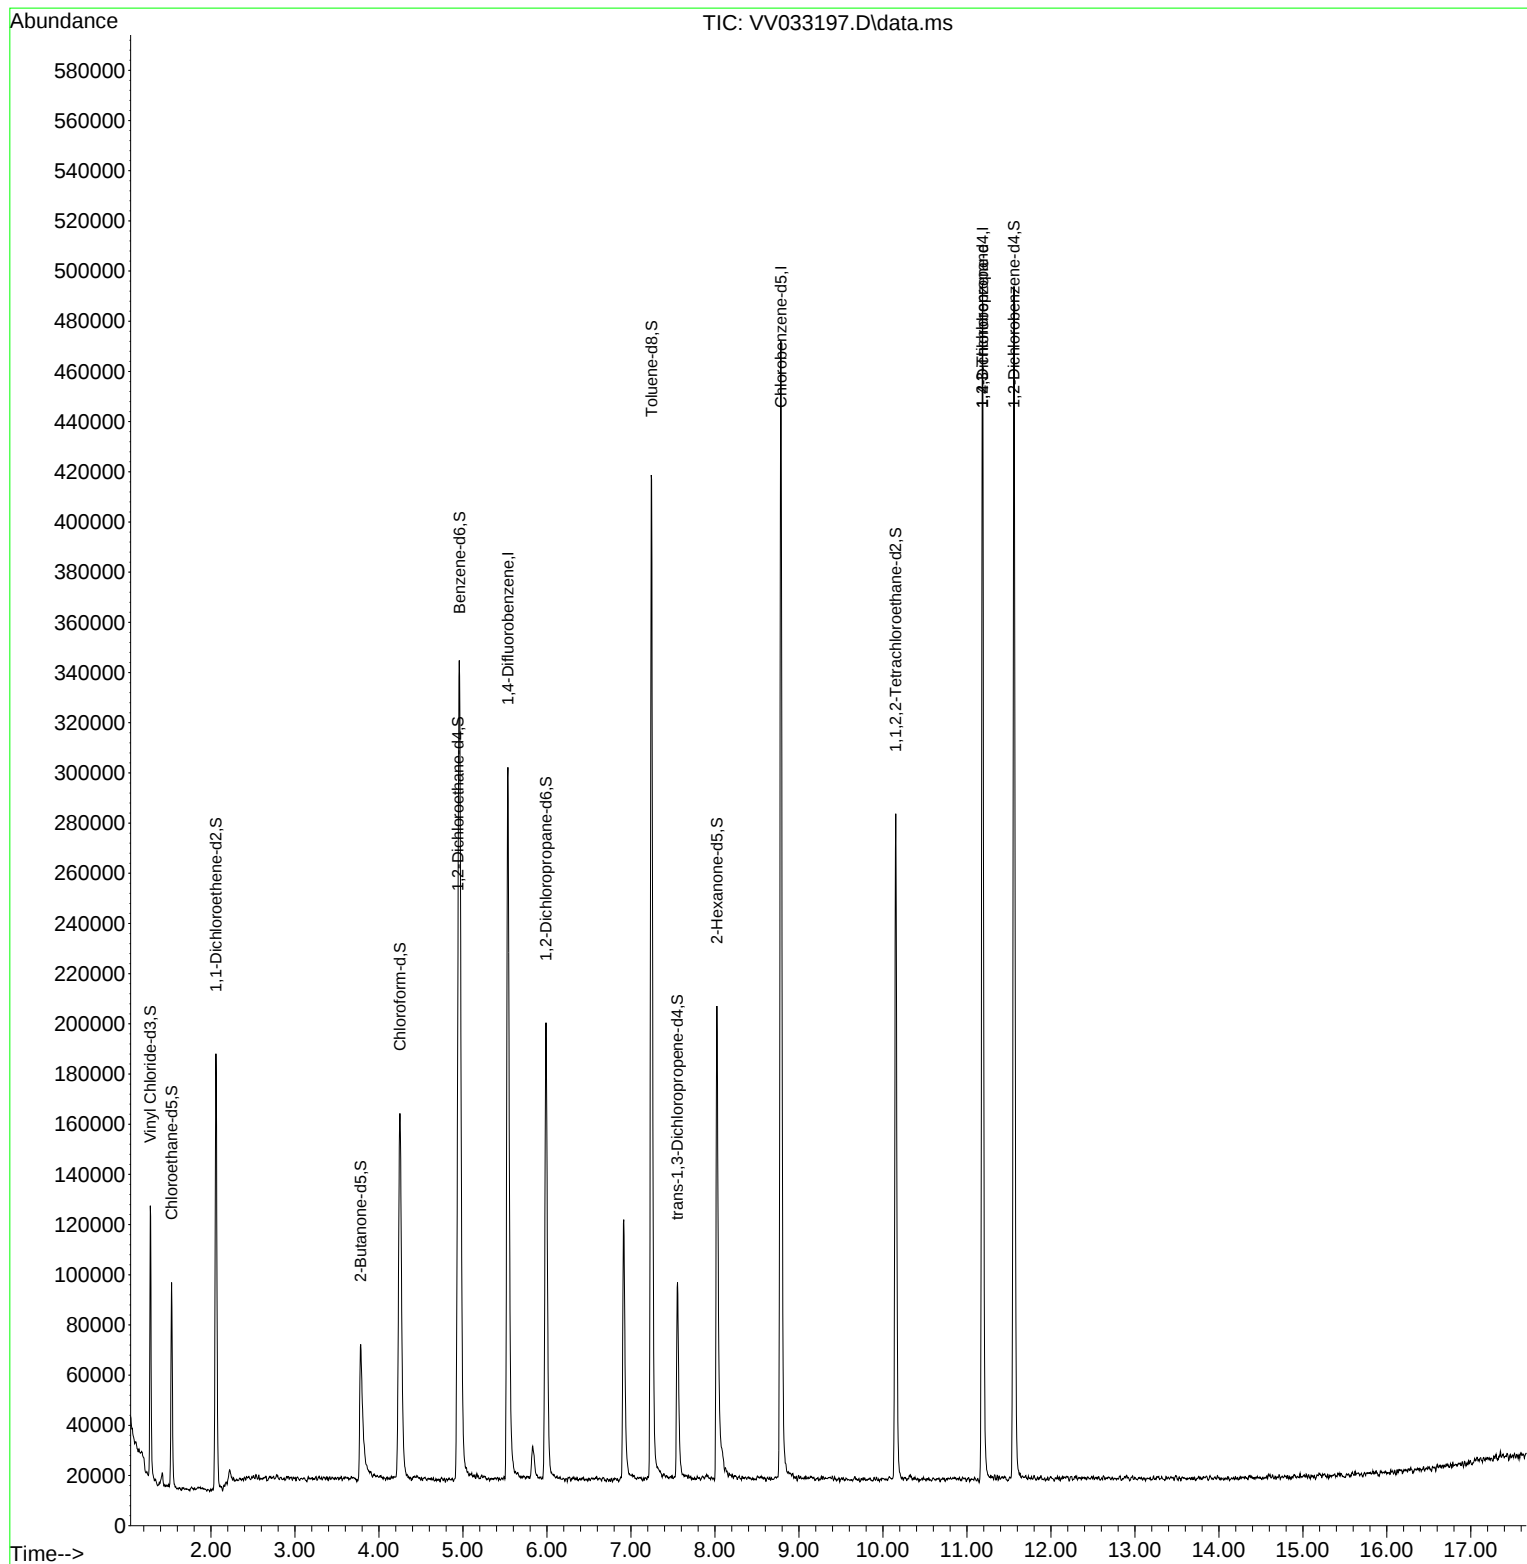

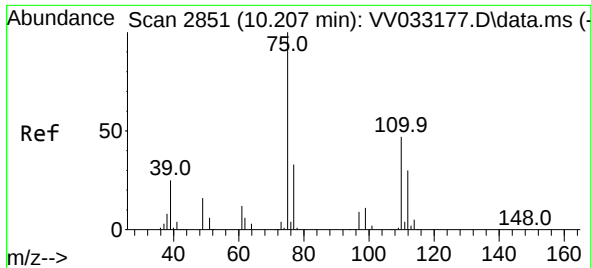

#61
 1,2,3-Trichloropropane
 Concen: 7.084 ug/L
 RT: 11.185 min Scan# 31
 Delta R.T. 0.977 min
 Lab File: VV033197.D
 Acq: 08 Dec 2023 17:49

Instrument :
 MSVOA_V
 ClientSampleId :

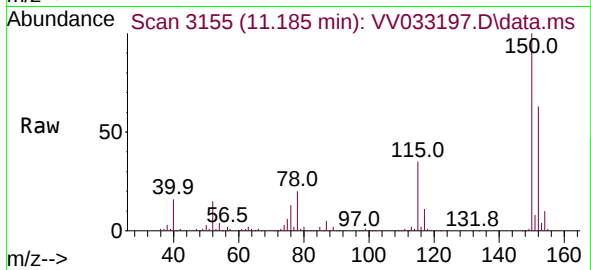

Tgt Ion: 75	Resp:	11943
Ion Ratio	Lower	Upper
75	100	
77	36.8	27.0 40.6
110	1.9	38.1 57.1#

