

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120823\
 Data File : VW033189.D
 Acq On : 08 Dec 2023 14:42
 Operator : SY/MD
 Sample : 05685-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHA9

Quant Time: Dec 08 22:01:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 08 21:51:12 2023
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Semsettin Yesilyurt 12/11/2023
 Supervised By :Mahesh Dadoda 12/11/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	252983	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	260604	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	133313	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	60778	40.188	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.380%		
7) Chloroethane-d5	1.532	69	48454	45.983	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.960%		
11) 1,1-Dichloroethene-d2	2.060	65	25174	43.756	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.520%		
21) 2-Butanone-d5	3.780	46	78751	104.841	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	104.840%		
24) Chloroform-d	4.246	84	157775	49.159	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.320%		
26) 1,2-Dichloroethane-d4	4.940	65	104211	52.225	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.460%		
32) Benzene-d6	4.960	84	288149	47.277	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.560%		
36) 1,2-Dichloropropane-d6	5.989	67	78831	48.103	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.200%		
41) Toluene-d8	7.243	98	262900	45.217	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.440%		
43) trans-1,3-Dichloroprop...	7.555	79	45949	44.340	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.680%		
47) 2-Hexanone-d5	8.024	63	62133	94.376	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	94.380%		
56) 1,1,2,2-Tetrachloroeth...	10.152	84	114301	49.065	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.120%		
66) 1,2-Dichlorobenzene-d4	11.561	152	126379	53.281	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.560%		
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.069	96	2885	2.275	ug/L	# 1
13) Acetone	2.111	43	24460	34.110	ug/L	97
19) 1,1-Dichloroethane	3.111	63	8182	2.969	ug/L	97
22) 2-Butanone	3.883	43	16482m	18.061	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033189.D
Acq On : 08 Dec 2023 14:42
Operator : SY/MD
Sample : 05685-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
YCHA9

Quant Time: Dec 08 22:01:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 08 21:51:12 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/11/2023
Supervised By :Mahesh Dadoda 12/11/2023

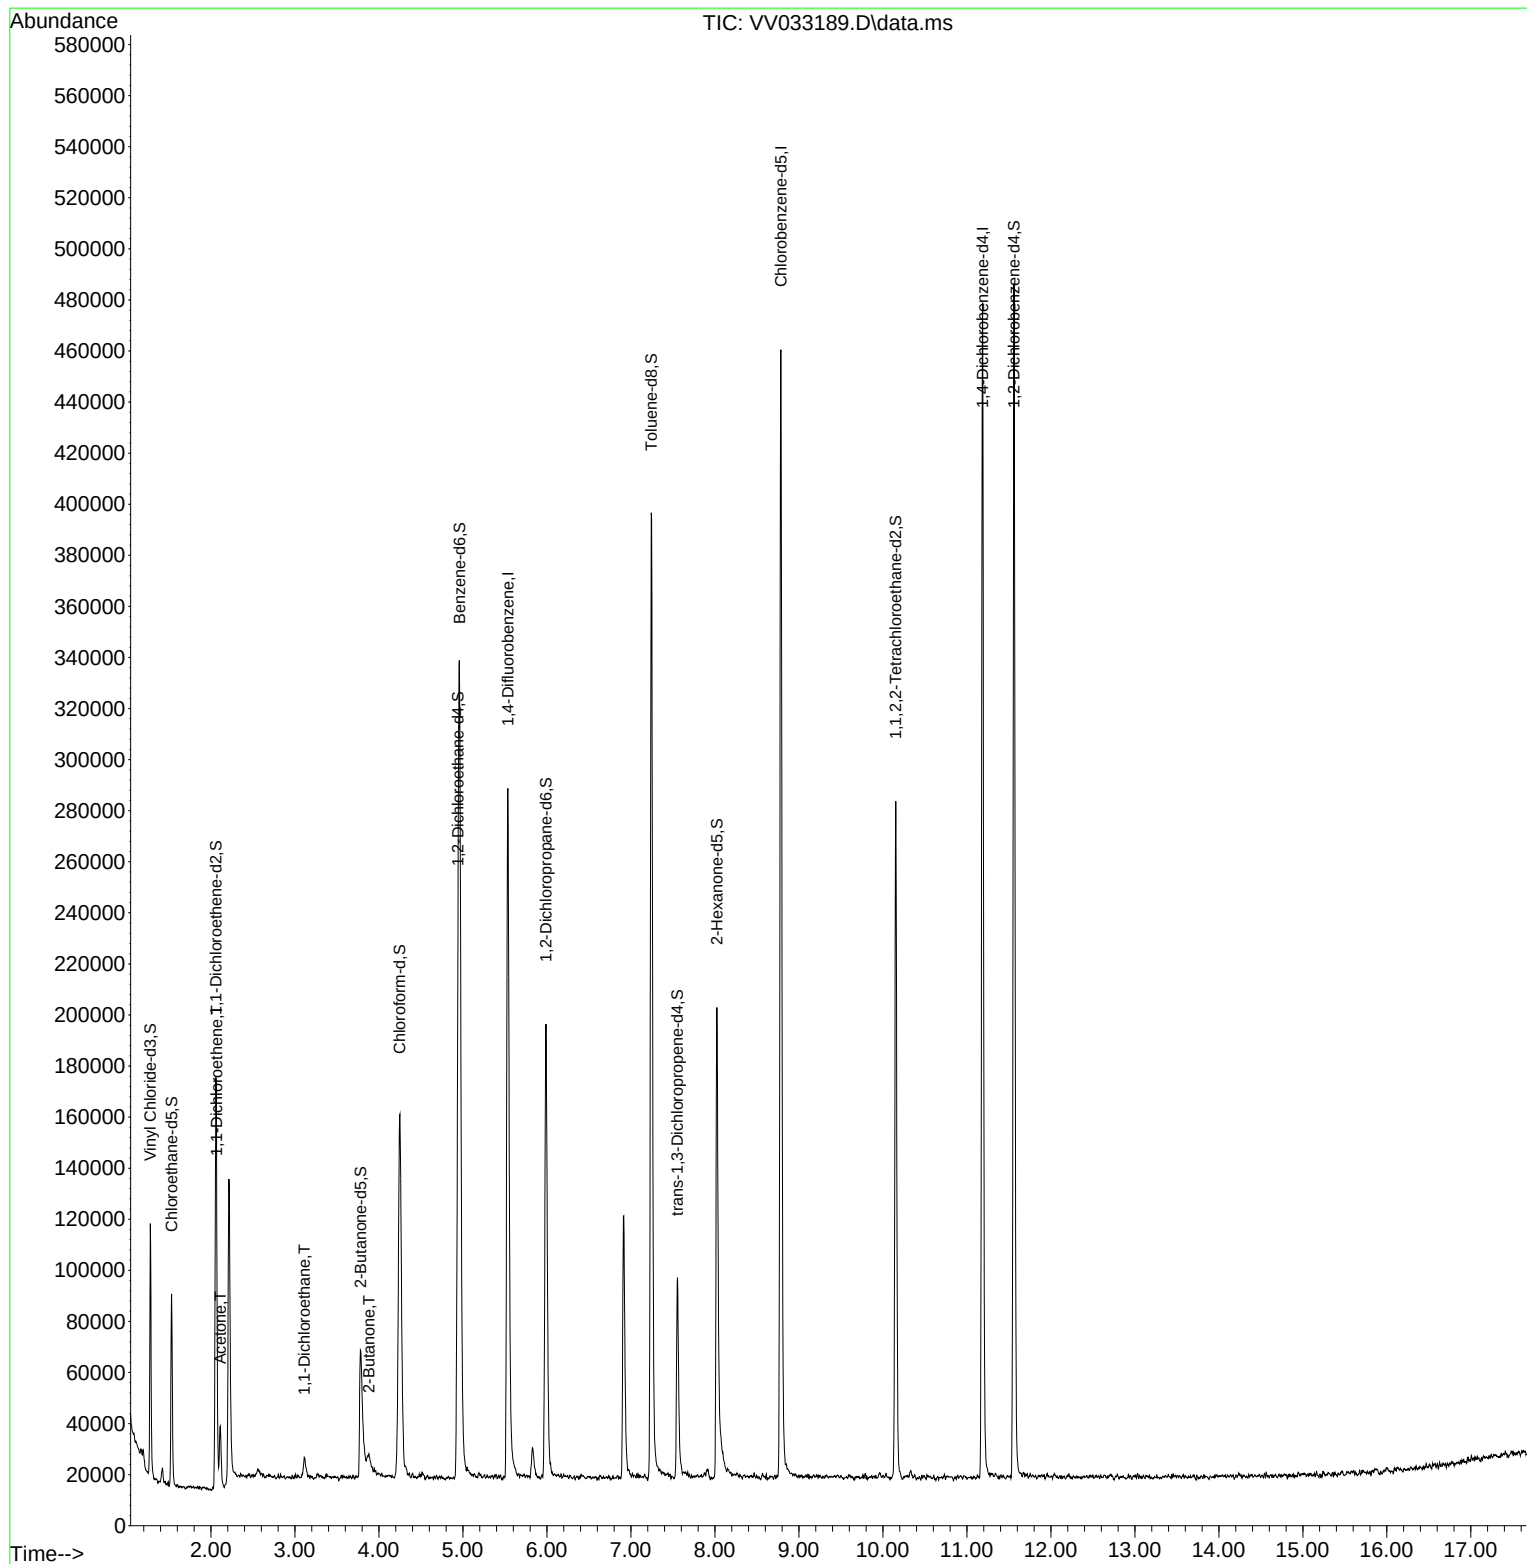

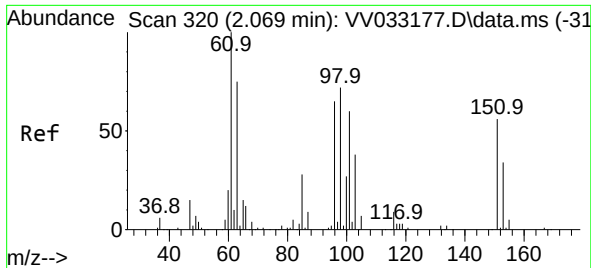

#12
1,1-Dichloroethene
Concen: 2.275 ug/L
RT: 2.069 min Scan# 31
Delta R.T. -0.000 min
Lab File: VV033189.D
Acq: 08 Dec 2023 14:42




Instrument :
MSVOA_V
ClientSampleId :
YCHA9

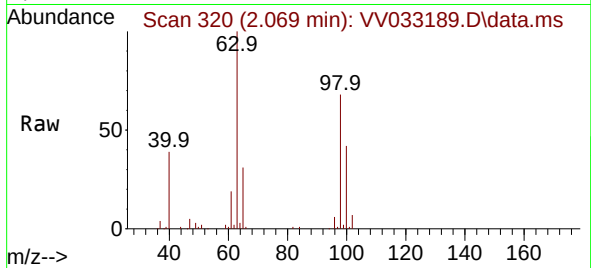

Tgt Ion: 96 Resp: 288
Ion Ratio Lower Upper
96 100
61 344.9 109.1 202.7
63 1770.0 85.3 158.1




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 12/11/2023
Supervised By :Mahesh Dadoda 12/11/2023

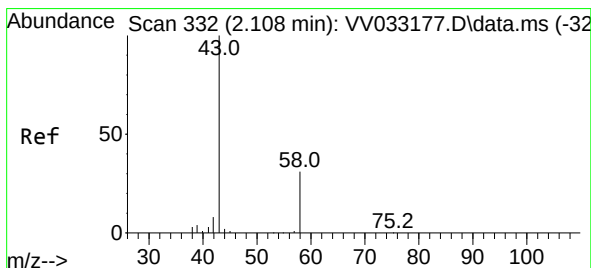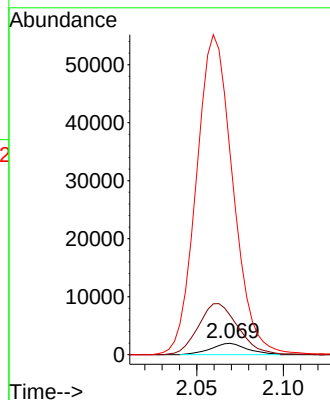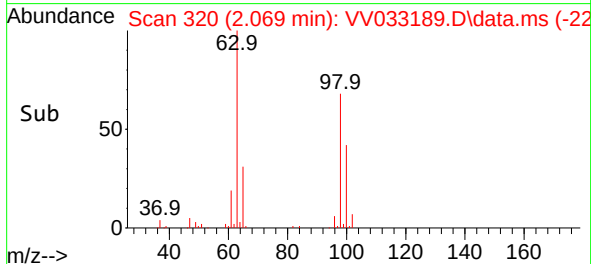

#13
Acetone
Concen: 34.110 ug/L
RT: 2.111 min Scan# 333
Delta R.T. 0.003 min
Lab File: VV033189.D
Acq: 08 Dec 2023 14:42

Tgt Ion: 43 Resp: 24460
Ion Ratio Lower Upper
43 100
58 29.8 0.0 62.8

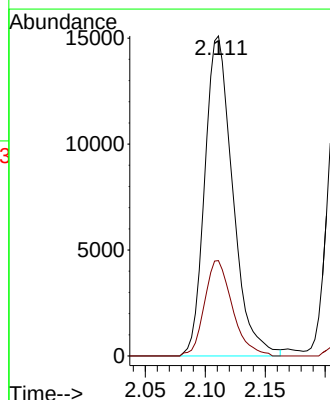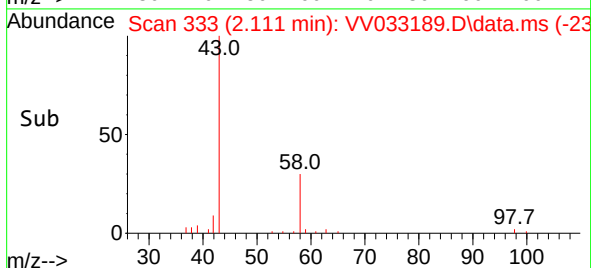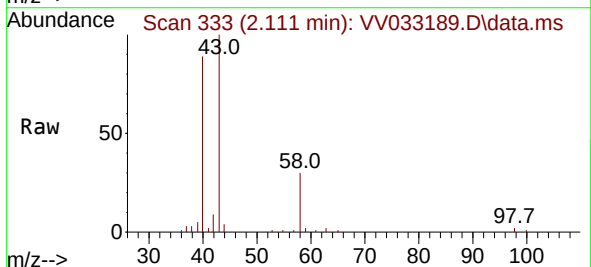

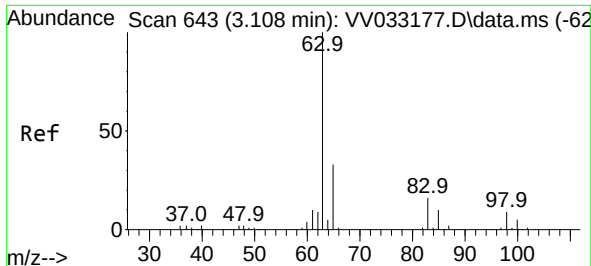





#19
1,1-Dichloroethane
Concen: 2.969 ug/L
RT: 3.111 min Scan# 64
Delta R.T. 0.003 min
Lab File: VV033189.D
Acq: 08 Dec 2023 14:42

Instrument :
MSVOA_V
ClientSampleId :
YCHA9

Tgt Ion: 63 Resp: 818
Ion Ratio Lower Upper
63 100
65 31.0 23.0 42.6
83 17.5 11.4 21.2

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 12/11/2023
Supervised By :Mahesh Dadoda 12/11/2023

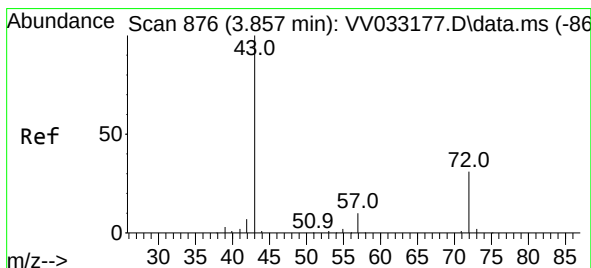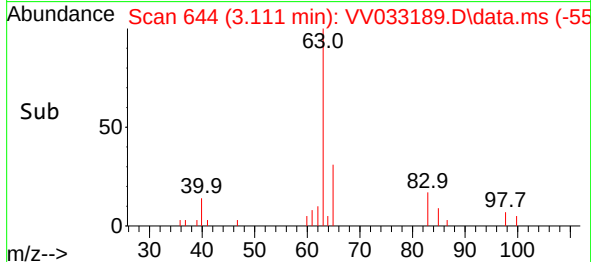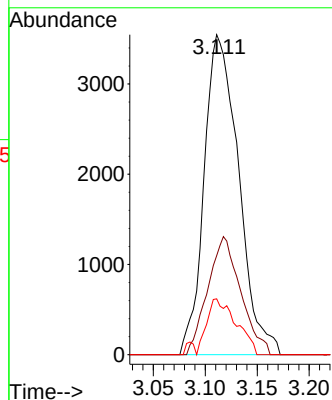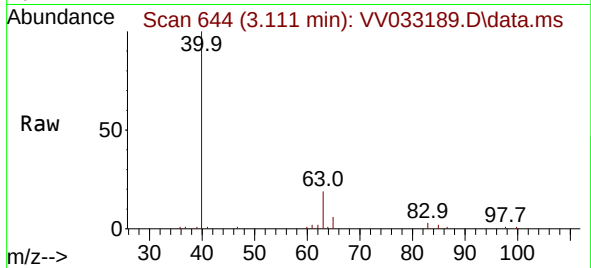

#22
2-Butanone
Concen: 18.061 ug/L m
RT: 3.883 min Scan# 884
Delta R.T. 0.026 min
Lab File: VV033189.D
Acq: 08 Dec 2023 14:42

Tgt Ion: 43 Resp: 16482
Ion Ratio Lower Upper
43 100
72 28.1 14.6 43.8

