

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033182.D
 Acq On : 08 Dec 2023 12:00
 Operator : SY/MD
 Sample : 05673-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEJ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

Signal : TIC: VV033182.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rVB	112421	117091	12.86%	1.438%
2	1.420	102	118	129	rBV2	5842	12023	1.32%	0.148%
3	1.471	132	134	137	rVV	1645	897	0.10%	0.011%
4	1.500	137	143	145	rVV2	2213	2367	0.26%	0.029%
5	1.532	145	153	171	rVV	84976	107366	11.79%	1.319%
6	1.597	171	173	178	rVB2	1626	1433	0.16%	0.018%
7	1.638	183	186	190	rVV3	1114	1007	0.11%	0.012%
8	1.796	230	235	237	rBV2	1080	813	0.09%	0.010%
9	1.809	237	239	243	rVB2	1121	782	0.09%	0.010%
10	1.863	253	256	260	rVB2	1265	956	0.10%	0.012%
11	1.999	295	298	303	rBV3	995	796	0.09%	0.010%
12	2.060	303	317	332	rBV	180937	267557	29.38%	3.286%
13	2.146	338	344	346	rBV	2282	2066	0.23%	0.025%
14	2.220	362	367	371	rBV3	2734	3411	0.37%	0.042%
15	2.388	416	419	421	rBV2	1145	850	0.09%	0.010%
16	2.452	432	439	444	rVB4	2881	3492	0.38%	0.043%
17	2.761	532	535	538	rBV2	1542	1113	0.12%	0.014%
18	3.053	622	626	630	rBV2	1732	1759	0.19%	0.022%
19	3.246	683	686	690	rBV	1276	1166	0.13%	0.014%
20	3.783	844	853	882	rBV2	55361	171358	18.81%	2.105%
21	4.108	951	954	957	rVB	1586	1090	0.12%	0.013%
22	4.249	984	998	1019	rBV	149416	379946	41.71%	4.667%
23	4.449	1057	1060	1062	rVB	1533	828	0.09%	0.010%
24	4.516	1078	1081	1086	rBV	1669	1415	0.16%	0.017%
25	4.590	1100	1104	1109	rVV3	1430	1849	0.20%	0.023%
26	4.715	1139	1143	1146	rVB	1397	977	0.11%	0.012%
27	4.751	1151	1154	1157	rBV	1391	1213	0.13%	0.015%
28	4.957	1201	1218	1251	rBV2	338983	910817	100.00%	11.188%
29	5.397	1352	1355	1360	rBV2	1546	1381	0.15%	0.017%
30	5.426	1361	1364	1367	rVB	1923	1245	0.14%	0.015%
31	5.535	1387	1398	1425	rVV	294608	612952	67.30%	7.529%
32	5.706	1449	1451	1457	rVB	2035	1296	0.14%	0.016%
33	5.831	1481	1490	1511	rVB6	19254	47343	5.20%	0.582%
34	5.989	1527	1539	1564	rVV2	189079	390253	42.85%	4.794%
35	6.095	1570	1572	1576	rBV4	1165	764	0.08%	0.009%
36	6.243	1615	1618	1620	rBV2	1309	897	0.10%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120823\
 Data File : VW033182.D
 Acq On : 08 Dec 2023 12:00
 Operator : SY/MD
 Sample : 05673-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEJ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.513	1699	1702	1705	rVB	2534	1619	0.18%	0.020%
38	6.587	1723	1725	1728	rVB	1597	872	0.10%	0.011%
39	6.609	1728	1732	1737	rBV	1205	1098	0.12%	0.013%
40	6.638	1738	1741	1744	rBV	1041	802	0.09%	0.010%
41	6.699	1758	1760	1763	rBV	1391	842	0.09%	0.010%
42	6.911	1817	1826	1846	rBV	109093	205325	22.54%	2.522%
43	7.018	1857	1859	1864	rVB	2006	1331	0.15%	0.016%
44	7.243	1918	1929	1957	rBV	420154	750459	82.39%	9.218%
45	7.551	2016	2025	2051	rBV2	83074	146168	16.05%	1.795%
46	7.905	2122	2135	2153	rBV	498709	844893	92.76%	10.378%
47	8.024	2163	2172	2198	rBV	181512	339848	37.31%	4.174%
48	8.246	2238	2241	2244	rBV	1450	1152	0.13%	0.014%
49	8.497	2317	2319	2323	rVB2	1301	849	0.09%	0.010%
50	8.526	2323	2328	2329	rBV	1471	1366	0.15%	0.017%
51	8.561	2336	2339	2344	rBV3	1489	1537	0.17%	0.019%
52	8.619	2354	2357	2360	rVB	1970	1043	0.11%	0.013%
53	8.638	2360	2363	2368	rBV	1536	1163	0.13%	0.014%
54	8.686	2375	2378	2383	rBV	1158	843	0.09%	0.010%
55	8.786	2398	2409	2432	rBV	478904	773575	84.93%	9.502%
56	9.172	2526	2529	2533	rBV	1471	1303	0.14%	0.016%
57	9.448	2612	2615	2619	rBV	1158	915	0.10%	0.011%
58	9.808	2724	2727	2730	rBV3	1299	981	0.11%	0.012%
59	10.091	2812	2815	2820	rVB	2045	1499	0.16%	0.018%
60	10.153	2823	2834	2855	rVV	262925	415701	45.64%	5.106%
61	10.400	2907	2911	2915	rBV	1816	2044	0.22%	0.025%
62	10.516	2944	2947	2950	rVB	1916	1106	0.12%	0.014%
63	10.545	2954	2956	2960	rVB	1705	1259	0.14%	0.015%
64	10.571	2960	2964	2967	rBV2	997	1021	0.11%	0.013%
65	10.622	2978	2980	2983	rBV	931	756	0.08%	0.009%
66	10.664	2989	2993	2996	rVB	1324	985	0.11%	0.012%
67	10.689	2996	3001	3004	rBV	1410	1469	0.16%	0.018%
68	10.908	3066	3069	3074	rBV	1723	1161	0.13%	0.014%
69	11.185	3145	3155	3175	rBV	509820	775954	85.19%	9.531%
70	11.471	3241	3244	3247	rBV	1435	1229	0.13%	0.015%
71	11.561	3259	3272	3290	rBV	484492	763934	83.87%	9.383%
72	11.841	3355	3359	3365	rBV	2406	3220	0.35%	0.040%
73	12.120	3443	3446	3452	rVB	1809	1712	0.19%	0.021%
74	12.365	3517	3522	3526	rBV	1370	1440	0.16%	0.018%
75	12.471	3552	3555	3559	rVB	2324	1669	0.18%	0.021%
76	12.529	3571	3573	3579	rVB	1929	1685	0.18%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033182.D
 Acq On : 08 Dec 2023 12:00
 Operator : SY/MD
 Sample : 05673-05DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEJ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.558	3579	3582	3585	rBV	1451	1162	0.13%	0.014%
78	13.059	3735	3738	3746	rBV3	1124	1508	0.17%	0.019%
79	13.101	3747	3751	3753	rBV	1159	1096	0.12%	0.013%
80	13.140	3760	3763	3765	rBV	1331	919	0.10%	0.011%
81	13.525	3880	3883	3886	rVV	1321	936	0.10%	0.011%
82	13.783	3960	3963	3965	rBV	1741	1277	0.14%	0.016%
83	13.992	4025	4028	4034	rVB	1720	1718	0.19%	0.021%
84	14.130	4067	4071	4074	rBV	1482	1240	0.14%	0.015%
85	14.246	4104	4107	4111	rBV	1152	981	0.11%	0.012%
86	14.381	4144	4149	4153	rBV3	1609	1749	0.19%	0.021%
87	14.419	4158	4161	4163	rBV2	1122	818	0.09%	0.010%
88	14.554	4198	4203	4206	rBV2	1599	1654	0.18%	0.020%
89	14.574	4206	4209	4216	rVB	1588	1759	0.19%	0.022%
90	14.766	4266	4269	4272	rBV	1119	855	0.09%	0.011%
91	14.844	4290	4293	4296	rBV3	1443	1251	0.14%	0.015%
92	15.165	4390	4393	4397	rBV	1608	1177	0.13%	0.014%
93	15.213	4403	4408	4413	rBV2	2211	2912	0.32%	0.036%
94	15.291	4430	4432	4435	rBV2	1202	859	0.09%	0.011%
95	15.612	4530	4532	4535	rVB3	1600	858	0.09%	0.011%
96	15.680	4550	4553	4556	rBV2	1919	1480	0.16%	0.018%
97	15.818	4594	4596	4601	rBV	1659	1356	0.15%	0.017%
98	15.995	4647	4651	4656	rBV3	2146	2160	0.24%	0.027%
99	16.217	4718	4720	4723	rBV2	1517	921	0.10%	0.011%
100	16.291	4741	4743	4750	rVB2	2323	2224	0.24%	0.027%




Sum of corrected areas: 8141267

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033182.D
Acq On : 08 Dec 2023 12:00
Operator : SY/MD
Sample : 05673-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEJ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

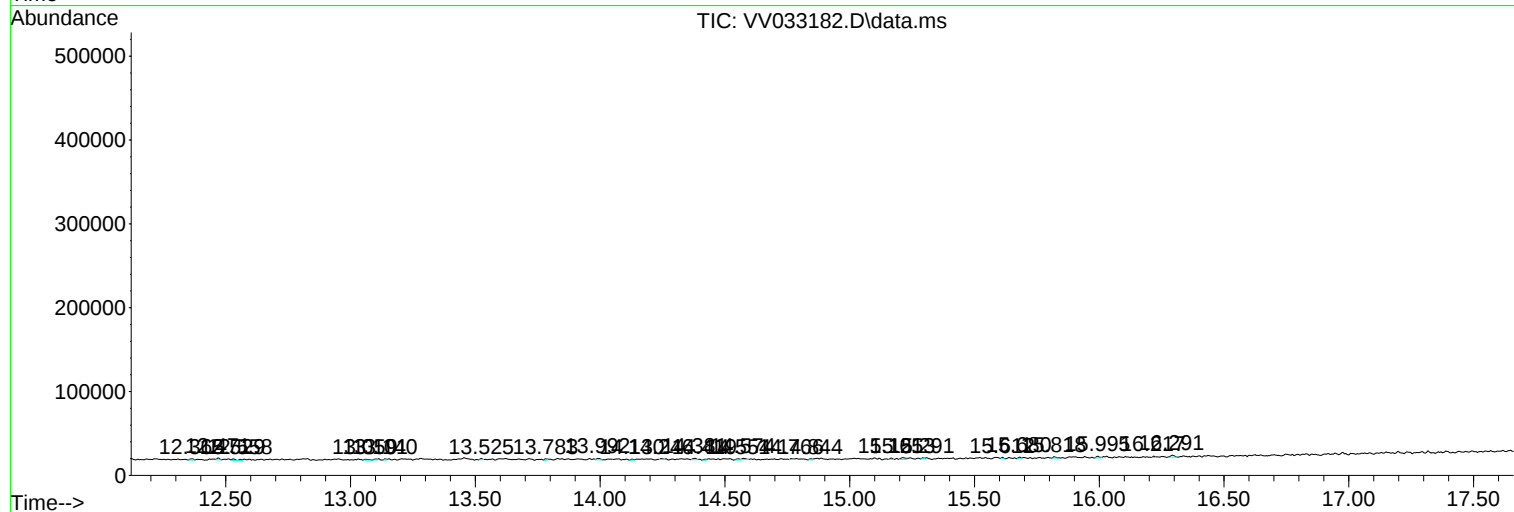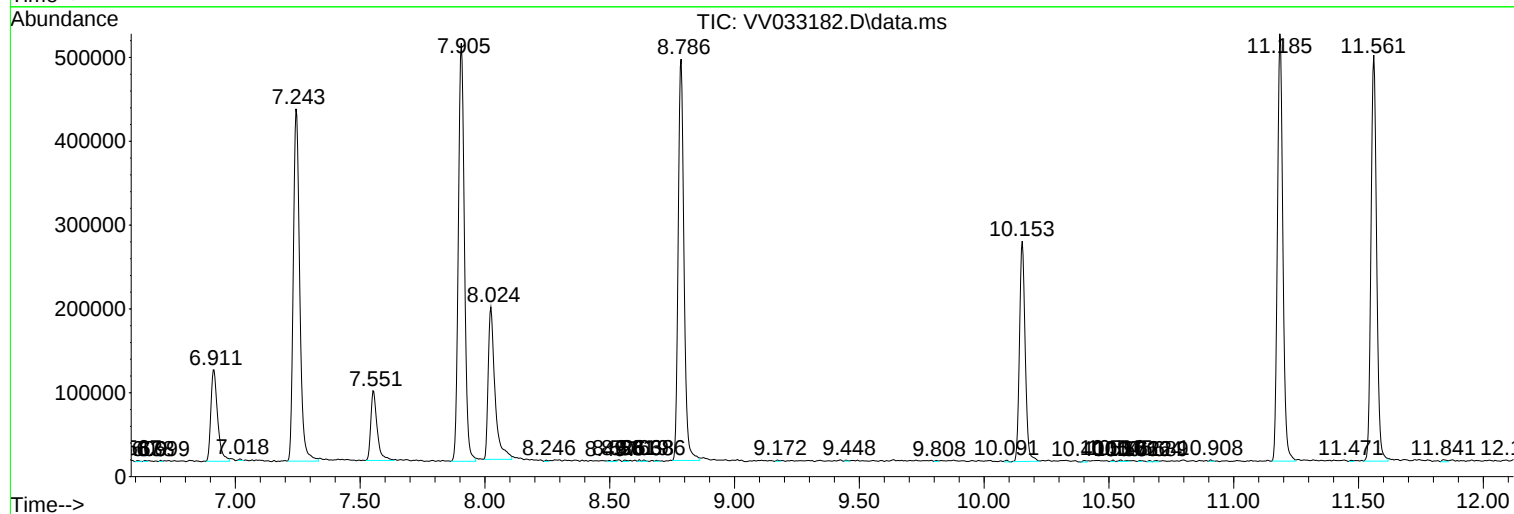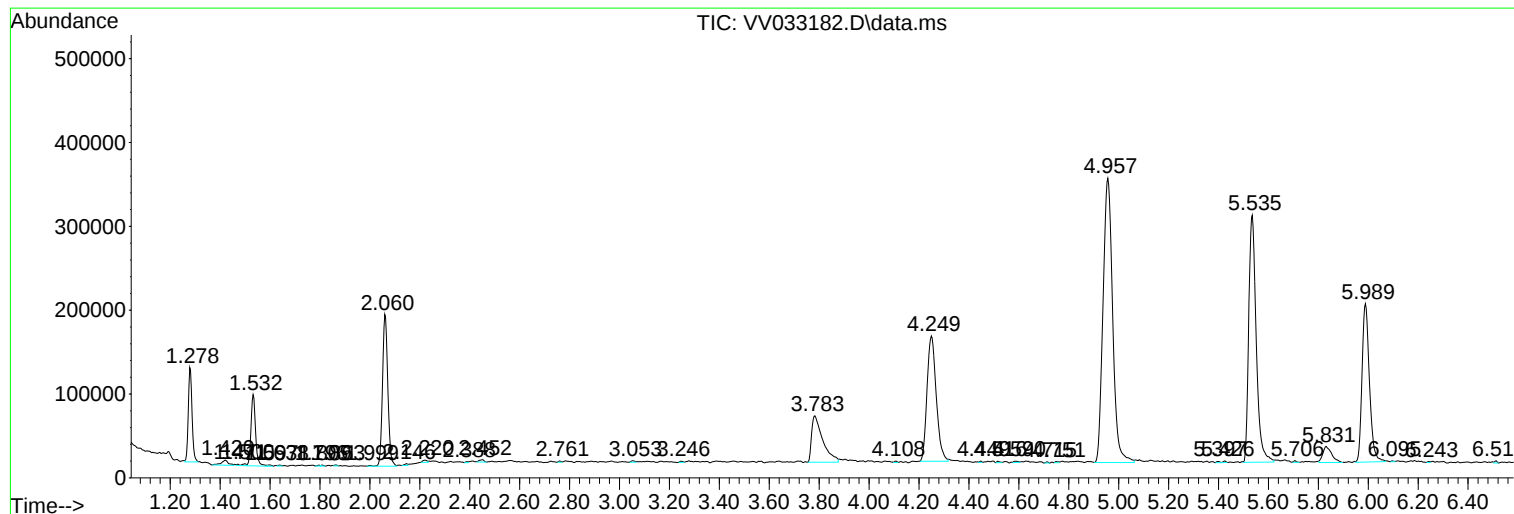

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033182.D
Acq On : 08 Dec 2023 12:00
Operator : SY/MD
Sample : 05673-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEJ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033182.D
Acq On : 08 Dec 2023 12:00
Operator : SY/MD
Sample : 05673-05DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEJ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------