

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033183.D
 Acq On : 08 Dec 2023 12:23
 Operator : SY/MD
 Sample : 05673-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033183.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	89	rVB	117959	127025	0.71%	0.474%
2	1.388	105	108	111	rVB	1045	722	0.00%	0.003%
3	1.413	111	116	122	rBV3	4525	4906	0.03%	0.018%
4	1.468	131	133	139	rVB	1349	1077	0.01%	0.004%
5	1.497	139	142	144	rVV3	1010	793	0.00%	0.003%
6	1.532	146	153	166	rVB	88014	104983	0.58%	0.392%
7	1.625	178	182	187	rVB	1216	921	0.01%	0.003%
8	1.690	197	202	204	rBV3	779	681	0.00%	0.003%
9	1.744	216	219	225	rVV2	1093	886	0.00%	0.003%
10	1.789	231	233	237	rVB	1969	1377	0.01%	0.005%
11	1.828	237	245	247	rBV2	1883	2421	0.01%	0.009%
12	1.844	247	250	254	rVV2	1779	1379	0.01%	0.005%
13	1.876	257	260	263	rVV	1155	951	0.01%	0.004%
14	1.892	263	265	268	rVV2	1222	754	0.00%	0.003%
15	1.912	268	271	275	rVV2	919	676	0.00%	0.003%
16	1.941	278	280	283	rVB2	1476	875	0.00%	0.003%
17	1.973	283	290	294	rBV3	1760	2382	0.01%	0.009%
18	2.063	307	318	336	rBV	188588	276565	1.54%	1.032%
19	2.159	340	348	349	rBV	2250	2010	0.01%	0.007%
20	2.227	362	369	373	rBV6	2625	3773	0.02%	0.014%
21	2.503	452	455	461	rVB	1964	2389	0.01%	0.009%
22	2.593	481	483	486	rVB	1600	835	0.00%	0.003%
23	2.651	498	501	503	rBV	1253	864	0.00%	0.003%
24	2.841	557	560	563	rBV2	1568	1279	0.01%	0.005%
25	2.860	563	566	568	rBV	1293	757	0.00%	0.003%
26	3.034	617	620	623	rBV	1619	983	0.01%	0.004%
27	3.133	648	651	654	rBV	1288	1132	0.01%	0.004%
28	3.204	671	673	678	rVB3	1703	1111	0.01%	0.004%
29	3.304	702	704	707	rBV2	1168	696	0.00%	0.003%
30	3.442	744	747	749	rBV	1564	916	0.01%	0.003%
31	3.519	769	771	774	rBV	1272	737	0.00%	0.003%
32	3.622	800	803	805	rBV	1300	725	0.00%	0.003%
33	3.812	844	862	897	rBV2	454424	1212914	6.74%	4.525%
34	4.249	983	998	1024	rBV2	157760	409008	2.27%	1.526%
35	4.812	1171	1173	1176	rVB	1699	1003	0.01%	0.004%
36	4.834	1177	1180	1183	rBV	1705	1290	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120823\
 Data File : VW033183.D
 Acq On : 08 Dec 2023 12:23
 Operator : SY/MD
 Sample : 05673-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.957	1203	1218	1245	rBV2	352099	935016	5.20%	3.488%
38	5.149	1275	1278	1283	rBV	1476	1171	0.01%	0.004%
39	5.297	1321	1324	1326	rBV	1510	1054	0.01%	0.004%
40	5.535	1387	1398	1418	rBV	301387	616149	3.42%	2.299%
41	5.651	1432	1434	1442	rVB2	2090	2006	0.01%	0.007%
42	5.770	1467	1471	1474	rVB2	1664	1253	0.01%	0.005%
43	5.789	1474	1477	1479	rBV	1607	959	0.01%	0.004%
44	5.834	1479	1491	1517	rVV2	138041	287248	1.60%	1.072%
45	5.931	1519	1521	1523	rBV2	1331	757	0.00%	0.003%
46	5.989	1527	1539	1560	rBV2	193560	394920	2.19%	1.473%
47	6.172	1593	1596	1601	rBV	1449	1406	0.01%	0.005%
48	6.304	1634	1637	1640	rBV2	1266	1080	0.01%	0.004%
49	6.744	1771	1774	1778	rVB	1547	948	0.01%	0.004%
50	6.770	1778	1782	1784	rBV	1406	1113	0.01%	0.004%
51	6.815	1791	1796	1799	rBV	1393	1219	0.01%	0.005%
52	6.911	1816	1826	1844	rBV	113245	208955	1.16%	0.780%
53	7.063	1870	1873	1879	rBV3	1803	1337	0.01%	0.005%
54	7.243	1919	1929	1954	rBV	440478	770074	4.28%	2.873%
55	7.555	2016	2026	2043	rBV	86267	153973	0.86%	0.574%
56	7.770	2090	2093	2096	rBV	1105	986	0.01%	0.004%
57	7.908	2115	2136	2163	rBV	10905051	17997220	100.00%	67.138%
58	8.024	2164	2172	2200	rVB	194057	388555	2.16%	1.450%
59	8.239	2236	2239	2243	rBV	2068	1571	0.01%	0.006%
60	8.786	2398	2409	2436	rBV	470869	781797	4.34%	2.916%
61	8.979	2466	2469	2471	rBV	1141	737	0.00%	0.003%
62	9.001	2473	2476	2478	rBV2	1316	808	0.00%	0.003%
63	9.194	2533	2536	2539	rBV	1924	1165	0.01%	0.004%
64	9.468	2618	2621	2622	rBV	1376	812	0.00%	0.003%
65	10.005	2784	2788	2789	rBV	1115	884	0.00%	0.003%
66	10.104	2815	2819	2823	rBV	1618	1790	0.01%	0.007%
67	10.152	2824	2834	2850	rVV	270240	424958	2.36%	1.585%
68	10.230	2855	2858	2862	rVB	1473	1009	0.01%	0.004%
69	10.326	2879	2888	2898	rVB5	6341	11237	0.06%	0.042%
70	10.921	3069	3073	3080	rVB	1322	1843	0.01%	0.007%
71	10.998	3095	3097	3101	rVB	1335	770	0.00%	0.003%
72	11.059	3113	3116	3119	rBV	2081	1535	0.01%	0.006%
73	11.130	3135	3138	3145	rVB3	2197	2070	0.01%	0.008%
74	11.185	3145	3155	3176	rBV	519741	807521	4.49%	3.012%
75	11.561	3261	3272	3289	rBV	523374	796763	4.43%	2.972%
76	11.689	3309	3312	3315	rBV	1410	771	0.00%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033183.D
 Acq On : 08 Dec 2023 12:23
 Operator : SY/MD
 Sample : 05673-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.969	3397	3399	3405	rVB	1270	1088	0.01%	0.004%
78	11.998	3405	3408	3411	rBV	1960	1378	0.01%	0.005%
79	12.191	3463	3468	3469	rBV	2075	1616	0.01%	0.006%
80	12.548	3575	3579	3582	rVB	1888	1343	0.01%	0.005%
81	12.567	3582	3585	3587	rBV	1270	787	0.00%	0.003%
82	12.586	3588	3591	3595	rVB3	1638	1289	0.01%	0.005%
83	12.609	3595	3598	3602	rBV3	1370	1452	0.01%	0.005%
84	12.664	3612	3615	3617	rBV	1223	789	0.00%	0.003%
85	12.824	3662	3665	3667	rBV	1410	1026	0.01%	0.004%
86	12.892	3684	3686	3689	rBV	1097	756	0.00%	0.003%
87	12.930	3694	3698	3702	rVB	1530	1559	0.01%	0.006%
88	12.956	3703	3706	3710	rBV	1305	1090	0.01%	0.004%
89	13.255	3796	3799	3801	rBV2	1366	1085	0.01%	0.004%
90	13.291	3806	3810	3812	rBV2	1310	1167	0.01%	0.004%
91	13.696	3934	3936	3939	rBV	1296	869	0.00%	0.003%
92	13.985	4023	4026	4033	rVB3	2018	2320	0.01%	0.009%
93	14.123	4066	4069	4073	rBV	1243	1178	0.01%	0.004%
94	14.220	4097	4099	4102	rBV3	1101	809	0.00%	0.003%
95	14.355	4138	4141	4143	rBV	1417	993	0.01%	0.004%
96	14.455	4169	4172	4174	rBV	1678	1019	0.01%	0.004%
97	14.529	4192	4195	4197	rBV	1295	958	0.01%	0.004%
98	15.065	4359	4362	4365	rBV	1364	825	0.00%	0.003%
99	15.384	4457	4461	4467	rBV	1978	2277	0.01%	0.008%
100	15.413	4467	4470	4473	rBV2	1740	1223	0.01%	0.005%


Sum of corrected areas: 26806132

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033183.D
Acq On : 08 Dec 2023 12:23
Operator : SY/MD
Sample : 05673-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

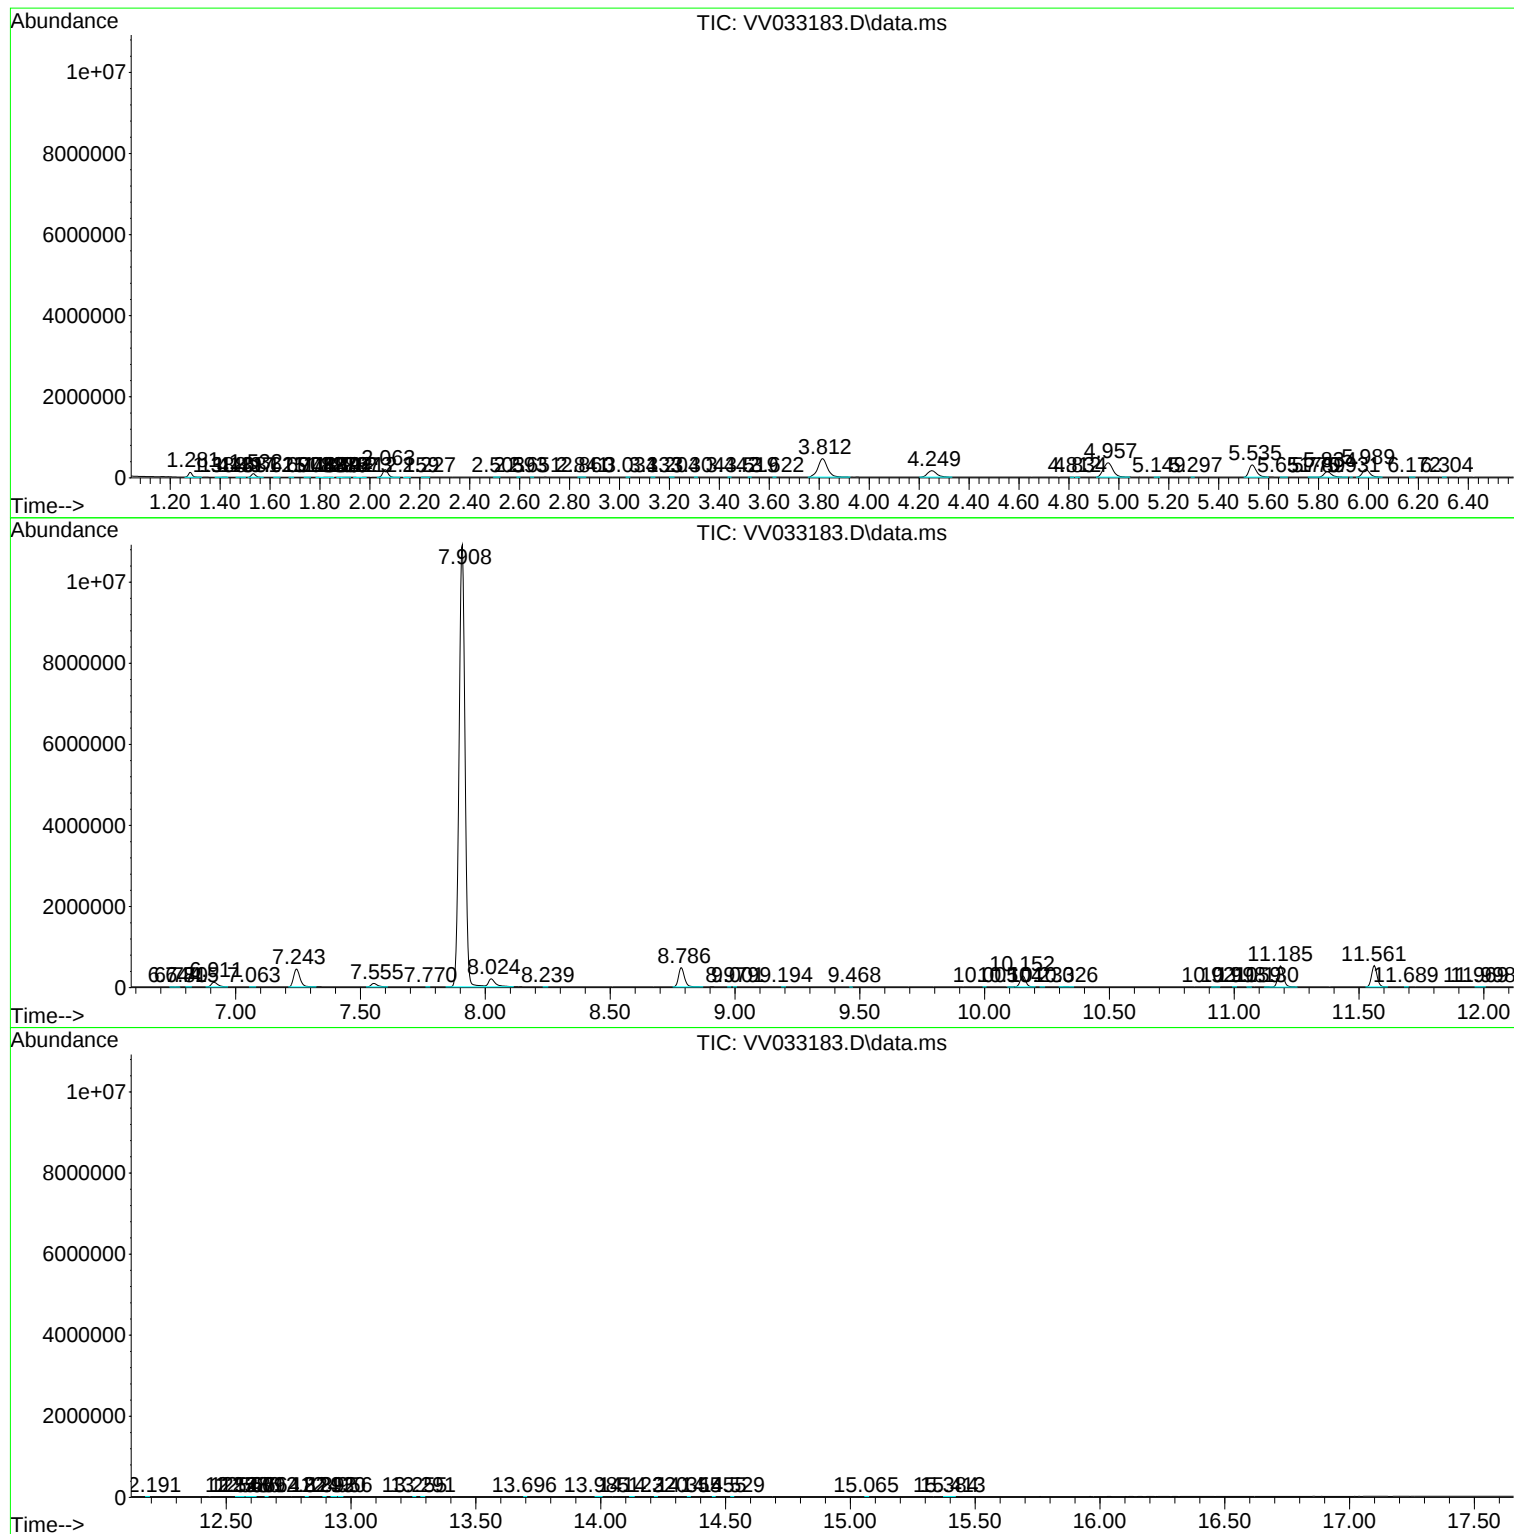

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033183.D
Acq On : 08 Dec 2023 12:23
Operator : SY/MD
Sample : 05673-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033183.D
Acq On : 08 Dec 2023 12:23
Operator : SY/MD
Sample : 05673-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc