

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033185.D
 Acq On : 08 Dec 2023 13:09
 Operator : SY/MD
 Sample : 05685-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHK1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033185.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	88	rVB	101678	108390	11.88%	1.482%
2	1.426	111	120	127	rVB3	6868	10804	1.18%	0.148%
3	1.532	146	153	163	rBV	79118	94304	10.34%	1.289%
4	1.571	163	165	173	rVB3	1653	1617	0.18%	0.022%
5	1.609	173	177	182	rVB3	951	1059	0.12%	0.014%
6	1.664	190	194	200	rBV2	712	798	0.09%	0.011%
7	1.696	200	204	209	rBV	925	875	0.10%	0.012%
8	1.786	225	232	234	rBV3	982	887	0.10%	0.012%
9	1.841	244	249	254	rBV2	691	791	0.09%	0.011%
10	1.870	254	258	262	rVB2	1714	1254	0.14%	0.017%
11	1.960	284	286	294	rVB2	799	898	0.10%	0.012%
12	2.063	308	318	331	rBV	163153	237781	26.06%	3.250%
13	2.159	343	348	351	rBV	2119	2316	0.25%	0.032%
14	2.195	351	359	361	rBV3	2098	2925	0.32%	0.040%
15	2.481	445	448	452	rVB	1412	885	0.10%	0.012%
16	2.529	460	463	467	rVB	1675	1288	0.14%	0.018%
17	2.561	469	473	475	rBV2	1260	1123	0.12%	0.015%
18	2.860	563	566	569	rBV	2031	1737	0.19%	0.024%
19	2.892	573	576	580	rVB	1467	1134	0.12%	0.016%
20	3.021	613	616	619	rBV	1257	1102	0.12%	0.015%
21	3.313	704	707	713	rVB	1998	1964	0.22%	0.027%
22	3.600	793	796	800	rBV	1456	1325	0.15%	0.018%
23	3.693	823	825	829	rBV	1238	924	0.10%	0.013%
24	3.783	845	853	874	rBV2	56425	144010	15.78%	1.969%
25	4.194	978	981	983	rBV2	1151	959	0.11%	0.013%
26	4.249	984	998	1030	rVB2	148383	392764	43.05%	5.369%
27	4.452	1057	1061	1065	rBV2	1360	1335	0.15%	0.018%
28	4.690	1131	1135	1139	rBV	1978	2083	0.23%	0.028%
29	4.957	1202	1218	1243	rBV2	341486	912382	100.00%	12.472%
30	5.284	1317	1320	1324	rVB2	1127	884	0.10%	0.012%
31	5.336	1333	1336	1341	rBV	1089	996	0.11%	0.014%
32	5.410	1357	1359	1363	rVB3	1594	1189	0.13%	0.016%
33	5.474	1376	1379	1384	rVB	1665	1419	0.16%	0.019%
34	5.535	1387	1398	1420	rBV	294677	599950	65.76%	8.201%
35	5.834	1479	1491	1501	rBV5	16873	37606	4.12%	0.514%
36	5.989	1527	1539	1557	rBV	193512	387892	42.51%	5.302%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033185.D
 Acq On : 08 Dec 2023 13:09
 Operator : SY/MD
 Sample : 05685-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHK1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.156	1588	1591	1595	rBV	1447	1005	0.11%	0.014%
38	6.256	1620	1622	1627	rBV	985	779	0.09%	0.011%
39	6.709	1758	1763	1764	rBV	1406	1248	0.14%	0.017%
40	6.850	1804	1807	1810	rBV	1270	842	0.09%	0.012%
41	6.870	1810	1813	1817	rBV	1109	1114	0.12%	0.015%
42	6.915	1817	1827	1851	rVV	114025	214671	23.53%	2.934%
43	7.172	1904	1907	1911	rVB	1424	846	0.09%	0.012%
44	7.243	1919	1929	1952	rBV	414588	725495	79.52%	9.917%
45	7.516	2011	2014	2016	rBV2	1017	775	0.08%	0.011%
46	7.554	2016	2026	2043	rVV	84594	146974	16.11%	2.009%
47	7.773	2092	2094	2099	rVB2	1473	1031	0.11%	0.014%
48	7.911	2128	2137	2151	rVB5	12480	23744	2.60%	0.325%
49	8.024	2163	2172	2206	rBV	190976	382573	41.93%	5.230%
50	8.532	2327	2330	2335	rVB	1546	1245	0.14%	0.017%
51	8.786	2397	2409	2434	rBV	475960	786905	86.25%	10.756%
52	8.956	2459	2462	2465	rBV	2173	1109	0.12%	0.015%
53	9.297	2566	2568	2573	rVB2	1139	866	0.09%	0.012%
54	9.448	2610	2615	2619	rBV	1740	1973	0.22%	0.027%
55	9.564	2648	2651	2653	rBV	1130	803	0.09%	0.011%
56	9.934	2763	2766	2773	rVB	1895	1503	0.16%	0.021%
57	9.972	2774	2778	2780	rBV2	1625	1368	0.15%	0.019%
58	10.152	2823	2834	2864	rBV	269776	435506	47.73%	5.953%
59	10.365	2897	2900	2906	rVB	2048	1730	0.19%	0.024%
60	10.390	2906	2908	2911	rVB	1788	897	0.10%	0.012%
61	10.445	2922	2925	2928	rBV	1395	852	0.09%	0.012%
62	10.860	3049	3054	3060	rBV2	1777	2833	0.31%	0.039%
63	10.911	3068	3070	3077	rVB	2038	2291	0.25%	0.031%
64	11.123	3132	3136	3141	rBV2	1914	2001	0.22%	0.027%
65	11.185	3145	3155	3173	rVV	502909	785365	86.08%	10.735%
66	11.390	3216	3219	3220	rBV2	1368	813	0.09%	0.011%
67	11.429	3229	3231	3238	rBV	1302	1607	0.18%	0.022%
68	11.484	3242	3248	3254	rBV	2536	3015	0.33%	0.041%
69	11.516	3254	3258	3260	rBV2	1309	1101	0.12%	0.015%
70	11.561	3261	3272	3291	rBV	499148	775357	84.98%	10.599%
71	11.747	3327	3330	3334	rVB	1791	1092	0.12%	0.015%
72	11.976	3397	3401	3404	rBV	1583	1185	0.13%	0.016%
73	12.117	3442	3445	3449	rVB	1659	1126	0.12%	0.015%
74	12.239	3480	3483	3487	rBV	1207	1052	0.12%	0.014%
75	12.747	3637	3641	3648	rBV2	1595	2368	0.26%	0.032%
76	12.799	3655	3657	3661	rBV2	1021	1007	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120823\
 Data File : VW033185.D
 Acq On : 08 Dec 2023 13:09
 Operator : SY/MD
 Sample : 05685-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCHK1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.873	3677	3680	3684	rVB2	1866	1409	0.15%	0.019%
78	13.001	3718	3720	3723	rVB	1596	782	0.09%	0.011%
79	13.194	3775	3780	3782	rBV2	1587	1659	0.18%	0.023%
80	13.210	3782	3785	3793	rVV2	2526	2946	0.32%	0.040%
81	13.258	3796	3800	3807	rVB	2219	2398	0.26%	0.033%
82	13.422	3848	3851	3856	rVB	2156	2197	0.24%	0.030%
83	13.455	3856	3861	3863	rBV3	2340	2142	0.23%	0.029%
84	13.593	3901	3904	3909	rBV3	1497	1506	0.17%	0.021%
85	13.693	3933	3935	3938	rVB2	1804	1061	0.12%	0.015%
86	13.879	3990	3993	3996	rBV	1316	835	0.09%	0.011%
87	14.101	4060	4062	4066	rVB	1797	1017	0.11%	0.014%
88	14.165	4080	4082	4089	rVB2	1694	2035	0.22%	0.028%
89	14.204	4091	4094	4099	rBV	1154	1280	0.14%	0.017%
90	14.410	4155	4158	4162	rBV	1219	1013	0.11%	0.014%
91	14.480	4177	4180	4186	rVB	2321	2227	0.24%	0.030%
92	14.641	4227	4230	4235	rBV2	1329	1113	0.12%	0.015%
93	14.911	4311	4314	4315	rBV	1730	1105	0.12%	0.015%
94	15.059	4358	4360	4367	rVB3	1382	1539	0.17%	0.021%
95	15.101	4370	4373	4380	rBV2	1433	1374	0.15%	0.019%
96	15.512	4496	4501	4506	rBV3	1611	1995	0.22%	0.027%
97	15.708	4560	4562	4565	rBV3	1242	839	0.09%	0.011%
98	15.763	4576	4579	4583	rBV	1865	1201	0.13%	0.016%
99	15.914	4623	4626	4629	rVB	1834	1240	0.14%	0.017%
100	16.191	4707	4712	4714	rBV	3177	3023	0.33%	0.041%


Sum of corrected areas: 7315653

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033185.D
Acq On : 08 Dec 2023 13:09
Operator : SY/MD
Sample : 05685-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

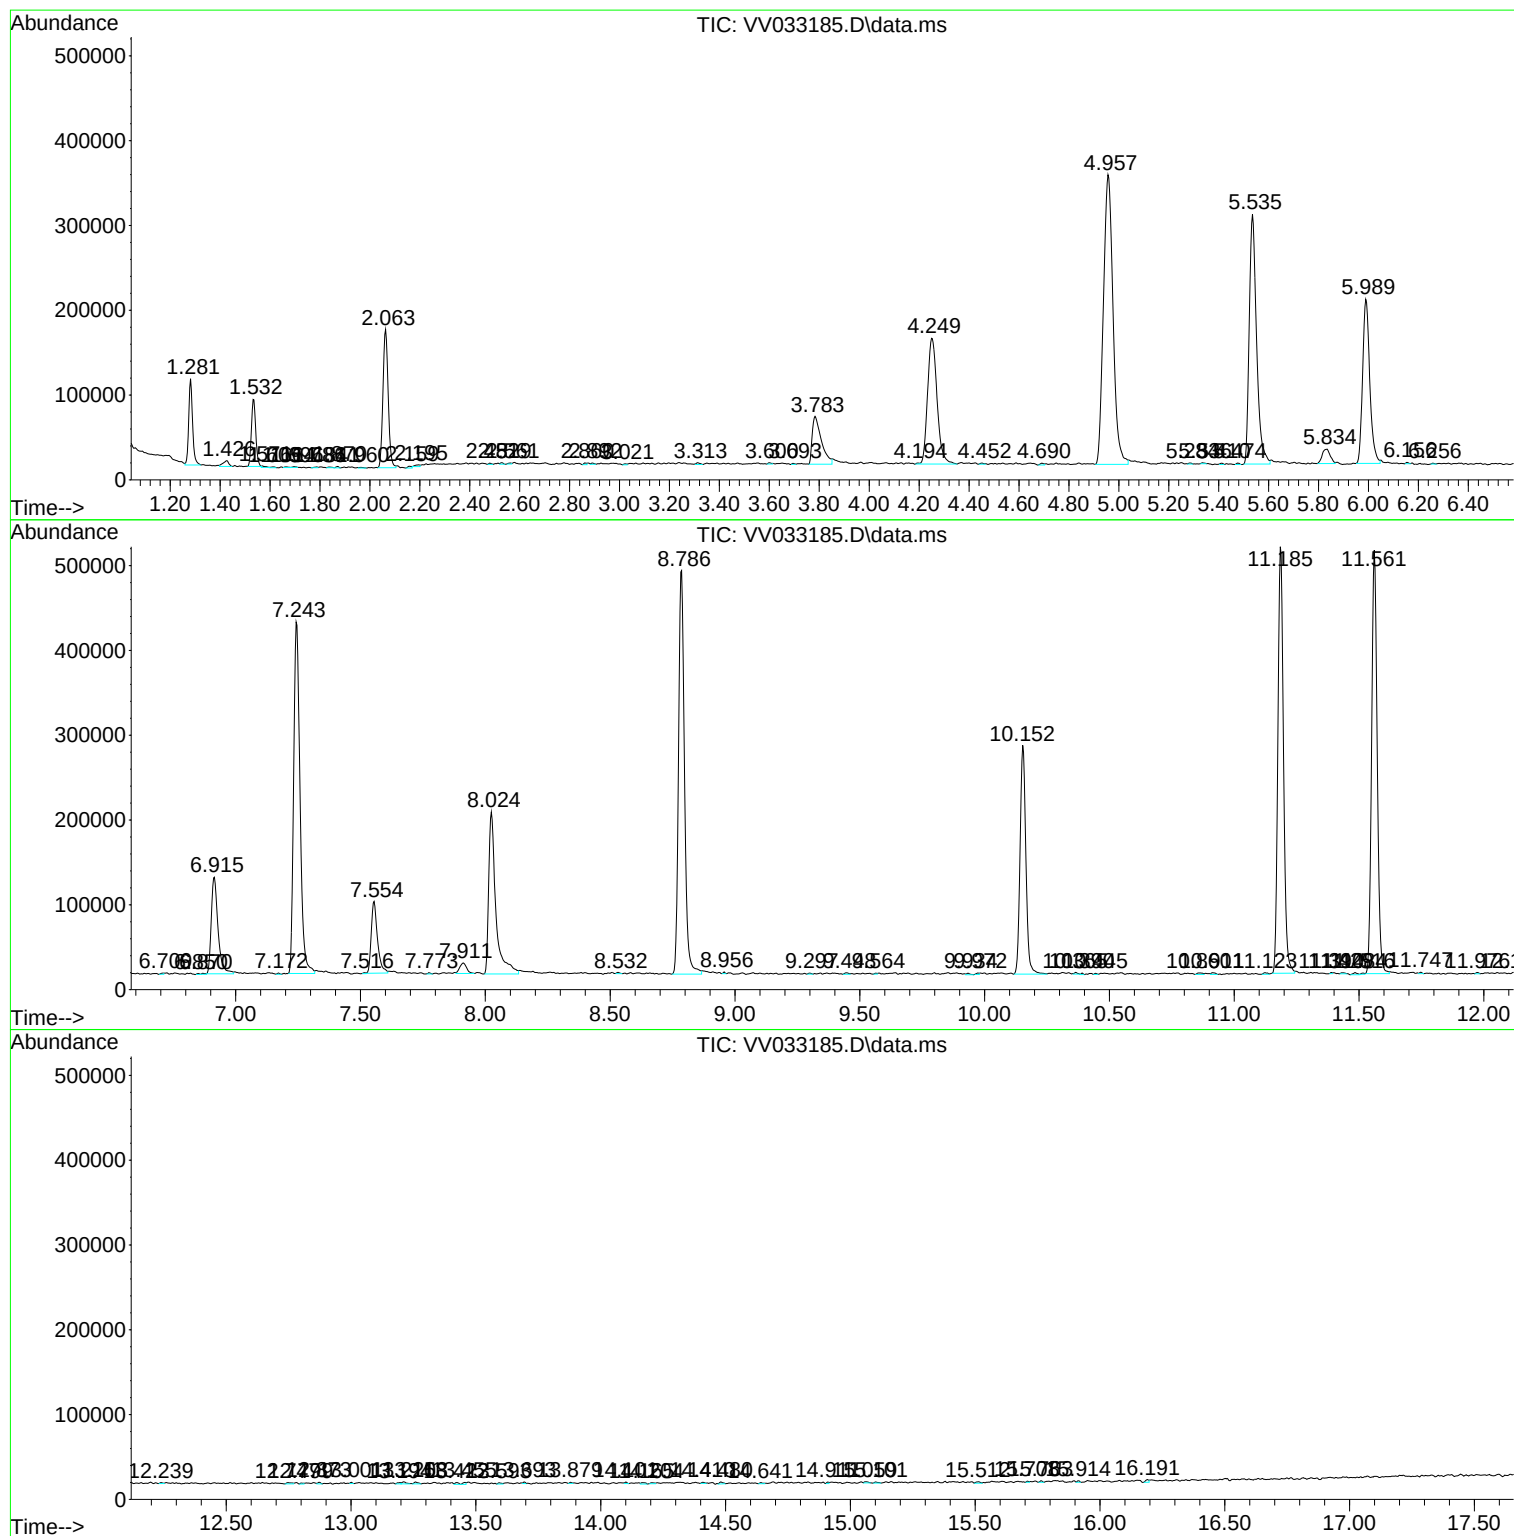

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033185.D
Acq On : 08 Dec 2023 13:09
Operator : SY/MD
Sample : 05685-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033185.D
Acq On : 08 Dec 2023 13:09
Operator : SY/MD
Sample : 05685-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCHK1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------