

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033186.D
 Acq On : 08 Dec 2023 13:32
 Operator : SY/MD
 Sample : 05685-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCH80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033186.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	116326	123241	13.80%	1.734%
2	1.381	104	106	109	rBV2	699	369	0.04%	0.005%
3	1.423	109	119	123	rBV3	4755	6974	0.78%	0.098%
4	1.487	136	139	141	rBV2	991	684	0.08%	0.010%
5	1.503	141	144	145	rVV	1138	737	0.08%	0.010%
6	1.532	145	153	164	rVV	86307	100782	11.29%	1.418%
7	1.574	164	166	172	rVB2	1525	1439	0.16%	0.020%
8	1.613	175	178	181	rBV2	1016	791	0.09%	0.011%
9	1.651	187	190	193	rBV	877	599	0.07%	0.008%
10	1.709	203	208	211	rBV2	1742	1691	0.19%	0.024%
11	1.751	218	221	223	rBV	1216	638	0.07%	0.009%
12	1.764	223	225	228	rVB3	522	244	0.03%	0.003%
13	1.783	228	231	233	rVB2	1309	741	0.08%	0.010%
14	1.809	233	239	244	rBV2	1815	2151	0.24%	0.030%
15	1.838	244	248	249	rBV2	919	628	0.07%	0.009%
16	1.870	256	258	260	rBV2	482	309	0.03%	0.004%
17	1.899	264	267	271	rVB	1065	883	0.10%	0.012%
18	1.924	271	275	278	rBV2	863	584	0.07%	0.008%
19	1.953	281	284	290	rVB2	1654	1695	0.19%	0.024%
20	1.989	290	295	297	rBV2	1385	1254	0.14%	0.018%
21	2.008	297	301	305	rBV2	600	375	0.04%	0.005%
22	2.060	306	317	334	rBV	178382	263000	29.45%	3.700%
23	2.166	342	350	354	rBV	3358	4893	0.55%	0.069%
24	2.188	354	357	359	rVV2	1255	897	0.10%	0.013%
25	2.240	367	373	375	rBV3	1739	1963	0.22%	0.028%
26	2.278	381	385	388	rBV	1615	1479	0.17%	0.021%
27	2.323	397	399	402	rBV	916	714	0.08%	0.010%
28	2.500	452	454	456	rBV	1224	784	0.09%	0.011%
29	3.111	638	644	646	rBV	1886	2227	0.25%	0.031%
30	3.166	657	661	664	rBV	1601	1760	0.20%	0.025%
31	3.272	692	694	696	rBV2	1432	895	0.10%	0.013%
32	3.783	844	853	876	rBV2	48652	126185	14.13%	1.775%
33	4.191	977	980	983	rBV3	1442	1277	0.14%	0.018%
34	4.249	983	998	1028	rVB	150251	388183	43.47%	5.461%
35	4.767	1156	1159	1160	rBV2	1091	689	0.08%	0.010%
36	4.867	1187	1190	1193	rBV	1515	1017	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120823\
 Data File : VW033186.D
 Acq On : 08 Dec 2023 13:32
 Operator : SY/MD
 Sample : 05685-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 YCH80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.957	1202	1218	1254	rBV2	333961	892955	100.00%	12.563%
38	5.079	1254	1256	1261	rVB2	1493	1302	0.15%	0.018%
39	5.211	1295	1297	1300	rBV	1254	784	0.09%	0.011%
40	5.330	1331	1334	1336	rBV	1632	1070	0.12%	0.015%
41	5.535	1387	1398	1420	rBV	286367	590918	66.18%	8.313%
42	5.793	1476	1478	1480	rBV	1613	979	0.11%	0.014%
43	5.825	1482	1488	1489	rBV4	8334	7275	0.81%	0.102%
44	5.989	1527	1539	1559	rBV2	189361	385486	43.17%	5.423%
45	6.403	1665	1668	1670	rBV	1519	944	0.11%	0.013%
46	6.455	1681	1684	1689	rBV	1729	1754	0.20%	0.025%
47	6.555	1712	1715	1716	rBV	1097	674	0.08%	0.009%
48	6.911	1817	1826	1844	rBV	109613	201003	22.51%	2.828%
49	7.143	1896	1898	1903	rVB2	1404	837	0.09%	0.012%
50	7.243	1918	1929	1950	rBV	421660	743738	83.29%	10.463%
51	7.554	2017	2026	2049	rBV	79299	143393	16.06%	2.017%
52	7.879	2121	2127	2130	rBV5	2652	3535	0.40%	0.050%
53	7.908	2133	2136	2148	rVB4	6608	8600	0.96%	0.121%
54	8.024	2163	2172	2205	rBV	172906	330291	36.99%	4.647%
55	8.288	2252	2254	2258	rVB	1507	861	0.10%	0.012%
56	8.345	2267	2272	2280	rBV	2213	3120	0.35%	0.044%
57	8.397	2285	2288	2293	rBV	1797	1832	0.21%	0.026%
58	8.481	2312	2314	2316	rBV	992	543	0.06%	0.008%
59	8.587	2344	2347	2351	rVB	1424	939	0.11%	0.013%
60	8.786	2398	2409	2431	rBV	465280	755235	84.58%	10.625%
61	9.101	2505	2507	2509	rBV	979	472	0.05%	0.007%
62	9.130	2514	2516	2519	rVV	1160	685	0.08%	0.010%
63	9.181	2530	2532	2539	rVB	1536	1203	0.13%	0.017%
64	9.847	2736	2739	2745	rBV	1599	1626	0.18%	0.023%
65	9.892	2751	2753	2756	rVB	1357	625	0.07%	0.009%
66	9.940	2765	2768	2771	rBV	1970	1476	0.17%	0.021%
67	10.101	2815	2818	2821	rBV	1544	903	0.10%	0.013%
68	10.152	2824	2834	2856	rVB	265181	415675	46.55%	5.848%
69	10.329	2882	2889	2894	rBV5	2998	4557	0.51%	0.064%
70	10.535	2951	2953	2958	rBB	957	615	0.07%	0.009%
71	10.628	2979	2982	2987	rBV	1438	1311	0.15%	0.018%
72	10.689	2998	3001	3009	rVB2	1693	1660	0.19%	0.023%
73	10.998	3095	3097	3100	rBV2	972	609	0.07%	0.009%
74	11.185	3144	3155	3178	rBV	492318	771708	86.42%	10.857%
75	11.561	3261	3272	3292	rBV	487786	767438	85.94%	10.797%
76	11.950	3390	3393	3395	rBV	1398	944	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033186.D
Acq On : 08 Dec 2023 13:32
Operator : SY/MD
Sample : 05685-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCH80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Title : VOC Analysis

77	12.075	3428	3432	3438	rBV	1668	1930	0.22%	0.027%
78	12.371	3521	3524	3527	rBV	1730	1303	0.15%	0.018%
79	12.580	3587	3589	3592	rVB	1139	593	0.07%	0.008%
80	13.210	3782	3785	3788	rBV2	1564	885	0.10%	0.012%
81	13.249	3793	3797	3798	rBV	1891	1240	0.14%	0.017%
82	13.651	3919	3922	3924	rBV	1496	1007	0.11%	0.014%
83	14.538	4194	4198	4202	rBV	1800	1841	0.21%	0.026%
84	14.911	4311	4314	4317	rBV	1569	1054	0.12%	0.015%
85	15.310	4435	4438	4441	rVB2	1460	972	0.11%	0.014%
86	15.561	4513	4516	4517	rBV	1866	987	0.11%	0.014%
87	15.599	4524	4528	4530	rBV2	2052	1760	0.20%	0.025%
88	15.824	4596	4598	4600	rBV3	1478	688	0.08%	0.010%
89	16.628	4846	4848	4850	rBV2	2245	1347	0.15%	0.019%




Sum of corrected areas: 7107954

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033186.D
Acq On : 08 Dec 2023 13:32
Operator : SY/MD
Sample : 05685-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCH80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

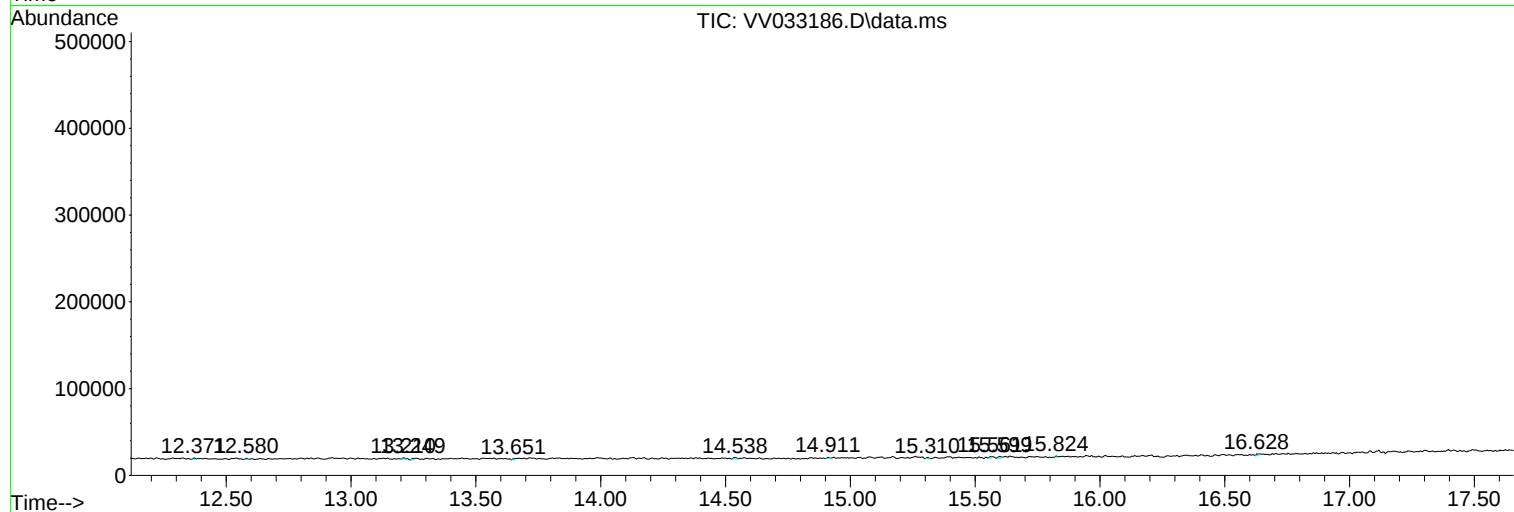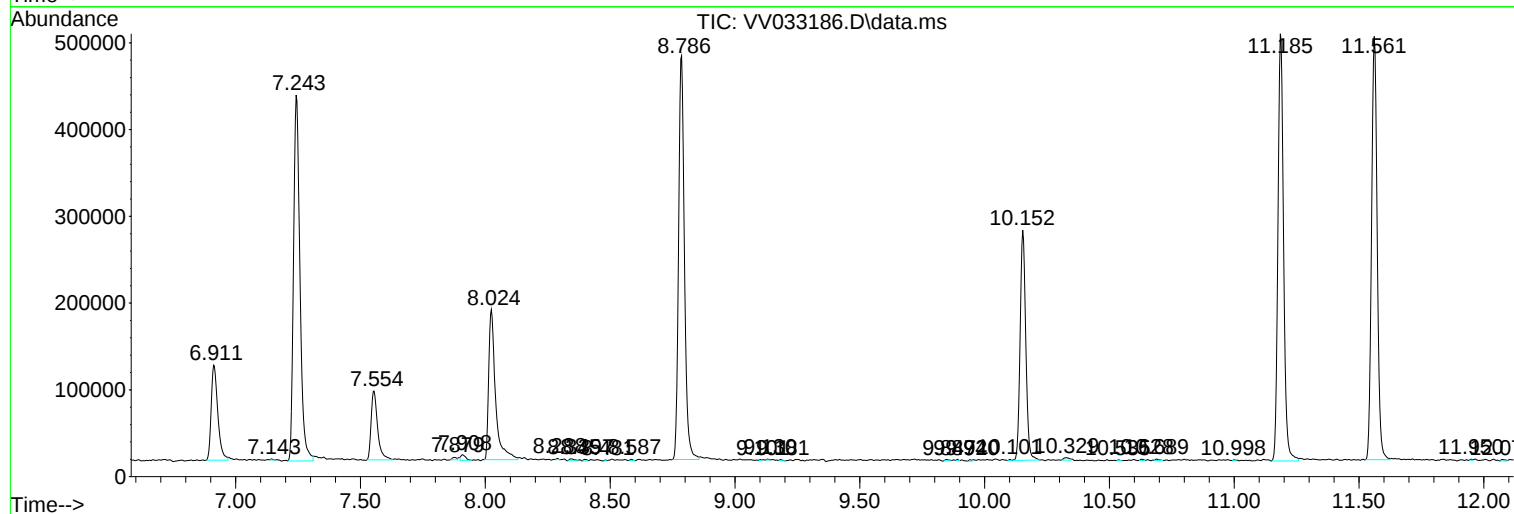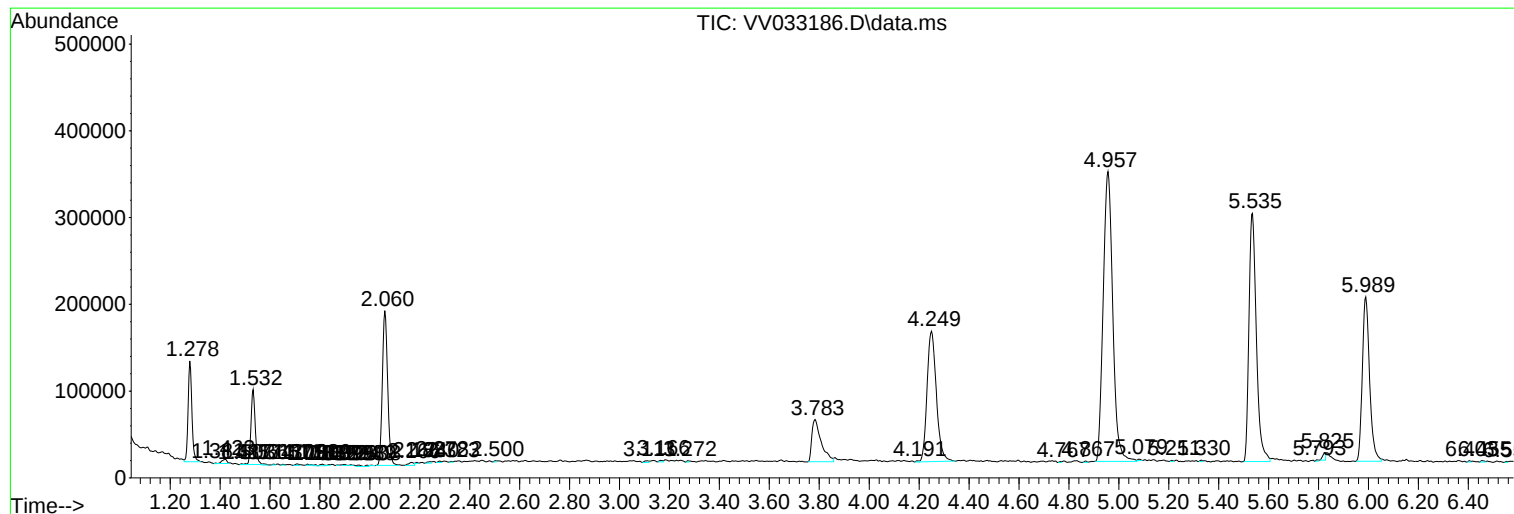

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033186.D
Acq On : 08 Dec 2023 13:32
Operator : SY/MD
Sample : 05685-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCH80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033186.D
Acq On : 08 Dec 2023 13:32
Operator : SY/MD
Sample : 05685-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
YCH80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------