

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033191.D
 Acq On : 08 Dec 2023 15:29
 Operator : SY/MD
 Sample : 05673-06DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEH9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M

Title : VOC Analysis

Signal : TIC: VV033191.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	85	rVB	108686	112137	7.45%	1.304%
2	1.381	103	106	110	rVB	2474	1896	0.13%	0.022%
3	1.420	110	118	125	rBV2	5264	7372	0.49%	0.086%
4	1.449	125	127	130	rVB	1670	773	0.05%	0.009%
5	1.474	130	135	136	rBV2	1334	1067	0.07%	0.012%
6	1.532	145	153	170	rVB	82769	99654	6.62%	1.159%
7	1.597	170	173	177	rVB2	934	683	0.05%	0.008%
8	1.626	177	182	184	rBV2	1310	1092	0.07%	0.013%
9	1.680	189	199	202	rBV	1573	2402	0.16%	0.028%
10	1.767	222	226	231	rVB3	1425	1666	0.11%	0.019%
11	1.793	231	234	237	rBV	866	709	0.05%	0.008%
12	1.841	246	249	252	rBV2	970	590	0.04%	0.007%
13	1.870	252	258	260	rBV	1039	903	0.06%	0.011%
14	1.918	270	273	278	rVB2	1040	916	0.06%	0.011%
15	1.954	278	284	289	rVB	727	943	0.06%	0.011%
16	2.008	294	301	304	rBV5	965	1060	0.07%	0.012%
17	2.060	307	317	333	rBV	177396	260190	17.28%	3.026%
18	2.124	333	337	341	rVB2	1031	944	0.06%	0.011%
19	2.156	344	347	350	rBV	2050	1542	0.10%	0.018%
20	2.185	350	356	357	rBV3	1288	1444	0.10%	0.017%
21	2.265	378	381	384	rVB	1150	753	0.05%	0.009%
22	2.285	384	387	390	rBV	1878	1018	0.07%	0.012%
23	2.307	390	394	397	rBV2	1080	1019	0.07%	0.012%
24	2.384	415	418	421	rBV	1537	1023	0.07%	0.012%
25	2.439	432	435	450	rVB4	2625	5168	0.34%	0.060%
26	2.558	469	472	476	rVB	1859	1270	0.08%	0.015%
27	2.629	490	494	497	rBV	1741	1303	0.09%	0.015%
28	2.741	525	529	532	rBV2	1072	963	0.06%	0.011%
29	2.847	559	562	565	rBV3	1330	916	0.06%	0.011%
30	3.201	670	672	674	rBV2	987	617	0.04%	0.007%
31	3.574	786	788	791	rVB	1355	722	0.05%	0.008%
32	3.786	844	854	858	rBV2	54145	101796	6.76%	1.184%
33	4.249	983	998	1021	rBV2	146572	376749	25.02%	4.382%
34	4.526	1080	1084	1086	rBV	1615	1328	0.09%	0.015%
35	4.764	1156	1158	1161	rBV2	1114	615	0.04%	0.007%
36	4.957	1202	1218	1243	rBV2	331959	877875	58.31%	10.211%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120823\
 Data File : VW033191.D
 Acq On : 08 Dec 2023 15:29
 Operator : SY/MD
 Sample : 05673-06DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEH9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.153	1276	1279	1281	rBV	1309	836	0.06%	0.010%
38	5.243	1304	1307	1310	rBV2	1332	1176	0.08%	0.014%
39	5.285	1317	1320	1325	rBV	1296	1372	0.09%	0.016%
40	5.532	1387	1397	1426	rBV	295541	599208	39.80%	6.970%
41	5.667	1437	1439	1442	rVB3	1501	836	0.06%	0.010%
42	5.831	1481	1490	1512	rVB8	20012	53408	3.55%	0.621%
43	5.989	1527	1539	1565	rBV2	182226	381239	25.32%	4.434%
44	6.095	1569	1572	1578	rVB	1532	1493	0.10%	0.017%
45	6.121	1578	1580	1583	rBV2	975	674	0.04%	0.008%
46	6.387	1660	1663	1666	rBV	1264	806	0.05%	0.009%
47	6.416	1669	1672	1674	rBV	1633	1043	0.07%	0.012%
48	6.494	1693	1696	1698	rBV	1168	783	0.05%	0.009%
49	6.632	1735	1739	1742	rBV	1807	1442	0.10%	0.017%
50	6.912	1817	1826	1854	rVB	103668	192615	12.79%	2.240%
51	7.114	1886	1889	1890	rBV2	992	591	0.04%	0.007%
52	7.185	1907	1911	1914	rBV	1587	1502	0.10%	0.017%
53	7.243	1919	1929	1951	rBV	410696	715982	47.56%	8.328%
54	7.555	2017	2026	2042	rBV	77339	141172	9.38%	1.642%
55	7.905	2122	2135	2153	rBV	894470	1505571	100.00%	17.512%
56	8.024	2163	2172	2199	rBV	183726	334899	22.24%	3.895%
57	8.529	2326	2329	2331	rBV	1342	823	0.05%	0.010%
58	8.786	2398	2409	2433	rBV	475901	776226	51.56%	9.029%
59	9.046	2487	2490	2493	rBV	1264	1005	0.07%	0.012%
60	9.153	2518	2523	2524	rBV	1817	1597	0.11%	0.019%
61	9.699	2690	2693	2698	rBV2	1382	1429	0.09%	0.017%
62	9.751	2706	2709	2714	rBV	1273	964	0.06%	0.011%
63	9.950	2768	2771	2777	rBV2	1098	1122	0.07%	0.013%
64	10.108	2815	2820	2822	rBV	1327	1331	0.09%	0.015%
65	10.153	2823	2834	2851	rVV	267884	420934	27.96%	4.896%
66	10.313	2880	2884	2887	rBV	2677	2480	0.16%	0.029%
67	10.538	2951	2954	2956	rBV	1279	617	0.04%	0.007%
68	11.017	3100	3103	3104	rBV	1316	779	0.05%	0.009%
69	11.127	3134	3137	3141	rBV	1679	1449	0.10%	0.017%
70	11.185	3145	3155	3176	rVV	508125	791335	52.56%	9.204%
71	11.342	3201	3204	3207	rBV	1612	1178	0.08%	0.014%
72	11.435	3228	3233	3236	rBV	1560	1741	0.12%	0.020%
73	11.561	3261	3272	3291	rBV	483465	754611	50.12%	8.777%
74	11.628	3291	3293	3299	rVB2	1938	1726	0.11%	0.020%
75	11.706	3314	3317	3319	rBV	1250	810	0.05%	0.009%
76	11.876	3368	3370	3374	rBV	1132	636	0.04%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033191.D
 Acq On : 08 Dec 2023 15:29
 Operator : SY/MD
 Sample : 05673-06DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHEH9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.972	3397	3400	3405	rBV	1247	1125	0.07%	0.013%
78	12.320	3505	3508	3513	rBV	1201	1229	0.08%	0.014%
79	12.349	3514	3517	3520	rVV2	1437	944	0.06%	0.011%
80	12.503	3561	3565	3572	rBV	1912	2652	0.18%	0.031%
81	12.532	3572	3574	3577	rBV	956	754	0.05%	0.009%
82	12.599	3592	3595	3599	rBV	1290	1039	0.07%	0.012%
83	12.982	3711	3714	3716	rBV	1548	964	0.06%	0.011%
84	13.259	3797	3800	3802	rBV	1044	766	0.05%	0.009%
85	13.291	3808	3810	3814	rBV3	1135	782	0.05%	0.009%
86	13.590	3900	3903	3904	rBV	1272	754	0.05%	0.009%
87	13.635	3912	3917	3920	rBV2	1455	1642	0.11%	0.019%
88	13.702	3935	3938	3943	rVB	1648	1312	0.09%	0.015%
89	13.898	3997	3999	4003	rBV	1086	881	0.06%	0.010%
90	13.940	4009	4012	4014	rBV2	1228	904	0.06%	0.011%
91	13.995	4025	4029	4030	rBV	1204	890	0.06%	0.010%
92	14.149	4074	4077	4079	rVB	1476	863	0.06%	0.010%
93	14.316	4126	4129	4133	rVB3	1318	962	0.06%	0.011%
94	14.612	4218	4221	4223	rBV2	1158	829	0.06%	0.010%
95	15.416	4469	4471	4474	rBV2	1223	781	0.05%	0.009%
96	15.464	4483	4486	4489	rVB2	1590	918	0.06%	0.011%
97	16.236	4723	4726	4728	rBV2	1878	1224	0.08%	0.014%
98	16.320	4749	4752	4754	rBV	1671	1183	0.08%	0.014%
99	16.911	4933	4936	4938	rBV4	2448	1755	0.12%	0.020%
100	17.483	5111	5114	5117	rBV3	2692	1717	0.11%	0.020%




Sum of corrected areas: 8597429

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033191.D
Acq On : 08 Dec 2023 15:29
Operator : SY/MD
Sample : 05673-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEH9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

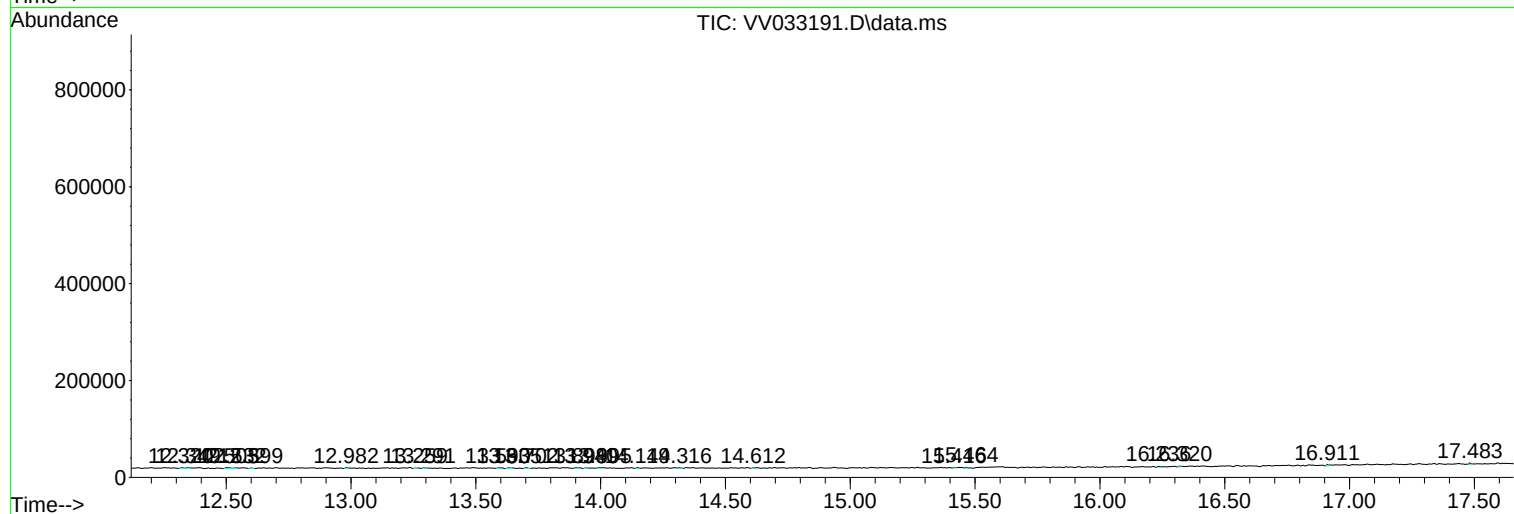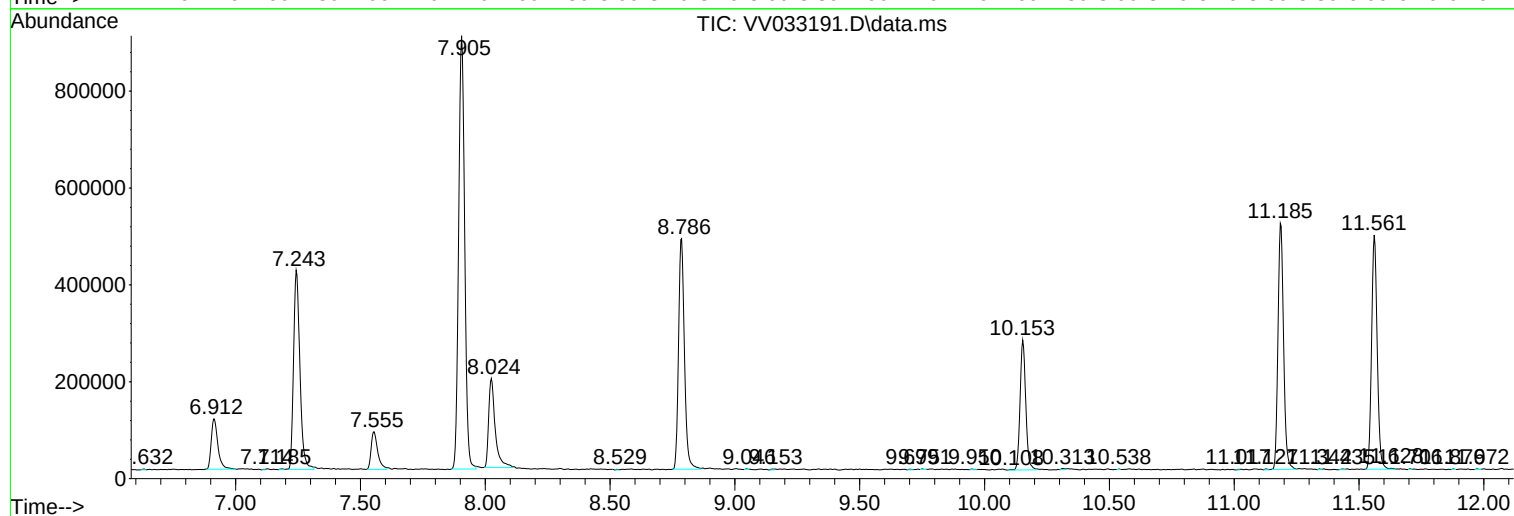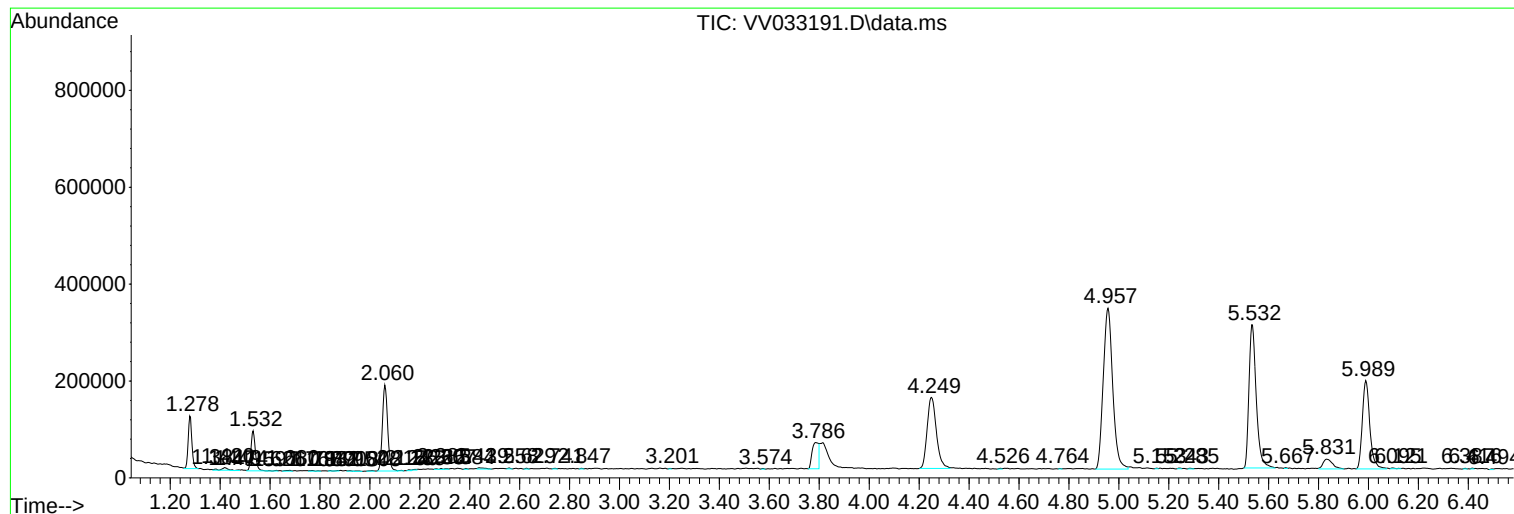

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033191.D
Acq On : 08 Dec 2023 15:29
Operator : SY/MD
Sample : 05673-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEH9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033191.D
Acq On : 08 Dec 2023 15:29
Operator : SY/MD
Sample : 05673-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHEH9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------