

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033192.D
 Acq On : 08 Dec 2023 15:52
 Operator : SY/MD
 Sample : 05673-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033192.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	94	rVB	112310	121668	13.66%	1.689%
2	1.372	99	103	107	rVB	1664	1200	0.13%	0.017%
3	1.420	110	118	126	rVB3	5432	8513	0.96%	0.118%
4	1.532	145	153	169	rVB	84293	102605	11.52%	1.424%
5	1.606	171	176	180	rVB2	992	937	0.11%	0.013%
6	1.654	185	191	194	rVB2	1261	1306	0.15%	0.018%
7	1.680	194	199	201	rBV2	876	843	0.09%	0.012%
8	1.732	210	215	222	rVB2	1954	1981	0.22%	0.028%
9	1.764	222	225	227	rBV	1003	743	0.08%	0.010%
10	1.818	239	242	248	rVB3	1150	877	0.10%	0.012%
11	1.854	248	253	256	rBV3	1070	1148	0.13%	0.016%
12	1.899	261	267	270	rBV2	894	1005	0.11%	0.014%
13	1.966	283	288	291	rBV	1311	1491	0.17%	0.021%
14	2.002	296	299	301	rVB2	887	625	0.07%	0.009%
15	2.060	305	317	335	rVB	180310	263707	29.62%	3.661%
16	2.130	335	339	342	rBV2	1037	582	0.07%	0.008%
17	2.172	342	352	353	rBV	3134	4295	0.48%	0.060%
18	2.314	393	396	398	rBV3	1507	1022	0.11%	0.014%
19	2.349	404	407	410	rBV2	1213	980	0.11%	0.014%
20	2.404	421	424	425	rBV2	1502	866	0.10%	0.012%
21	2.966	597	599	602	rBV	1074	558	0.06%	0.008%
22	3.101	637	641	646	rBV2	1238	1450	0.16%	0.020%
23	3.159	656	659	662	rBV	1031	849	0.10%	0.012%
24	3.326	709	711	717	rVB	1859	1791	0.20%	0.025%
25	3.410	734	737	741	rBV2	1468	1262	0.14%	0.018%
26	3.545	776	779	782	rBV	1487	1190	0.13%	0.017%
27	3.561	782	784	787	rVV	1051	611	0.07%	0.008%
28	3.616	798	801	803	rBV	1089	706	0.08%	0.010%
29	3.783	844	853	883	rBV	51116	141415	15.88%	1.963%
30	4.249	984	998	1019	rBV	147295	372878	41.88%	5.177%
31	4.474	1066	1068	1070	rBV	1001	612	0.07%	0.008%
32	4.558	1091	1094	1096	rBV	1545	1021	0.11%	0.014%
33	4.767	1156	1159	1163	rVB	2109	1495	0.17%	0.021%
34	4.957	1201	1218	1241	rBV2	334938	890415	100.00%	12.362%
35	5.121	1267	1269	1272	rBV3	1204	718	0.08%	0.010%
36	5.291	1318	1322	1324	rBV2	1988	1756	0.20%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033192.D
 Acq On : 08 Dec 2023 15:52
 Operator : SY/MD
 Sample : 05673-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.339	1334	1337	1344	rBV	1457	1613	0.18%	0.022%
38	5.387	1350	1352	1355	rBV	934	538	0.06%	0.007%
39	5.535	1386	1398	1423	rBV	294999	610158	68.53%	8.471%
40	5.793	1475	1478	1480	rBV	1509	816	0.09%	0.011%
41	5.828	1480	1489	1506	rVV3	12027	27600	3.10%	0.383%
42	5.989	1526	1539	1566	rBV	182177	383427	43.06%	5.323%
43	6.211	1605	1608	1611	rBV	1740	1389	0.16%	0.019%
44	6.535	1704	1709	1714	rBV	1840	2350	0.26%	0.033%
45	6.600	1726	1729	1731	rVB	1365	732	0.08%	0.010%
46	6.616	1731	1734	1735	rBV	1151	680	0.08%	0.009%
47	6.664	1746	1749	1751	rBV	1651	1064	0.12%	0.015%
48	6.764	1776	1780	1782	rBV	1501	1065	0.12%	0.015%
49	6.789	1783	1788	1792	rVV	1550	1657	0.19%	0.023%
50	6.912	1816	1826	1847	rBV	107011	200783	22.55%	2.788%
51	7.098	1882	1884	1887	rBV2	1208	738	0.08%	0.010%
52	7.243	1918	1929	1957	rBV	413100	736054	82.66%	10.219%
53	7.378	1968	1971	1974	rBV2	1386	1073	0.12%	0.015%
54	7.555	2017	2026	2038	rBV	81258	141844	15.93%	1.969%
55	7.728	2077	2080	2083	rBV2	1581	1358	0.15%	0.019%
56	7.805	2101	2104	2108	rBV	1636	1374	0.15%	0.019%
57	7.847	2115	2117	2120	rBV	1187	597	0.07%	0.008%
58	7.908	2130	2136	2144	rBV9	3251	5175	0.58%	0.072%
59	7.985	2158	2160	2163	rBV	1031	549	0.06%	0.008%
60	8.024	2163	2172	2203	rBV	185905	363843	40.86%	5.051%
61	8.275	2245	2250	2254	rBV	1748	2331	0.26%	0.032%
62	8.336	2267	2269	2270	rBV	1298	648	0.07%	0.009%
63	8.464	2307	2309	2313	rVB	1689	1078	0.12%	0.015%
64	8.683	2374	2377	2380	rBV	1499	912	0.10%	0.013%
65	8.786	2397	2409	2429	rBV	471828	770766	86.56%	10.701%
66	9.021	2479	2482	2485	rBV	1649	1137	0.13%	0.016%
67	9.104	2505	2508	2513	rBV3	1333	1422	0.16%	0.020%
68	9.165	2521	2527	2529	rBV	1987	1912	0.21%	0.027%
69	9.307	2568	2571	2576	rBV2	1462	1494	0.17%	0.021%
70	9.365	2586	2589	2592	rBV	1343	1032	0.12%	0.014%
71	9.628	2668	2671	2676	rVB	1901	1670	0.19%	0.023%
72	9.661	2676	2681	2683	rBV	1473	1642	0.18%	0.023%
73	9.677	2684	2686	2689	rVB	1651	920	0.10%	0.013%
74	10.153	2824	2834	2855	rVB	266603	423225	47.53%	5.876%
75	10.522	2946	2949	2952	rBV	1766	1272	0.14%	0.018%
76	10.577	2964	2966	2974	rVB	1482	1306	0.15%	0.018%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033192.D
 Acq On : 08 Dec 2023 15:52
 Operator : SY/MD
 Sample : 05673-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	10.805	3035	3037	3042	rVB2	1374	923	0.10%	0.013%
78	11.069	3117	3119	3123	rVB2	1665	975	0.11%	0.014%
79	11.185	3145	3155	3178	rBV	510009	784192	88.07%	10.887%
80	11.361	3207	3210	3213	rBV2	1491	1176	0.13%	0.016%
81	11.400	3219	3222	3225	rBV	1291	1185	0.13%	0.016%
82	11.561	3261	3272	3292	rBV	483788	758969	85.24%	10.537%
83	12.185	3462	3466	3473	rBV2	2107	2438	0.27%	0.034%
84	12.622	3597	3602	3605	rBV2	1349	1623	0.18%	0.023%
85	12.866	3676	3678	3682	rVB	1223	724	0.08%	0.010%
86	13.066	3737	3740	3743	rBV2	1270	1005	0.11%	0.014%
87	13.233	3790	3792	3796	rBV2	1256	829	0.09%	0.012%
88	13.268	3800	3803	3805	rBV2	1519	1039	0.12%	0.014%
89	13.516	3878	3880	3884	rBV2	1396	865	0.10%	0.012%
90	13.667	3925	3927	3928	rBV	1008	525	0.06%	0.007%
91	13.747	3950	3952	3956	rVB	1628	1052	0.12%	0.015%
92	14.422	4160	4162	4164	rBV	1120	604	0.07%	0.008%
93	14.554	4197	4203	4205	rBV	2268	2526	0.28%	0.035%
94	14.937	4319	4322	4323	rBV	1399	916	0.10%	0.013%
95	15.004	4340	4343	4345	rBV	1621	1084	0.12%	0.015%
96	15.120	4376	4379	4384	rBV	1524	1510	0.17%	0.021%
97	15.207	4404	4406	4408	rBV2	1158	606	0.07%	0.008%
98	15.336	4443	4446	4449	rBV2	1840	1176	0.13%	0.016%
99	15.467	4483	4487	4490	rBV2	1546	1523	0.17%	0.021%
100	15.651	4542	4544	4546	rBV2	1782	1123	0.13%	0.016%




Sum of corrected areas: 7202953

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033192.D
Acq On : 08 Dec 2023 15:52
Operator : SY/MD
Sample : 05673-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

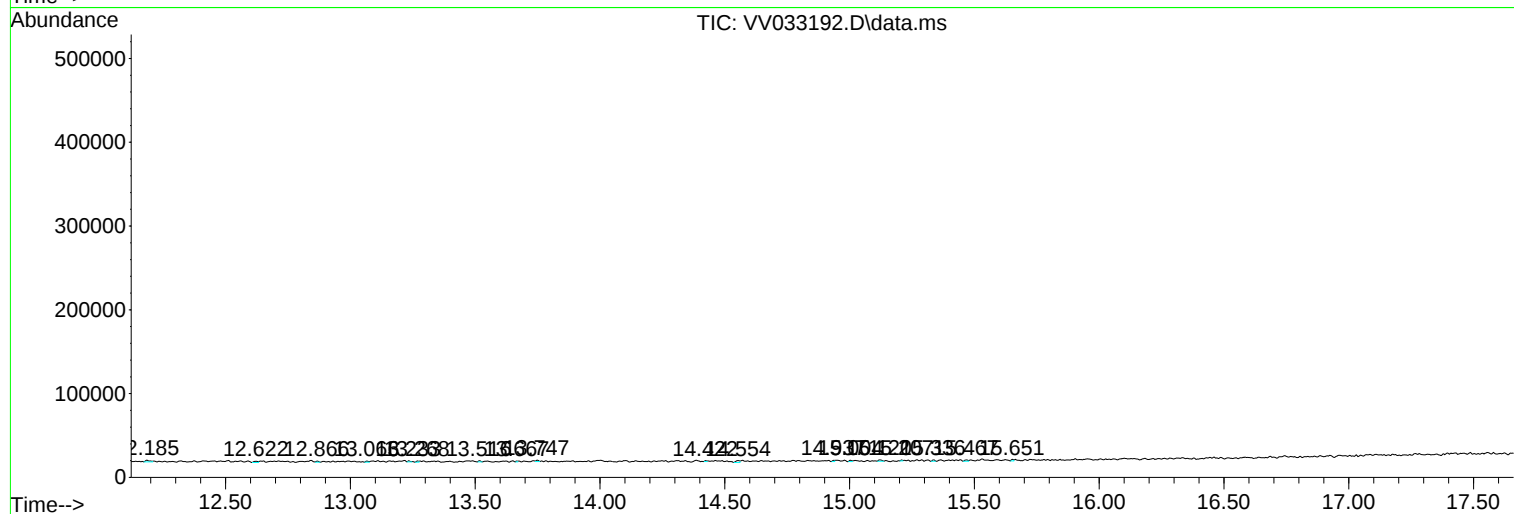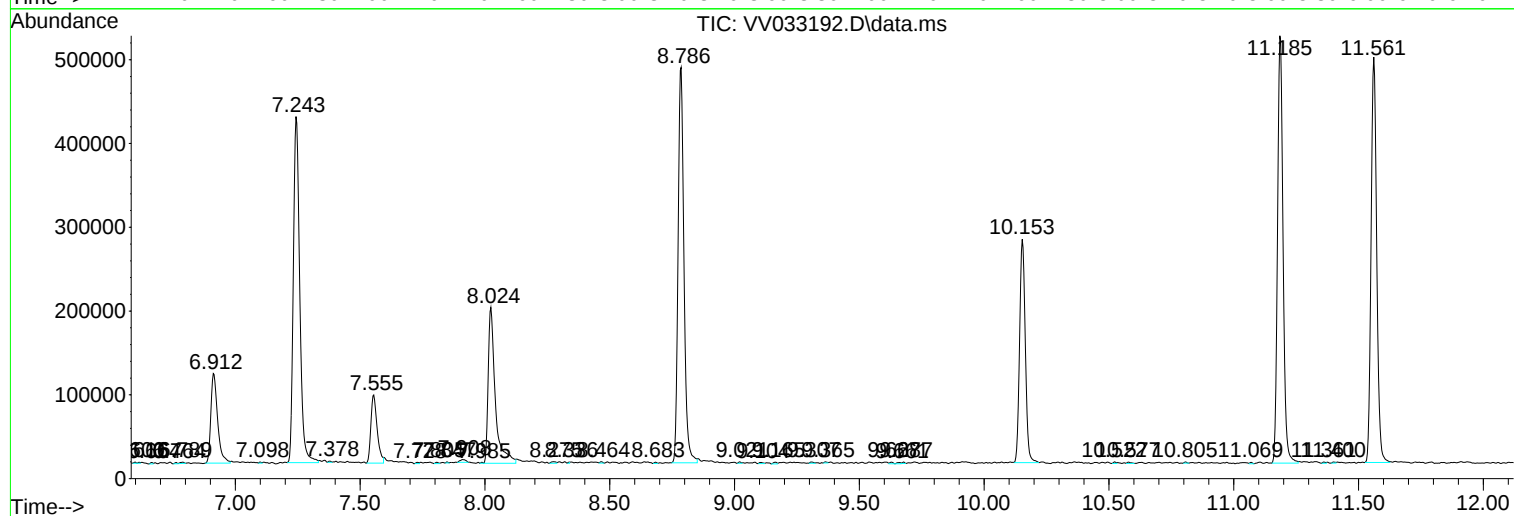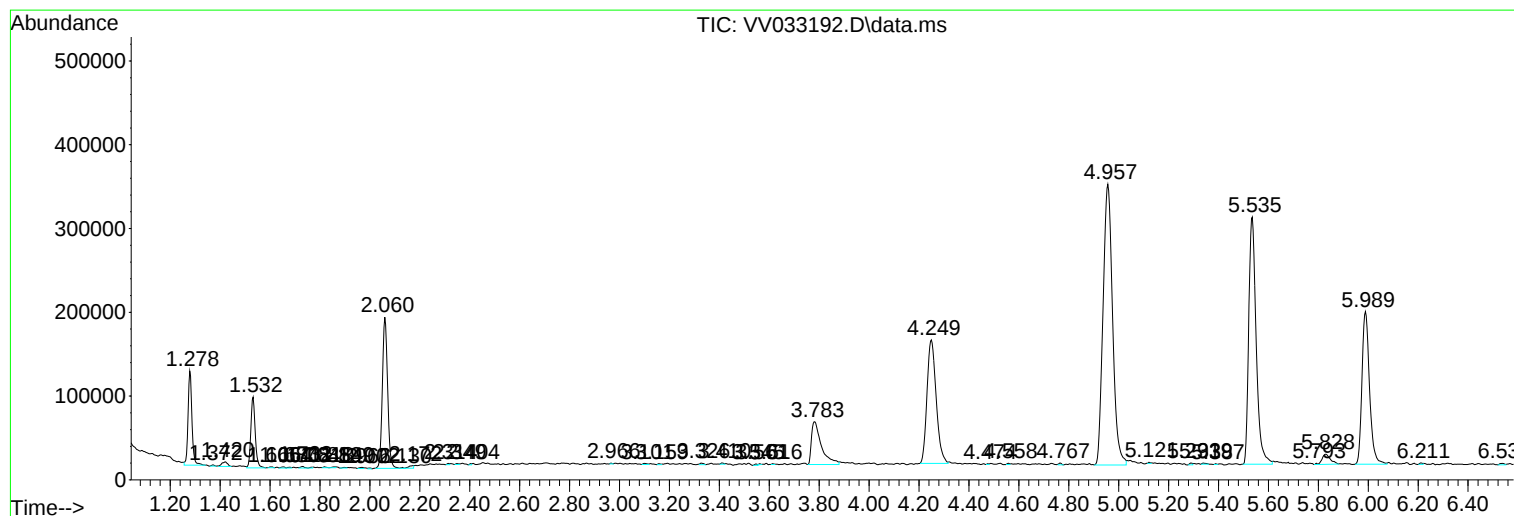

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033192.D
Acq On : 08 Dec 2023 15:52
Operator : SY/MD
Sample : 05673-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033192.D
Acq On : 08 Dec 2023 15:52
Operator : SY/MD
Sample : 05673-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------