

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033194.D
 Acq On : 08 Dec 2023 16:39
 Operator : SY/MD
 Sample : 05689-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	113781	115967	13.25%	1.632%
2	1.423	111	119	122	rVV3	3982	4605	0.53%	0.065%
3	1.452	126	128	131	rVB	2034	1031	0.12%	0.015%
4	1.468	131	133	137	rBV2	1171	1029	0.12%	0.014%
5	1.491	137	140	142	rBV	1253	977	0.11%	0.014%
6	1.532	145	153	164	rBV	82872	96746	11.05%	1.362%
7	1.706	205	207	209	rBV	831	522	0.06%	0.007%
8	1.725	210	213	216	rVB	1077	681	0.08%	0.010%
9	1.767	221	226	228	rBV3	853	614	0.07%	0.009%
10	1.796	231	235	241	rBV3	965	1023	0.12%	0.014%
11	1.918	270	273	279	rVB2	1650	1283	0.15%	0.018%
12	1.954	279	284	289	rBV	1810	1932	0.22%	0.027%
13	1.989	293	295	298	rVB2	1152	705	0.08%	0.010%
14	2.060	306	317	332	rBV	179333	262455	29.98%	3.694%
15	2.114	332	334	339	rVB3	1898	1257	0.14%	0.018%
16	2.146	339	344	346	rBV	1596	1455	0.17%	0.020%
17	2.175	346	353	354	rBV	1435	1409	0.16%	0.020%
18	2.220	354	367	376	rBV	10533	21024	2.40%	0.296%
19	2.651	499	501	507	rBV	1032	960	0.11%	0.014%
20	2.802	544	548	549	rBV	1261	1004	0.11%	0.014%
21	3.082	633	635	638	rBV	1029	562	0.06%	0.008%
22	3.214	673	676	678	rBV	972	633	0.07%	0.009%
23	3.285	695	698	702	rVB	1493	1192	0.14%	0.017%
24	3.384	727	729	733	rVB	1299	798	0.09%	0.011%
25	3.410	733	737	739	rBV	1372	1180	0.13%	0.017%
26	3.571	785	787	791	rBV	1016	777	0.09%	0.011%
27	3.703	825	828	833	rBV2	1271	1102	0.13%	0.016%
28	3.780	844	852	878	rBV2	52906	147026	16.80%	2.069%
29	4.249	982	998	1018	rBV	148462	374644	42.80%	5.273%
30	4.555	1091	1093	1097	rVB2	1342	740	0.08%	0.010%
31	4.596	1104	1106	1109	rVB	1837	913	0.10%	0.013%
32	4.616	1109	1112	1115	rBV2	1130	694	0.08%	0.010%
33	4.812	1170	1173	1175	rBV2	989	671	0.08%	0.009%
34	4.957	1202	1218	1244	rBV3	328103	875410	100.00%	12.322%
35	5.207	1294	1296	1299	rBV	1586	920	0.11%	0.013%
36	5.230	1299	1303	1305	rVV	1429	903	0.10%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120823\
 Data File : VW033194.D
 Acq On : 08 Dec 2023 16:39
 Operator : SY/MD
 Sample : 05689-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.301	1322	1325	1329	rVB	1431	1026	0.12%	0.014%
38	5.535	1386	1398	1420	rBV	292386	600675	68.62%	8.455%
39	5.789	1475	1477	1479	rBV	1157	638	0.07%	0.009%
40	5.834	1481	1491	1506	rVB7	10903	25060	2.86%	0.353%
41	5.989	1527	1539	1563	rBV	187115	378167	43.20%	5.323%
42	6.236	1613	1616	1618	rBV2	1059	668	0.08%	0.009%
43	6.342	1645	1649	1652	rBV	1585	1234	0.14%	0.017%
44	6.384	1658	1662	1663	rBV	1050	785	0.09%	0.011%
45	6.468	1685	1688	1694	rBV	1159	1419	0.16%	0.020%
46	6.571	1717	1720	1722	rBV	1165	731	0.08%	0.010%
47	6.661	1745	1748	1750	rBV2	1496	940	0.11%	0.013%
48	6.731	1767	1770	1774	rBV2	1391	1027	0.12%	0.014%
49	6.757	1775	1778	1780	rBV	903	765	0.09%	0.011%
50	6.876	1812	1815	1816	rBV	895	526	0.06%	0.007%
51	6.915	1816	1827	1844	rVV	106186	199617	22.80%	2.810%
52	7.243	1918	1929	1947	rBV	415978	721888	82.46%	10.161%
53	7.503	2008	2010	2013	rBV2	1007	599	0.07%	0.008%
54	7.555	2017	2026	2049	rVV	79166	142341	16.26%	2.004%
55	8.024	2163	2172	2196	rBV	187154	349144	39.88%	4.914%
56	8.297	2255	2257	2260	rBV	1318	704	0.08%	0.010%
57	8.786	2398	2409	2434	rBV	464576	766488	87.56%	10.789%
58	9.288	2560	2565	2568	rBV	1774	1969	0.22%	0.028%
59	9.391	2592	2597	2600	rBV3	1741	2009	0.23%	0.028%
60	9.464	2617	2620	2623	rBV	1088	631	0.07%	0.009%
61	9.490	2623	2628	2632	rBV	1487	1375	0.16%	0.019%
62	9.513	2632	2635	2637	rBV	1124	661	0.08%	0.009%
63	9.561	2648	2650	2652	rBV	1037	657	0.08%	0.009%
64	9.638	2671	2674	2677	rBV2	1540	1214	0.14%	0.017%
65	9.757	2709	2711	2714	rBV	896	549	0.06%	0.008%
66	9.915	2757	2760	2764	rVB	1564	1038	0.12%	0.015%
67	9.956	2770	2773	2778	rBV	1130	1111	0.13%	0.016%
68	10.085	2809	2813	2815	rBV2	1152	1036	0.12%	0.015%
69	10.153	2823	2834	2858	rBV	271114	426736	48.75%	6.007%
70	10.484	2935	2937	2940	rBV2	1271	921	0.11%	0.013%
71	10.554	2956	2959	2960	rBV2	902	526	0.06%	0.007%
72	10.728	3011	3013	3016	rBV2	962	674	0.08%	0.009%
73	10.808	3034	3038	3043	rBV	1979	1915	0.22%	0.027%
74	10.915	3068	3071	3074	rBV2	892	651	0.07%	0.009%
75	10.931	3074	3076	3080	rVB	1567	917	0.10%	0.013%
76	10.950	3080	3082	3085	rBV2	1010	591	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033194.D
 Acq On : 08 Dec 2023 16:39
 Operator : SY/MD
 Sample : 05689-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	11.040	3107	3110	3115	rVB	2211	1636	0.19%	0.023%
78	11.085	3122	3124	3127	rVB	1117	576	0.07%	0.008%
79	11.101	3127	3129	3133	rBV2	842	545	0.06%	0.008%
80	11.185	3145	3155	3181	rBV	489821	761869	87.03%	10.724%
81	11.561	3261	3272	3291	rBV	486017	753588	86.08%	10.607%
82	12.217	3474	3476	3481	rVB	1603	1067	0.12%	0.015%
83	12.294	3498	3500	3504	rVB	1725	1060	0.12%	0.015%
84	12.490	3558	3561	3565	rBV	1614	994	0.11%	0.014%
85	12.699	3620	3626	3627	rBV	1488	1511	0.17%	0.021%
86	13.014	3720	3724	3731	rBV	1707	1773	0.20%	0.025%
87	13.062	3737	3739	3741	rBV	1263	766	0.09%	0.011%
88	13.197	3777	3781	3783	rBV2	1667	1384	0.16%	0.019%
89	13.294	3808	3811	3815	rBV2	1364	1404	0.16%	0.020%
90	13.519	3879	3881	3888	rBV2	1060	1031	0.12%	0.015%
91	13.641	3917	3919	3922	rVB2	1782	933	0.11%	0.013%
92	13.660	3922	3925	3931	rVB	2131	1779	0.20%	0.025%
93	13.738	3944	3949	3952	rBV3	1572	1800	0.21%	0.025%
94	13.795	3965	3967	3971	rVB2	1168	765	0.09%	0.011%
95	14.400	4152	4155	4158	rBV	1697	1034	0.12%	0.015%
96	14.464	4173	4175	4177	rBV2	1265	702	0.08%	0.010%
97	14.676	4238	4241	4245	rBV2	1431	953	0.11%	0.013%
98	14.731	4255	4258	4260	rBV2	1083	725	0.08%	0.010%
99	15.516	4500	4502	4504	rBV2	1210	742	0.08%	0.010%
100	15.799	4588	4590	4595	rVB2	2216	1441	0.16%	0.020%




Sum of corrected areas: 7104545

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033194.D
Acq On : 08 Dec 2023 16:39
Operator : SY/MD
Sample : 05689-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

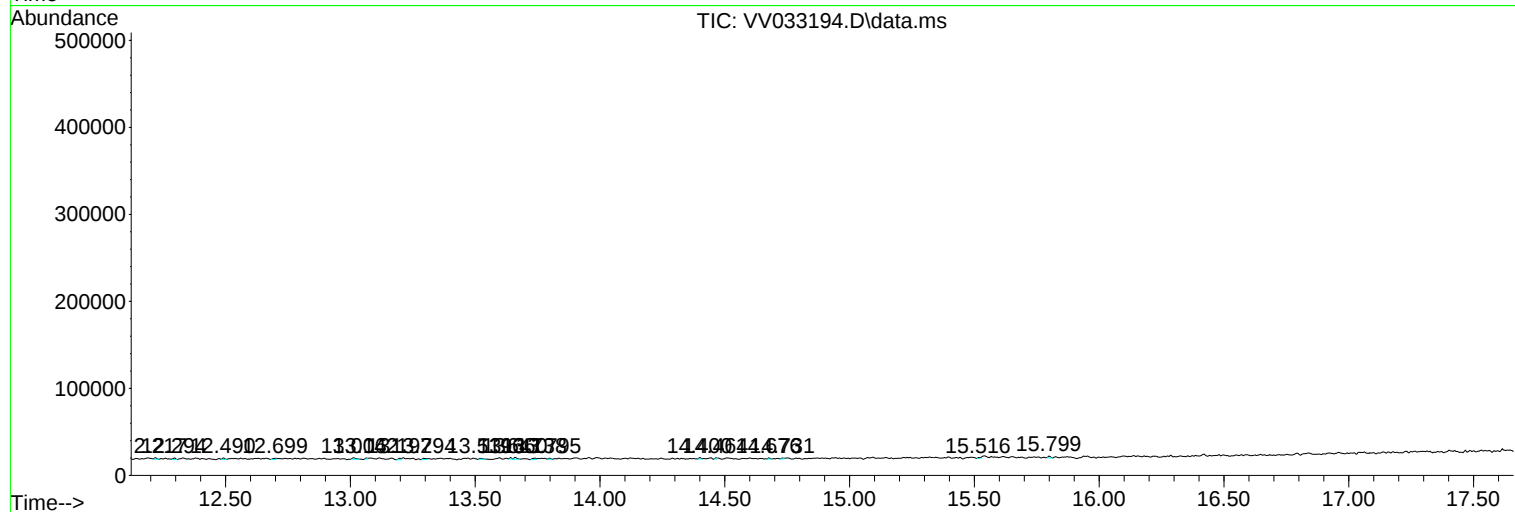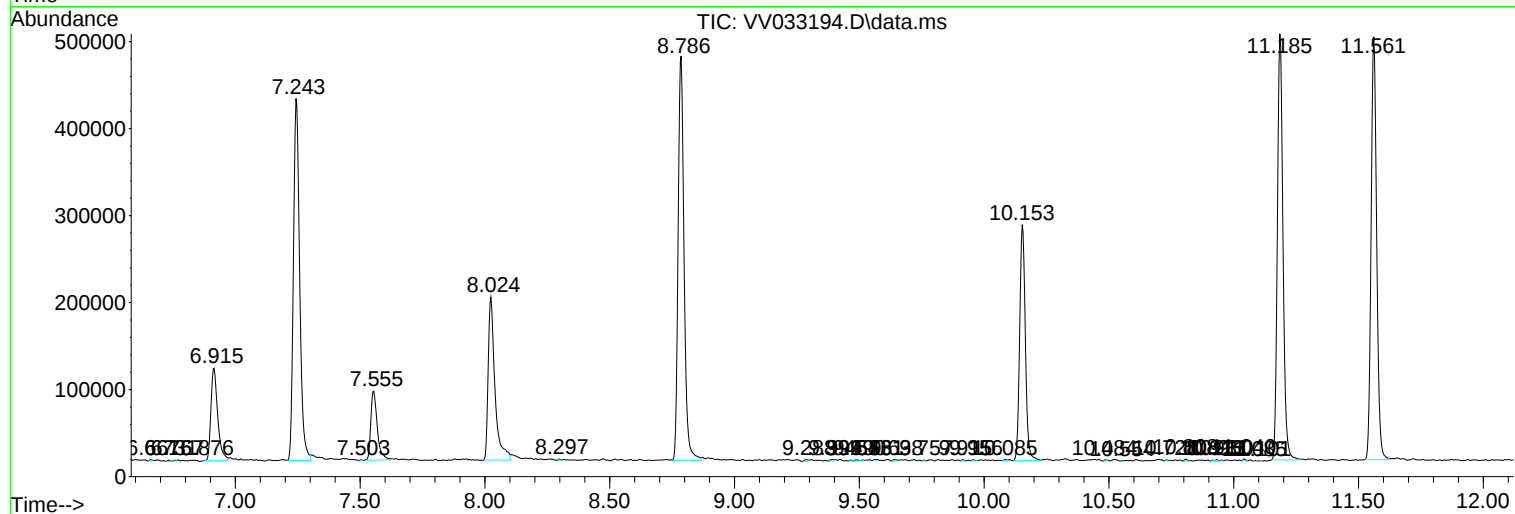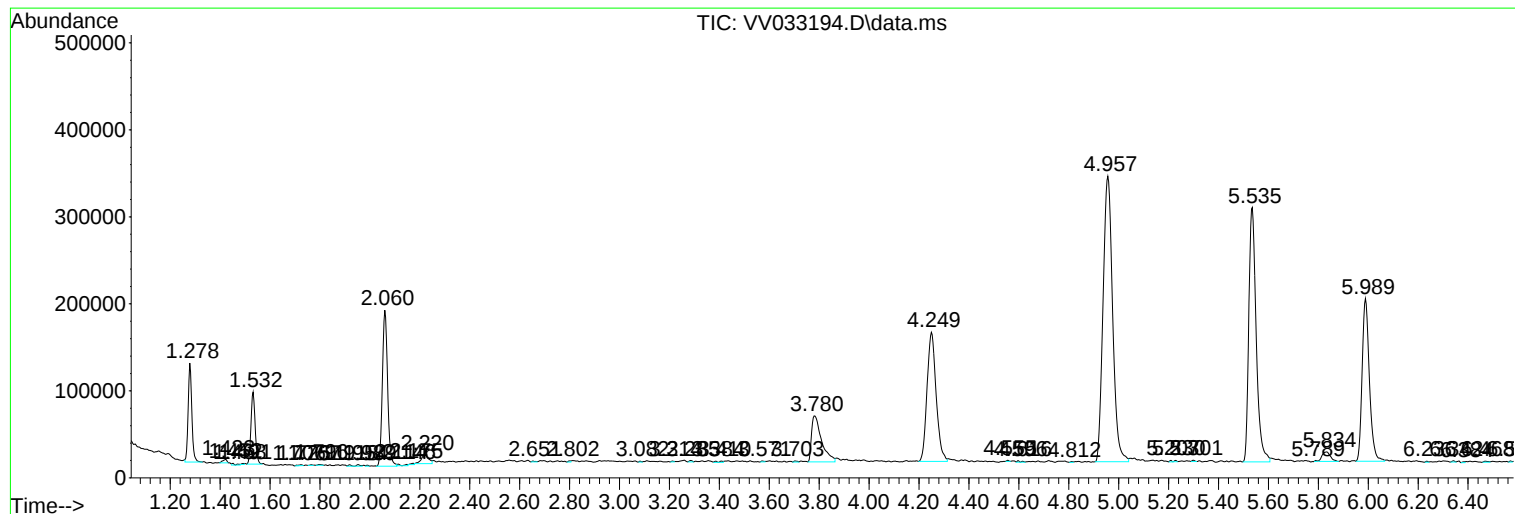

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033194.D
Acq On : 08 Dec 2023 16:39
Operator : SY/MD
Sample : 05689-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033194.D
Acq On : 08 Dec 2023 16:39
Operator : SY/MD
Sample : 05689-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------