

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033195.D
 Acq On : 08 Dec 2023 17:02
 Operator : SY/MD
 Sample : 05689-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033195.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	109148	115486	13.38%	1.616%
2	1.420	112	118	124	rVB2	5202	6207	0.72%	0.087%
3	1.532	140	153	168	rVB	83094	101388	11.75%	1.418%
4	1.600	168	174	178	rBV3	748	803	0.09%	0.011%
5	1.626	178	182	184	rBV	963	795	0.09%	0.011%
6	1.680	194	199	204	rVB	932	1130	0.13%	0.016%
7	1.719	204	211	215	rVB4	1641	2111	0.24%	0.030%
8	1.744	215	219	222	rBV	1495	1442	0.17%	0.020%
9	1.793	231	234	237	rBV2	1054	830	0.10%	0.012%
10	1.815	237	241	246	rVV2	1354	1334	0.15%	0.019%
11	1.883	257	262	267	rBV	1098	924	0.11%	0.013%
12	1.908	267	270	274	rBV3	1055	821	0.10%	0.011%
13	1.928	274	276	282	rVB	1515	1329	0.15%	0.019%
14	1.970	286	289	294	rVB2	1571	1625	0.19%	0.023%
15	1.992	294	296	302	rVB	1579	1232	0.14%	0.017%
16	2.024	302	306	307	rBV	1129	909	0.11%	0.013%
17	2.060	307	317	340	rVB	177021	262446	30.41%	3.671%
18	2.169	340	351	353	rBV	3571	5304	0.61%	0.074%
19	2.220	360	367	374	rBV2	6587	10990	1.27%	0.154%
20	2.310	392	395	402	rBV	1614	1474	0.17%	0.021%
21	2.452	437	439	443	rVB2	1311	881	0.10%	0.012%
22	2.510	454	457	459	rBV2	1136	872	0.10%	0.012%
23	3.127	646	649	652	rBV	1376	1016	0.12%	0.014%
24	3.339	710	715	718	rBV2	1756	1671	0.19%	0.023%
25	3.449	746	749	752	rBV	1734	1103	0.13%	0.015%
26	3.551	777	781	785	rBV	1738	1390	0.16%	0.019%
27	3.748	839	842	844	rBV	1199	836	0.10%	0.012%
28	3.783	844	853	881	rVV2	51625	149026	17.27%	2.085%
29	4.150	964	967	969	rBV	1544	1124	0.13%	0.016%
30	4.185	975	978	982	rVB	1296	950	0.11%	0.013%
31	4.249	982	998	1022	rBV	149538	377640	43.76%	5.283%
32	4.590	1101	1104	1108	rVB	1379	958	0.11%	0.013%
33	4.715	1141	1143	1146	rVB	1564	907	0.11%	0.013%
34	4.802	1166	1170	1178	rBV	1709	1825	0.21%	0.026%
35	4.957	1201	1218	1241	rBV3	324717	862982	100.00%	12.072%
36	5.098	1260	1262	1270	rVB4	2484	2328	0.27%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120823\
 Data File : VW033195.D
 Acq On : 08 Dec 2023 17:02
 Operator : SY/MD
 Sample : 05689-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.275	1314	1317	1319	rBV	1151	792	0.09%	0.011%
38	5.471	1374	1378	1381	rBV2	995	887	0.10%	0.012%
39	5.535	1385	1398	1428	rBV	275545	575435	66.68%	8.050%
40	5.674	1438	1441	1443	rBV	1356	848	0.10%	0.012%
41	5.748	1461	1464	1466	rBV	2141	1634	0.19%	0.023%
42	5.834	1478	1491	1511	rBV4	92063	205430	23.80%	2.874%
43	5.989	1527	1539	1560	rBV2	181026	373914	43.33%	5.231%
44	6.436	1675	1678	1682	rBV2	1231	954	0.11%	0.013%
45	6.574	1718	1721	1724	rVB	1376	925	0.11%	0.013%
46	6.731	1767	1770	1773	rBV	1728	1321	0.15%	0.018%
47	6.860	1806	1810	1814	rBV4	1255	1379	0.16%	0.019%
48	6.915	1817	1827	1847	rBV	105832	195586	22.66%	2.736%
49	7.030	1861	1863	1868	rVB	1445	892	0.10%	0.012%
50	7.101	1883	1885	1890	rVB	1849	1237	0.14%	0.017%
51	7.243	1918	1929	1948	rBV	401439	704695	81.66%	9.858%
52	7.432	1985	1988	1992	rVB3	1341	1010	0.12%	0.014%
53	7.490	2003	2006	2007	rBV	1442	867	0.10%	0.012%
54	7.555	2017	2026	2048	rBV	77303	140130	16.24%	1.960%
55	8.024	2163	2172	2208	rBV	182638	345107	39.99%	4.828%
56	8.786	2396	2409	2437	rBV	444147	737504	85.46%	10.317%
57	9.001	2474	2476	2482	rVB2	1544	1055	0.12%	0.015%
58	9.030	2482	2485	2491	rBV	1583	1634	0.19%	0.023%
59	9.223	2542	2545	2549	rBV2	1354	918	0.11%	0.013%
60	9.384	2590	2595	2601	rVB2	1961	2231	0.26%	0.031%
61	9.410	2601	2603	2607	rBV	1392	1184	0.14%	0.017%
62	9.464	2617	2620	2625	rBV2	1379	1492	0.17%	0.021%
63	9.529	2637	2640	2642	rBV2	1654	1044	0.12%	0.015%
64	9.966	2773	2776	2779	rVB	1809	1015	0.12%	0.014%
65	10.107	2816	2820	2824	rBV	1335	1186	0.14%	0.017%
66	10.152	2824	2834	2853	rVV	266298	411784	47.72%	5.760%
67	10.365	2897	2900	2903	rBV	1434	1121	0.13%	0.016%
68	10.519	2945	2948	2954	rVB	1842	1971	0.23%	0.028%
69	10.693	2999	3002	3006	rVB2	1284	861	0.10%	0.012%
70	10.783	3026	3030	3033	rBV	1274	1179	0.14%	0.016%
71	10.898	3063	3066	3069	rBV	1698	1347	0.16%	0.019%
72	11.040	3107	3110	3112	rBV	1127	804	0.09%	0.011%
73	11.188	3144	3156	3176	rBV	463874	733794	85.03%	10.265%
74	11.561	3261	3272	3289	rVV	473259	733129	84.95%	10.256%
75	11.722	3319	3322	3325	rBV2	1367	920	0.11%	0.013%
76	12.191	3465	3468	3473	rVB	1341	1153	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033195.D
 Acq On : 08 Dec 2023 17:02
 Operator : SY/MD
 Sample : 05689-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GC8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.242	3481	3484	3488	rBV	1275	1310	0.15%	0.018%
78	12.487	3557	3560	3563	rBV	1574	970	0.11%	0.014%
79	12.731	3633	3636	3640	rBV	1156	1004	0.12%	0.014%
80	12.812	3656	3661	3668	rVB	2181	2759	0.32%	0.039%
81	12.850	3668	3673	3676	rBV2	1626	1729	0.20%	0.024%
82	13.066	3737	3740	3744	rVB	1711	1063	0.12%	0.015%
83	13.281	3803	3807	3810	rBV	1493	1407	0.16%	0.020%
84	13.535	3883	3886	3888	rBV	1497	1015	0.12%	0.014%
85	13.866	3984	3989	3993	rBV2	1783	1998	0.23%	0.028%
86	14.075	4050	4054	4056	rVB	1447	997	0.12%	0.014%
87	14.098	4057	4061	4064	rVB	1805	1367	0.16%	0.019%
88	14.297	4120	4123	4127	rBV2	1543	1384	0.16%	0.019%
89	14.320	4127	4130	4136	rVV2	1971	1758	0.20%	0.025%
90	14.660	4233	4236	4240	rVB2	1478	1187	0.14%	0.017%
91	14.728	4255	4257	4262	rVB	1334	828	0.10%	0.012%
92	14.927	4316	4319	4324	rBV2	1553	1513	0.18%	0.021%
93	15.303	4432	4436	4440	rBV3	1303	1625	0.19%	0.023%
94	15.422	4471	4473	4480	rVB	1421	1375	0.16%	0.019%
95	15.583	4520	4523	4525	rBV3	1414	880	0.10%	0.012%
96	15.619	4532	4534	4538	rVB2	1496	912	0.11%	0.013%
97	15.824	4595	4598	4601	rBV4	1839	1736	0.20%	0.024%
98	16.242	4722	4728	4730	rBV3	2849	3147	0.36%	0.044%
99	16.618	4843	4845	4847	rBV	1956	1001	0.12%	0.014%
100	16.789	4895	4898	4899	rBV2	1932	1021	0.12%	0.014%




Sum of corrected areas: 7148444

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033195.D
Acq On : 08 Dec 2023 17:02
Operator : SY/MD
Sample : 05689-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

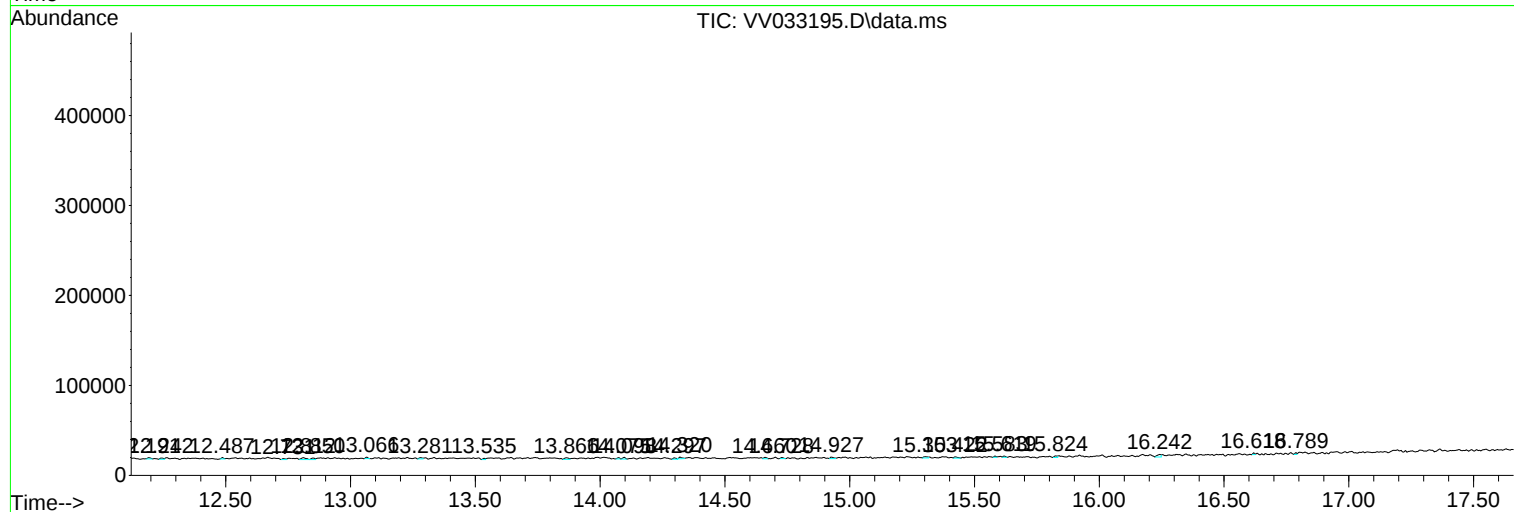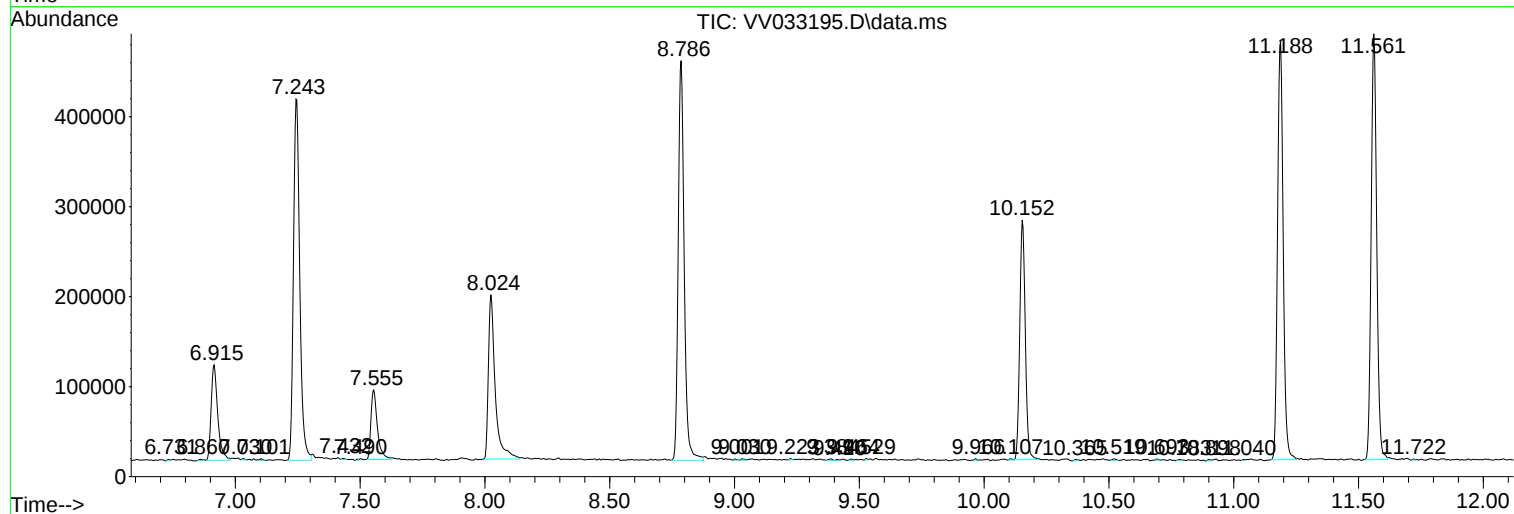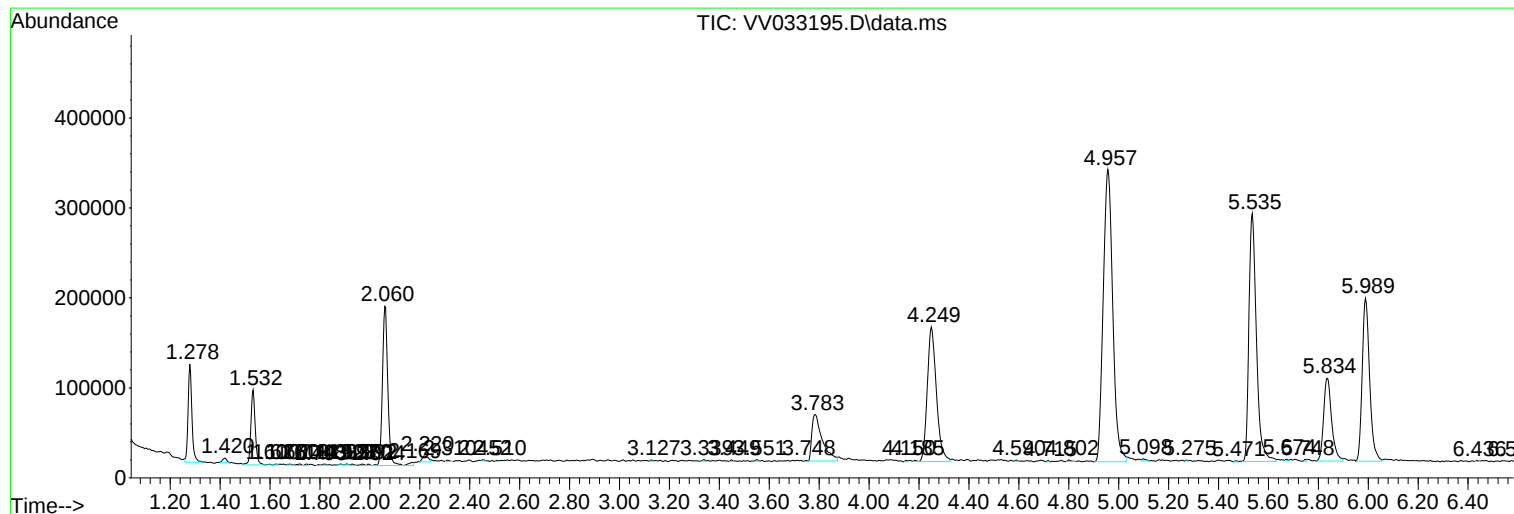

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033195.D
Acq On : 08 Dec 2023 17:02
Operator : SY/MD
Sample : 05689-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033195.D
Acq On : 08 Dec 2023 17:02
Operator : SY/MD
Sample : 05689-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GC8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc