

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033196.D
 Acq On : 08 Dec 2023 17:25
 Operator : SY/MD
 Sample : 05689-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033196.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	116837	123298	13.65%	1.527%
2	1.343	91	94	98	rBV3	1257	935	0.10%	0.012%
3	1.420	110	118	126	rVB4	5935	9565	1.06%	0.118%
4	1.532	144	153	163	rVV	82674	98904	10.95%	1.225%
5	1.635	177	185	189	rBV4	917	1216	0.13%	0.015%
6	1.677	195	198	202	rVB	1538	987	0.11%	0.012%
7	1.719	202	211	216	rBV3	1283	1796	0.20%	0.022%
8	1.818	238	242	246	rVB2	1036	953	0.11%	0.012%
9	1.902	261	268	270	rBV	1117	1028	0.11%	0.013%
10	1.918	270	273	281	rVB2	1065	1180	0.13%	0.015%
11	1.976	286	291	296	rVB4	1068	1032	0.11%	0.013%
12	2.060	307	317	333	rBV2	184521	290254	32.13%	3.596%
13	2.163	346	349	352	rVV2	941	770	0.09%	0.010%
14	2.188	352	357	358	rVV	2038	1727	0.19%	0.021%
15	2.224	358	368	379	rVV3	5382	12845	1.42%	0.159%
16	2.288	385	388	390	rBV	1490	896	0.10%	0.011%
17	2.301	390	392	396	rVB	1441	938	0.10%	0.012%
18	2.445	433	437	442	rVB2	1788	1873	0.21%	0.023%
19	2.571	473	476	479	rBV2	1307	900	0.10%	0.011%
20	2.767	534	537	541	rVB	2147	1618	0.18%	0.020%
21	2.806	546	549	552	rBV	1519	1008	0.11%	0.012%
22	2.883	567	573	580	rBV	1740	2356	0.26%	0.029%
23	2.931	585	588	594	rBV	1280	1027	0.11%	0.013%
24	2.957	594	596	599	rBV	1081	883	0.10%	0.011%
25	3.111	642	644	647	rVB	2098	1088	0.12%	0.013%
26	3.294	698	701	703	rBV	1192	840	0.09%	0.010%
27	3.580	785	790	793	rBV	1537	1604	0.18%	0.020%
28	3.786	844	854	884	rBV3	53714	183779	20.34%	2.277%
29	3.992	915	918	923	rVB2	2277	1698	0.19%	0.021%
30	4.121	955	958	961	rBV3	1129	1099	0.12%	0.014%
31	4.249	982	998	1020	rBV2	144175	373144	41.30%	4.622%
32	4.400	1042	1045	1048	rVB3	1747	1068	0.12%	0.013%
33	4.519	1069	1082	1092	rBV5	6096	14350	1.59%	0.178%
34	4.635	1115	1118	1126	rVB	2498	2918	0.32%	0.036%
35	4.670	1126	1129	1132	rBV	1421	1057	0.12%	0.013%
36	4.957	1201	1218	1244	rBV3	329776	866915	95.95%	10.739%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120823\
 Data File : VW033196.D
 Acq On : 08 Dec 2023 17:25
 Operator : SY/MD
 Sample : 05689-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	5.535	1386	1398	1425	rBV	290210	599978	66.41%	7.432%
38	5.712	1451	1453	1459	rVB3	1495	1242	0.14%	0.015%
39	5.831	1477	1490	1516	rBV	446656	903462	100.00%	11.192%
40	5.989	1527	1539	1565	rVB2	182773	374728	41.48%	4.642%
41	6.410	1668	1670	1675	rVB	1289	1072	0.12%	0.013%
42	6.474	1683	1690	1694	rBV	2035	2582	0.29%	0.032%
43	6.571	1715	1720	1723	rBV2	1976	1909	0.21%	0.024%
44	6.587	1723	1725	1730	rVV	913	858	0.09%	0.011%
45	6.915	1816	1827	1850	rBV	106011	205344	22.73%	2.544%
46	7.243	1918	1929	1952	rBV	402403	710101	78.60%	8.796%
47	7.555	2017	2026	2045	rBV	79379	139443	15.43%	1.727%
48	7.667	2057	2061	2064	rBV2	1430	1047	0.12%	0.013%
49	7.863	2119	2122	2124	rBV	1520	957	0.11%	0.012%
50	7.879	2124	2127	2132	rVV3	2087	2448	0.27%	0.030%
51	7.908	2133	2136	2142	rVB3	1975	1791	0.20%	0.022%
52	8.024	2163	2172	2200	rBV	187824	355052	39.30%	4.398%
53	8.194	2222	2225	2227	rBV2	1512	875	0.10%	0.011%
54	8.352	2271	2274	2277	rBV	1680	1190	0.13%	0.015%
55	8.535	2328	2331	2337	rBV	1691	1501	0.17%	0.019%
56	8.609	2351	2354	2360	rVB	1683	1497	0.17%	0.019%
57	8.657	2367	2369	2374	rVB	1737	1337	0.15%	0.017%
58	8.683	2374	2377	2379	rBV	1678	1117	0.12%	0.014%
59	8.786	2398	2409	2434	rBV	465859	769896	85.22%	9.537%
60	9.124	2511	2514	2517	rBV	1233	787	0.09%	0.010%
61	9.291	2563	2566	2569	rBV	1681	1195	0.13%	0.015%
62	9.561	2648	2650	2653	rBV2	982	812	0.09%	0.010%
63	9.622	2666	2669	2671	rBV2	1324	941	0.10%	0.012%
64	9.950	2768	2771	2777	rBV2	1249	1212	0.13%	0.015%
65	10.153	2824	2834	2857	rVB	265782	422734	46.79%	5.237%
66	10.297	2876	2879	2882	rVB	1319	857	0.09%	0.011%
67	10.336	2885	2891	2895	rBV5	1612	1744	0.19%	0.022%
68	10.400	2907	2911	2914	rBV	1445	1124	0.12%	0.014%
69	10.416	2914	2916	2918	rVV2	1157	746	0.08%	0.009%
70	10.432	2918	2921	2926	rVB	2135	1935	0.21%	0.024%
71	10.509	2942	2945	2952	rBV	1359	1467	0.16%	0.018%
72	10.934	3074	3077	3085	rVB	2343	2227	0.25%	0.028%
73	11.185	3145	3155	3173	rBV	496347	776916	85.99%	9.624%
74	11.339	3198	3203	3204	rBV	1546	1453	0.16%	0.018%
75	11.561	3261	3272	3292	rBV	471074	735363	81.39%	9.109%
76	11.882	3369	3372	3377	rVV2	1046	1042	0.12%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033196.D
 Acq On : 08 Dec 2023 17:25
 Operator : SY/MD
 Sample : 05689-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GD3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	12.493	3557	3562	3566	rBV2	1619	1592	0.18%	0.020%
78	12.847	3668	3672	3676	rBV3	1766	1418	0.16%	0.018%
79	12.921	3693	3695	3699	rVB	1465	900	0.10%	0.011%
80	13.496	3872	3874	3877	rBV	1261	816	0.09%	0.010%
81	13.619	3909	3912	3915	rBV	1471	1168	0.13%	0.014%
82	13.779	3960	3962	3967	rVB	2202	1668	0.18%	0.021%
83	13.937	4009	4011	4016	rVB	1274	821	0.09%	0.010%
84	13.966	4017	4020	4023	rVV	1438	1168	0.13%	0.014%
85	13.988	4025	4027	4031	rVB	2113	1437	0.16%	0.018%
86	14.075	4051	4054	4057	rBV2	1587	1007	0.11%	0.012%
87	14.230	4099	4102	4109	rBV2	1321	1254	0.14%	0.016%
88	14.493	4181	4184	4187	rBV	2003	1407	0.16%	0.017%
89	14.638	4223	4229	4234	rVB2	2164	2825	0.31%	0.035%
90	14.702	4246	4249	4251	rBV	1125	836	0.09%	0.010%
91	14.760	4264	4267	4269	rBV2	1102	796	0.09%	0.010%
92	15.178	4394	4397	4402	rBV2	1143	912	0.10%	0.011%
93	15.255	4419	4421	4424	rBV3	1600	837	0.09%	0.010%
94	15.275	4424	4427	4430	rBV3	1299	1136	0.13%	0.014%
95	15.358	4448	4453	4457	rBV	1769	1903	0.21%	0.024%
96	15.387	4457	4462	4464	rBV4	1967	1924	0.21%	0.024%
97	15.693	4554	4557	4560	rBV	1513	1237	0.14%	0.015%
98	15.943	4632	4635	4637	rBV3	1852	1272	0.14%	0.016%
99	15.985	4644	4648	4655	rBV3	2000	2736	0.30%	0.034%
100	16.037	4661	4664	4667	rBV2	2505	2007	0.22%	0.025%




Sum of corrected areas: 8072608

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033196.D
Acq On : 08 Dec 2023 17:25
Operator : SY/MD
Sample : 05689-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

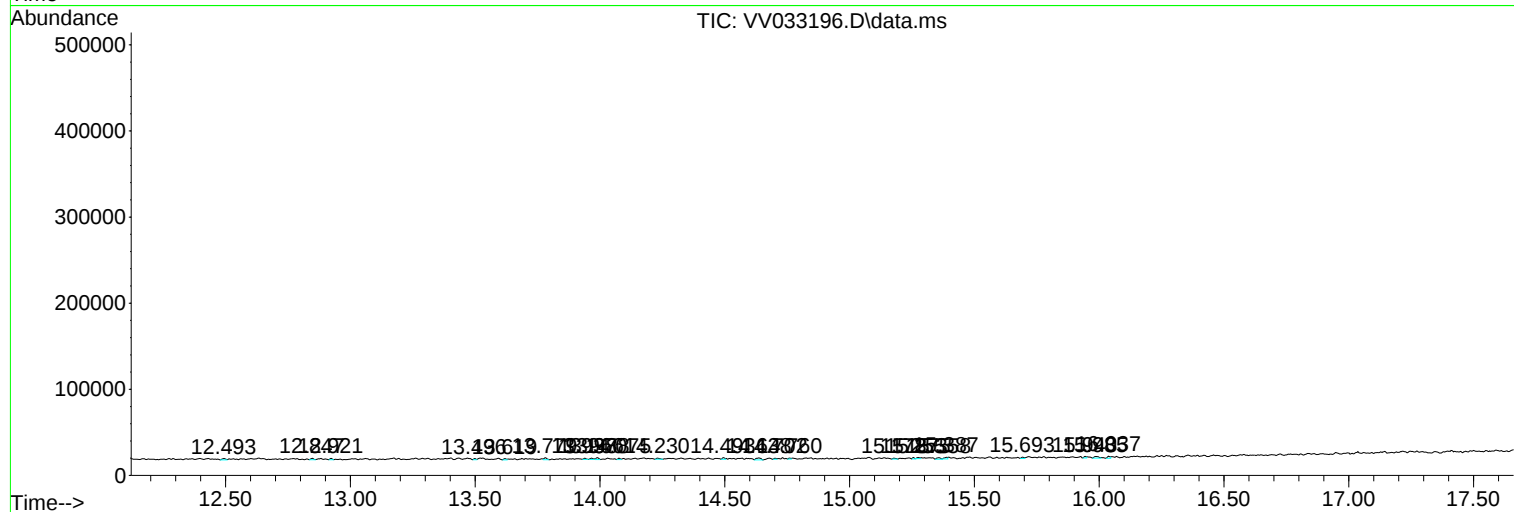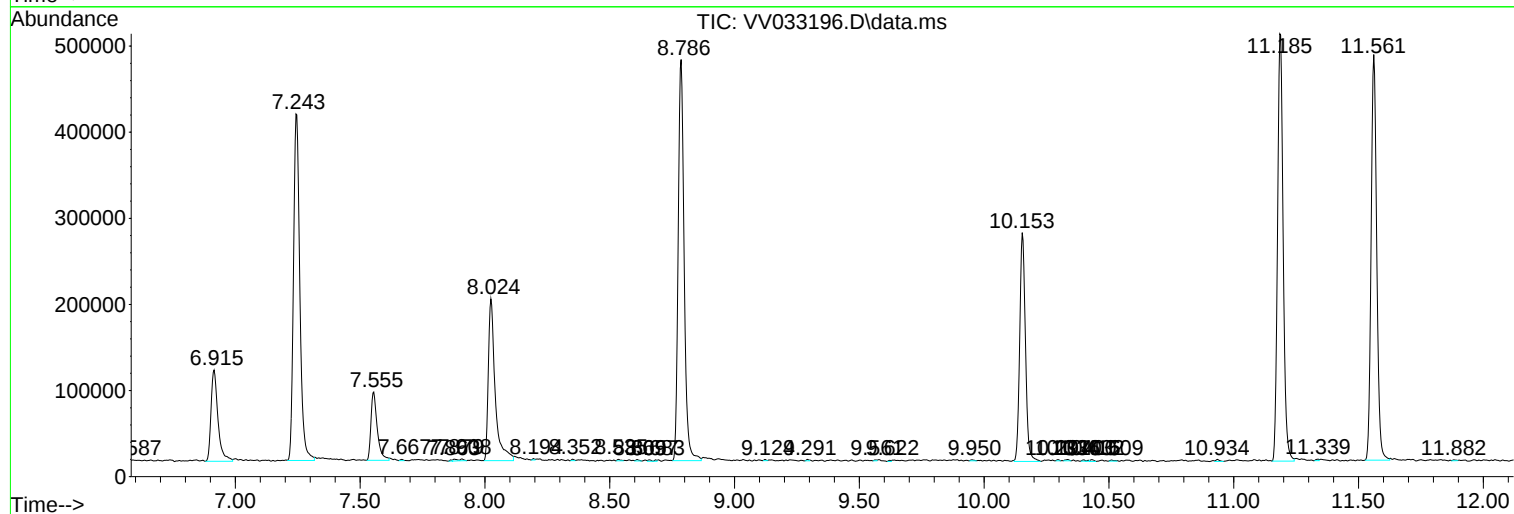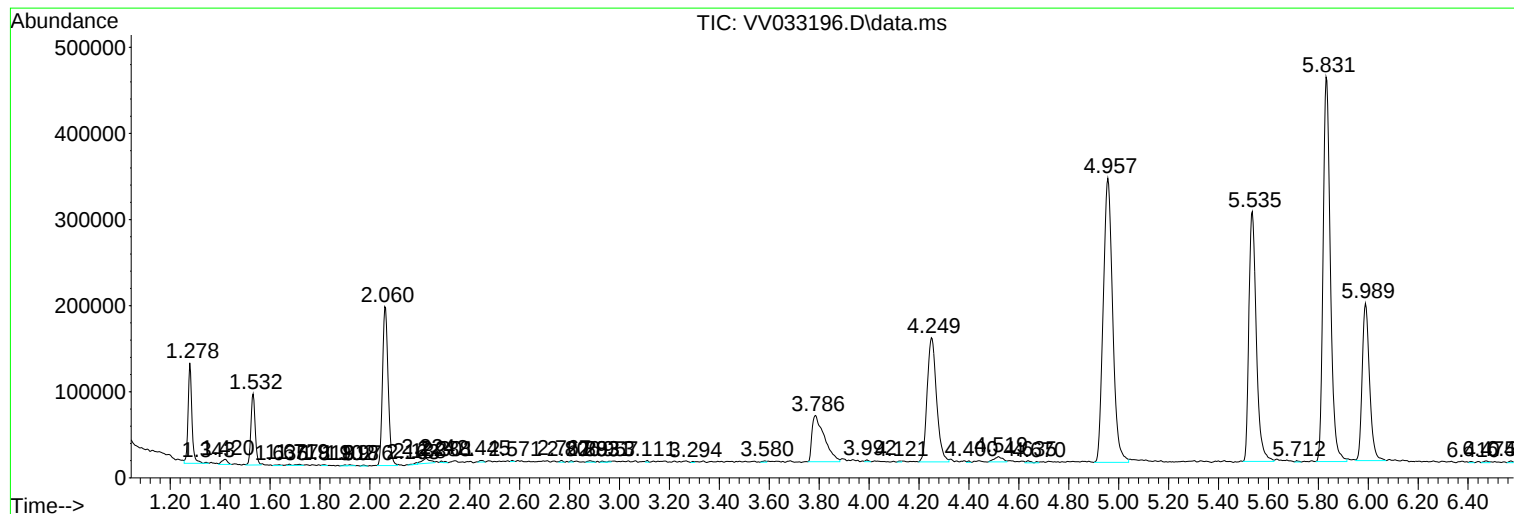

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033196.D
Acq On : 08 Dec 2023 17:25
Operator : SY/MD
Sample : 05689-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033196.D
Acq On : 08 Dec 2023 17:25
Operator : SY/MD
Sample : 05689-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GD3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc