

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033197.D
 Acq On : 08 Dec 2023 17:49
 Operator : SY/MD
 Sample : 05689-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	89	rVB	109626	117380	13.71%	1.683%
2	1.423	109	119	124	rVB3	5274	8081	0.94%	0.116%
3	1.532	144	153	163	rBV	81388	95963	11.21%	1.376%
4	1.622	179	181	187	rVB4	920	891	0.10%	0.013%
5	1.770	220	227	232	rBV4	1567	2353	0.27%	0.034%
6	1.847	244	251	254	rBV2	813	884	0.10%	0.013%
7	2.060	306	317	331	rBV	173994	253385	29.60%	3.634%
8	2.156	341	347	349	rBV	2413	2349	0.27%	0.034%
9	2.182	349	355	358	rVV	2100	2582	0.30%	0.037%
10	2.224	358	368	375	rVV3	5771	11697	1.37%	0.168%
11	2.269	380	382	387	rVB2	1460	1285	0.15%	0.018%
12	2.397	419	422	427	rBV	1481	1466	0.17%	0.021%
13	2.423	427	430	434	rBV	1438	1288	0.15%	0.018%
14	2.535	462	465	471	rVV	1875	1746	0.20%	0.025%
15	2.571	473	476	479	rVB	1869	1253	0.15%	0.018%
16	2.979	600	603	607	rBV	1338	1184	0.14%	0.017%
17	3.159	654	659	661	rBV	2123	1877	0.22%	0.027%
18	3.783	843	853	883	rBV	54194	146632	17.13%	2.103%
19	4.056	936	938	942	rBV2	890	680	0.08%	0.010%
20	4.249	984	998	1022	rBV	144757	366084	42.77%	5.250%
21	4.529	1082	1085	1087	rBV2	986	841	0.10%	0.012%
22	4.648	1120	1122	1126	rVB2	1304	715	0.08%	0.010%
23	4.748	1147	1153	1158	rBV2	1718	2325	0.27%	0.033%
24	4.802	1167	1170	1175	rBV3	1367	1569	0.18%	0.023%
25	4.957	1203	1218	1241	rBV2	325830	855951	100.00%	12.275%
26	5.166	1281	1283	1286	rBV	1427	812	0.09%	0.012%
27	5.432	1363	1366	1371	rBV2	1041	783	0.09%	0.011%
28	5.535	1387	1398	1423	rBV	283647	582564	68.06%	8.355%
29	5.831	1482	1490	1505	rVB6	11655	23804	2.78%	0.341%
30	5.989	1527	1539	1558	rBV	181596	370226	43.25%	5.309%
31	6.252	1618	1621	1622	rBV	1584	947	0.11%	0.014%
32	6.297	1632	1635	1637	rBV2	1006	710	0.08%	0.010%
33	6.358	1652	1654	1658	rVB2	1348	801	0.09%	0.011%
34	6.500	1695	1698	1703	rBV	1039	931	0.11%	0.013%
35	6.667	1745	1750	1757	rBV	1469	2094	0.24%	0.030%
36	6.767	1778	1781	1785	rVB	1480	1111	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120823\
 Data File : VW033197.D
 Acq On : 08 Dec 2023 17:49
 Operator : SY/MD
 Sample : 05689-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	6.789	1785	1788	1791	rBV2	1365	1067	0.12%	0.015%
38	6.915	1817	1827	1847	rBV	102946	192156	22.45%	2.756%
39	7.146	1897	1899	1902	rBV	1163	672	0.08%	0.010%
40	7.165	1903	1905	1908	rBV3	1011	841	0.10%	0.012%
41	7.198	1913	1915	1918	rBV2	1161	863	0.10%	0.012%
42	7.243	1919	1929	1951	rBV	399336	706982	82.60%	10.139%
43	7.555	2017	2026	2043	rBV	77457	136096	15.90%	1.952%
44	7.686	2065	2067	2072	rBV	1276	868	0.10%	0.012%
45	8.024	2163	2172	2200	rBV	189136	361934	42.28%	5.190%
46	8.169	2214	2217	2220	rBV	1556	1123	0.13%	0.016%
47	8.326	2263	2266	2268	rBV2	1524	1028	0.12%	0.015%
48	8.628	2354	2360	2365	rBV	1672	2261	0.26%	0.032%
49	8.673	2371	2374	2377	rBV	1040	730	0.09%	0.010%
50	8.786	2398	2409	2433	rBV	452771	735930	85.98%	10.554%
51	8.995	2470	2474	2478	rBV	1978	1997	0.23%	0.029%
52	9.288	2562	2565	2569	rVB	1105	871	0.10%	0.012%
53	9.497	2627	2630	2631	rBV	1084	691	0.08%	0.010%
54	9.561	2648	2650	2656	rBV2	843	701	0.08%	0.010%
55	9.895	2751	2754	2759	rVB	1172	875	0.10%	0.013%
56	9.924	2760	2763	2768	rVB	1334	1040	0.12%	0.015%
57	9.976	2774	2779	2781	rBV	1037	1032	0.12%	0.015%
58	10.152	2824	2834	2856	rVB	265069	421934	49.29%	6.051%
59	10.911	3067	3070	3075	rVB	1378	1045	0.12%	0.015%
60	10.947	3079	3081	3087	rBV	1138	1129	0.13%	0.016%
61	11.091	3123	3126	3129	rBV	1229	894	0.10%	0.013%
62	11.130	3135	3138	3143	rVB	1551	1333	0.16%	0.019%
63	11.185	3143	3155	3176	rBV	477811	745884	87.14%	10.697%
64	11.332	3197	3201	3205	rVB	2177	1961	0.23%	0.028%
65	11.361	3206	3210	3213	rVB	1897	1452	0.17%	0.021%
66	11.384	3213	3217	3221	rBV	1614	1336	0.16%	0.019%
67	11.561	3261	3272	3292	rBV	474798	742633	86.76%	10.650%
68	11.731	3322	3325	3329	rBV2	1483	1020	0.12%	0.015%
69	12.053	3422	3425	3428	rBV	1214	1139	0.13%	0.016%
70	12.078	3431	3433	3436	rVB	1416	818	0.10%	0.012%
71	12.140	3449	3452	3454	rBV	1175	709	0.08%	0.010%
72	12.371	3522	3524	3526	rBV	1239	716	0.08%	0.010%
73	12.625	3600	3603	3609	rBV2	1588	1706	0.20%	0.024%
74	12.902	3686	3689	3692	rVB	1171	835	0.10%	0.012%
75	12.959	3703	3707	3708	rBV2	1111	864	0.10%	0.012%
76	13.371	3832	3835	3839	rBV	1482	1184	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033197.D
 Acq On : 08 Dec 2023 17:49
 Operator : SY/MD
 Sample : 05689-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GD4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	13.484	3865	3870	3871	rBV2	1854	1508	0.18%	0.022%
78	13.529	3880	3884	3886	rBV	1453	1187	0.14%	0.017%
79	13.564	3891	3895	3898	rBV	1314	1340	0.16%	0.019%
80	13.709	3938	3940	3944	rVB	1428	923	0.11%	0.013%
81	13.982	4023	4025	4029	rBV3	1229	878	0.10%	0.013%
82	14.107	4061	4064	4066	rBV	1190	786	0.09%	0.011%
83	14.197	4089	4092	4094	rBV	1187	770	0.09%	0.011%
84	14.310	4125	4127	4132	rBV	939	720	0.08%	0.010%
85	14.358	4139	4142	4143	rBV3	1474	852	0.10%	0.012%
86	14.590	4211	4214	4218	rBV2	1960	1849	0.22%	0.027%
87	14.718	4251	4254	4258	rVB	1880	1527	0.18%	0.022%
88	14.818	4283	4285	4289	rVB	1470	993	0.12%	0.014%
89	14.966	4328	4331	4334	rBV	1721	950	0.11%	0.014%
90	15.040	4352	4354	4359	rVB	1693	1140	0.13%	0.016%
91	15.069	4359	4363	4369	rVB	1709	1826	0.21%	0.026%
92	15.098	4369	4372	4374	rBV3	1600	1072	0.13%	0.015%
93	15.236	4412	4415	4417	rBV3	1552	1036	0.12%	0.015%
94	15.297	4431	4434	4437	rVB	1787	1263	0.15%	0.018%
95	15.416	4468	4471	4473	rBV2	1448	1042	0.12%	0.015%
96	15.583	4520	4523	4524	rBV	1310	784	0.09%	0.011%
97	15.622	4532	4535	4537	rBV	1658	828	0.10%	0.012%
98	16.046	4664	4667	4669	rBV2	1952	1166	0.14%	0.017%
99	16.123	4687	4691	4694	rBV4	1938	1769	0.21%	0.025%
100	16.599	4834	4839	4843	rBV5	2750	3220	0.38%	0.046%




Sum of corrected areas: 6973023

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033197.D
Acq On : 08 Dec 2023 17:49
Operator : SY/MD
Sample : 05689-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

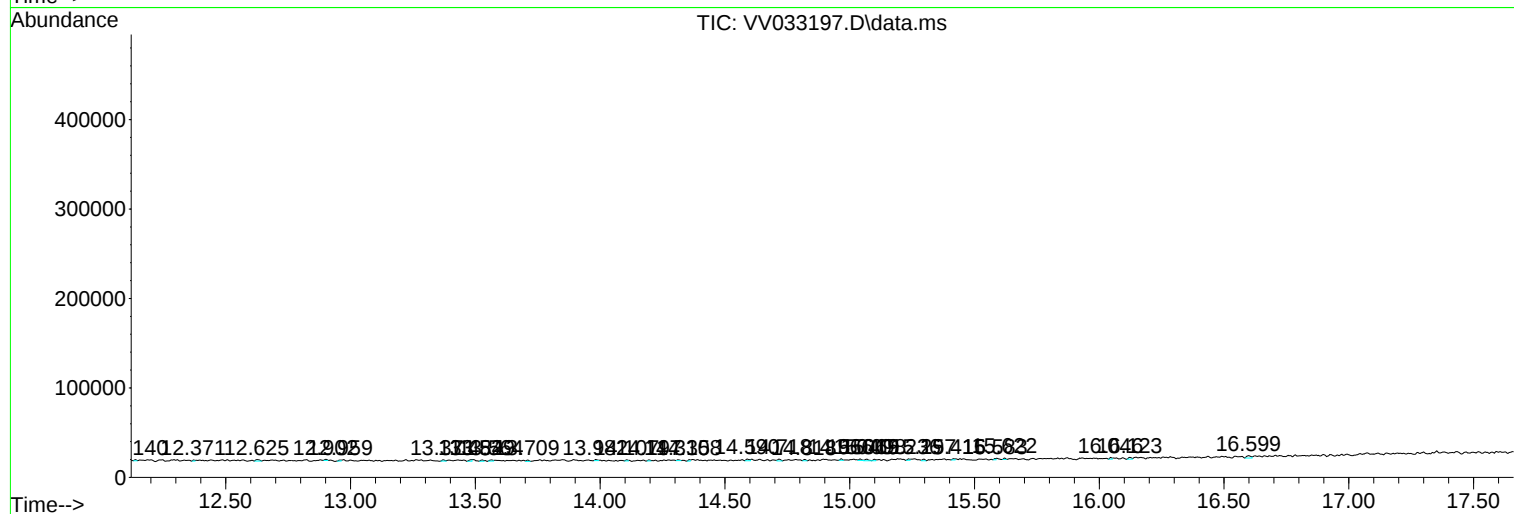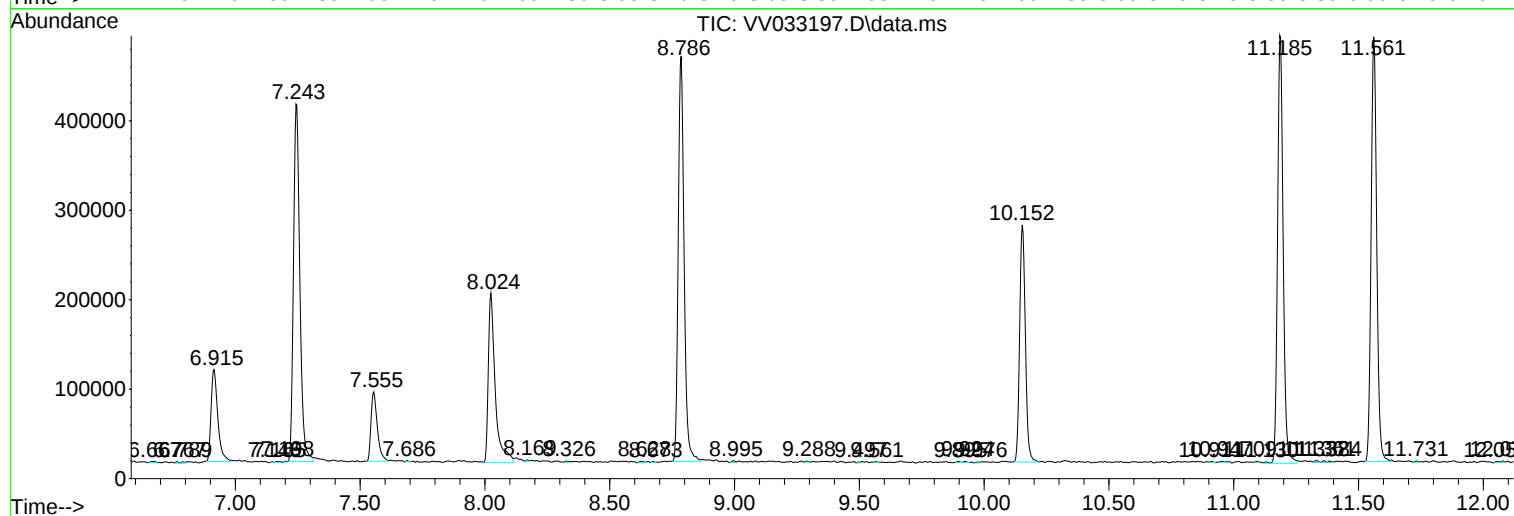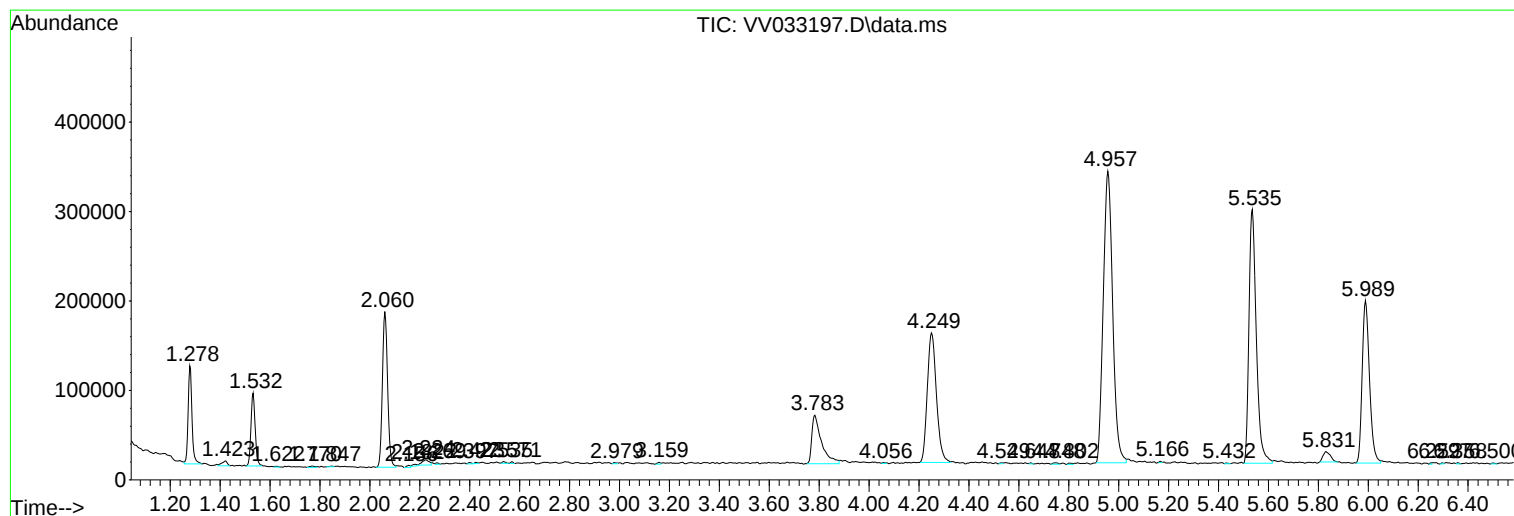

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033197.D
Acq On : 08 Dec 2023 17:49
Operator : SY/MD
Sample : 05689-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033197.D
Acq On : 08 Dec 2023 17:49
Operator : SY/MD
Sample : 05689-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc