

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033198.D
 Acq On : 08 Dec 2023 18:12
 Operator : SY/MD
 Sample : 05689-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

Signal : TIC: VV033198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	102601	110036	12.85%	1.586%
2	1.384	105	107	110	rBV	1334	891	0.10%	0.013%
3	1.420	113	118	127	rVB2	5554	7241	0.85%	0.104%
4	1.458	128	130	134	rBV	908	784	0.09%	0.011%
5	1.494	139	141	145	rVB2	1162	846	0.10%	0.012%
6	1.532	145	153	167	rBV	78554	95195	11.12%	1.372%
7	1.613	176	178	183	rVB	1355	943	0.11%	0.014%
8	1.635	183	185	189	rVB2	1026	583	0.07%	0.008%
9	1.661	189	193	196	rBV	977	878	0.10%	0.013%
10	1.709	205	208	212	rBV	1143	980	0.11%	0.014%
11	1.732	212	215	217	rVV	603	373	0.04%	0.005%
12	1.764	222	225	228	rVV2	1571	1050	0.12%	0.015%
13	1.790	228	233	235	rVV3	1213	951	0.11%	0.014%
14	1.831	243	246	250	rBV2	538	326	0.04%	0.005%
15	1.883	256	262	264	rBV	1413	1290	0.15%	0.019%
16	1.934	276	278	284	rVB	1350	1049	0.12%	0.015%
17	1.976	288	291	296	rBV3	837	644	0.08%	0.009%
18	1.999	296	298	304	rVB	977	664	0.08%	0.010%
19	2.060	304	317	329	rBV	167526	246601	28.80%	3.554%
20	2.130	335	339	342	rVB3	1110	649	0.08%	0.009%
21	2.163	342	349	356	rBV	3024	5937	0.69%	0.086%
22	2.220	357	367	371	rBV2	6295	10238	1.20%	0.148%
23	2.301	389	392	395	rBV3	1565	1143	0.13%	0.016%
24	2.436	427	434	442	rBV	2438	4529	0.53%	0.065%
25	2.873	565	570	574	rBV2	1229	1600	0.19%	0.023%
26	3.111	641	644	653	rVB	1756	2400	0.28%	0.035%
27	3.150	653	656	659	rBV	1562	1238	0.14%	0.018%
28	3.246	684	686	692	rVB	2279	2081	0.24%	0.030%
29	3.275	692	695	696	rBV	1335	781	0.09%	0.011%
30	3.494	761	763	767	rVB2	1160	629	0.07%	0.009%
31	3.629	802	805	811	rBV	1148	1123	0.13%	0.016%
32	3.783	844	853	881	rBV	55234	145386	16.98%	2.096%
33	4.098	947	951	952	rBV	1440	1002	0.12%	0.014%
34	4.249	983	998	1021	rBV	144427	376749	44.01%	5.430%
35	4.410	1046	1048	1055	rVB2	1482	1129	0.13%	0.016%
36	4.548	1089	1091	1098	rBV	1204	990	0.12%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120823\
 Data File : VW033198.D
 Acq On : 08 Dec 2023 18:12
 Operator : SY/MD
 Sample : 05689-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

37	4.674	1127	1130	1136	rBV3	1365	1625	0.19%	0.023%
38	4.857	1184	1187	1191	rVB	1762	1409	0.16%	0.020%
39	4.957	1202	1218	1248	rBV2	318635	856139	100.00%	12.340%
40	5.207	1294	1296	1299	rBV	1257	752	0.09%	0.011%
41	5.259	1307	1312	1318	rBV2	1704	2121	0.25%	0.031%
42	5.384	1348	1351	1359	rBV2	1744	2970	0.35%	0.043%
43	5.535	1387	1398	1421	rBV	274525	565974	66.11%	8.158%
44	5.834	1480	1491	1506	rVB4	11607	27436	3.20%	0.395%
45	5.989	1527	1539	1560	rBV	178493	366761	42.84%	5.286%
46	6.272	1624	1627	1634	rBV	1650	1766	0.21%	0.025%
47	6.317	1638	1641	1643	rBV	1241	975	0.11%	0.014%
48	6.413	1668	1671	1675	rVB	2149	1652	0.19%	0.024%
49	6.455	1681	1684	1690	rVB	2077	2210	0.26%	0.032%
50	6.854	1802	1808	1809	rBV	1495	1545	0.18%	0.022%
51	6.915	1817	1827	1847	rBV	103766	191681	22.39%	2.763%
52	6.998	1851	1853	1861	rVB2	1354	1280	0.15%	0.018%
53	7.069	1873	1875	1876	rBV2	1087	498	0.06%	0.007%
54	7.162	1901	1904	1907	rBV2	1416	880	0.10%	0.013%
55	7.246	1918	1930	1952	rBV	387358	697638	81.49%	10.056%
56	7.429	1984	1987	1988	rBV3	1482	900	0.11%	0.013%
57	7.555	2015	2026	2047	rBV2	78923	145324	16.97%	2.095%
58	7.886	2126	2129	2133	rBV2	1460	1305	0.15%	0.019%
59	7.908	2133	2136	2137	rBV3	1367	798	0.09%	0.012%
60	8.024	2163	2172	2208	rBV	192627	370809	43.31%	5.345%
61	8.506	2320	2322	2325	rBV	1327	744	0.09%	0.011%
62	8.574	2340	2343	2346	rBV	1609	1243	0.15%	0.018%
63	8.696	2378	2381	2384	rBV2	1701	1380	0.16%	0.020%
64	8.786	2398	2409	2428	rBV	442282	729497	85.21%	10.515%
65	8.944	2455	2458	2460	rBV2	1615	1077	0.13%	0.016%
66	8.989	2469	2472	2475	rBV	1702	1148	0.13%	0.017%
67	9.201	2535	2538	2541	rVB2	2202	1327	0.15%	0.019%
68	9.455	2615	2617	2621	rVB2	1175	717	0.08%	0.010%
69	9.477	2621	2624	2630	rBV2	1522	1548	0.18%	0.022%
70	9.612	2662	2666	2668	rBV	1946	1364	0.16%	0.020%
71	9.657	2678	2680	2683	rVB	1255	626	0.07%	0.009%
72	9.696	2689	2692	2694	rBV	1339	907	0.11%	0.013%
73	10.011	2786	2790	2794	rBV	1841	1948	0.23%	0.028%
74	10.040	2795	2799	2809	rVB2	1889	3195	0.37%	0.046%
75	10.079	2809	2811	2814	rBV	1207	624	0.07%	0.009%
76	10.153	2823	2834	2849	rBV	269840	419382	48.99%	6.045%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
 Data File : VV033198.D
 Acq On : 08 Dec 2023 18:12
 Operator : SY/MD
 Sample : 05689-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GD6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
 Title : VOC Analysis

77	10.333	2887	2890	2898	rVB2	1722	1878	0.22%	0.027%
78	10.464	2929	2931	2933	rBV	1000	486	0.06%	0.007%
79	10.792	3030	3033	3038	rBV	1881	1464	0.17%	0.021%
80	10.908	3066	3069	3071	rBV	1106	775	0.09%	0.011%
81	10.985	3091	3093	3095	rBV2	1062	539	0.06%	0.008%
82	11.053	3110	3114	3117	rBV	2040	1676	0.20%	0.024%
83	11.098	3125	3128	3132	rBV2	1267	1254	0.15%	0.018%
84	11.185	3144	3155	3175	rBV	465394	733762	85.71%	10.576%
85	11.561	3261	3272	3295	rBV	469349	735478	85.91%	10.601%
86	11.972	3398	3400	3404	rVB	2164	1465	0.17%	0.021%
87	12.178	3461	3464	3466	rBV	1466	952	0.11%	0.014%
88	12.603	3594	3596	3598	rBV	820	346	0.04%	0.005%
89	12.725	3631	3634	3643	rBV	1695	2048	0.24%	0.030%
90	13.326	3818	3821	3824	rVB2	1779	1201	0.14%	0.017%
91	13.532	3882	3885	3889	rBV2	1466	1055	0.12%	0.015%
92	13.850	3982	3984	3989	rVB	1678	1226	0.14%	0.018%
93	14.062	4047	4050	4056	rBV	1781	1930	0.23%	0.028%
94	14.191	4084	4090	4094	rVB2	1514	1667	0.19%	0.024%
95	14.458	4170	4173	4175	rBV	1485	774	0.09%	0.011%
96	14.632	4222	4227	4230	rBV	2016	2087	0.24%	0.030%
97	14.821	4283	4286	4289	rBV2	1283	1120	0.13%	0.016%
98	15.403	4465	4467	4471	rVB4	1560	767	0.09%	0.011%
99	15.590	4523	4525	4529	rBV2	1864	1484	0.17%	0.021%
100	16.596	4833	4838	4839	rBV	2485	2242	0.26%	0.032%




Sum of corrected areas: 6937780

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033198.D
Acq On : 08 Dec 2023 18:12
Operator : SY/MD
Sample : 05689-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

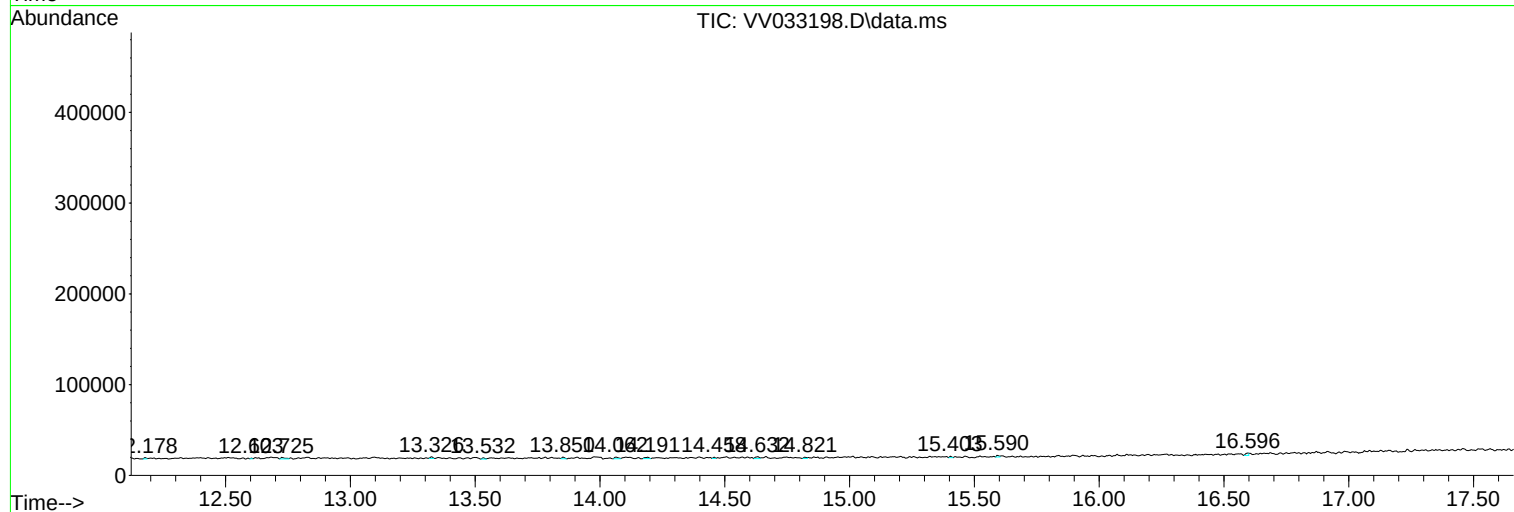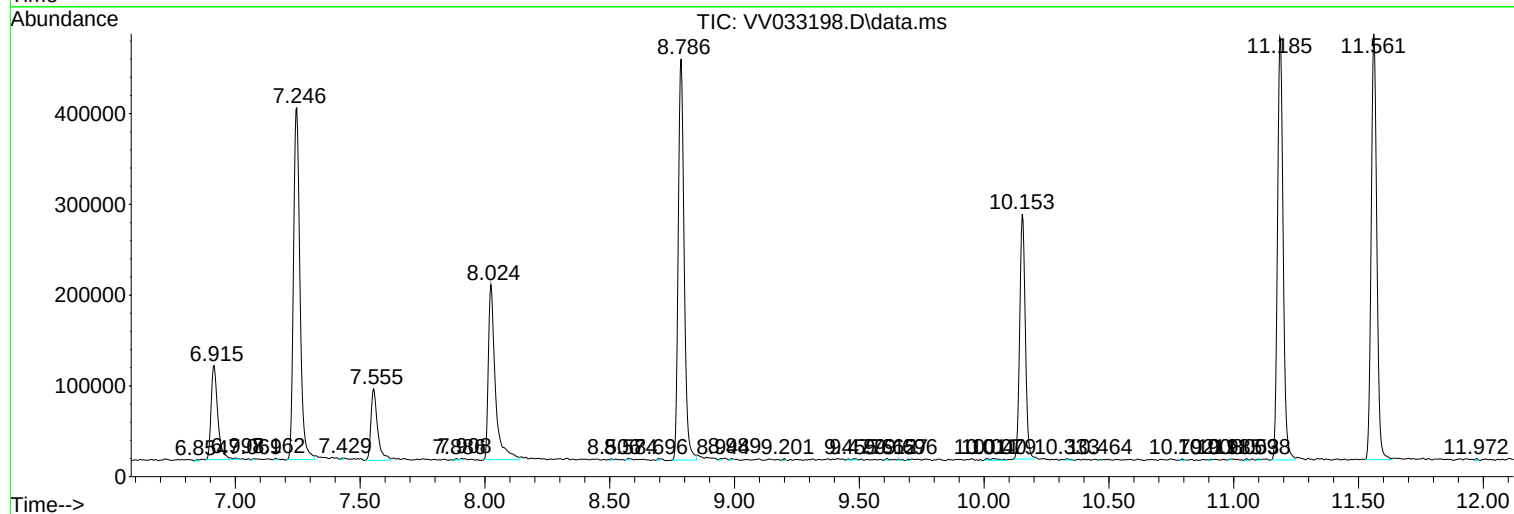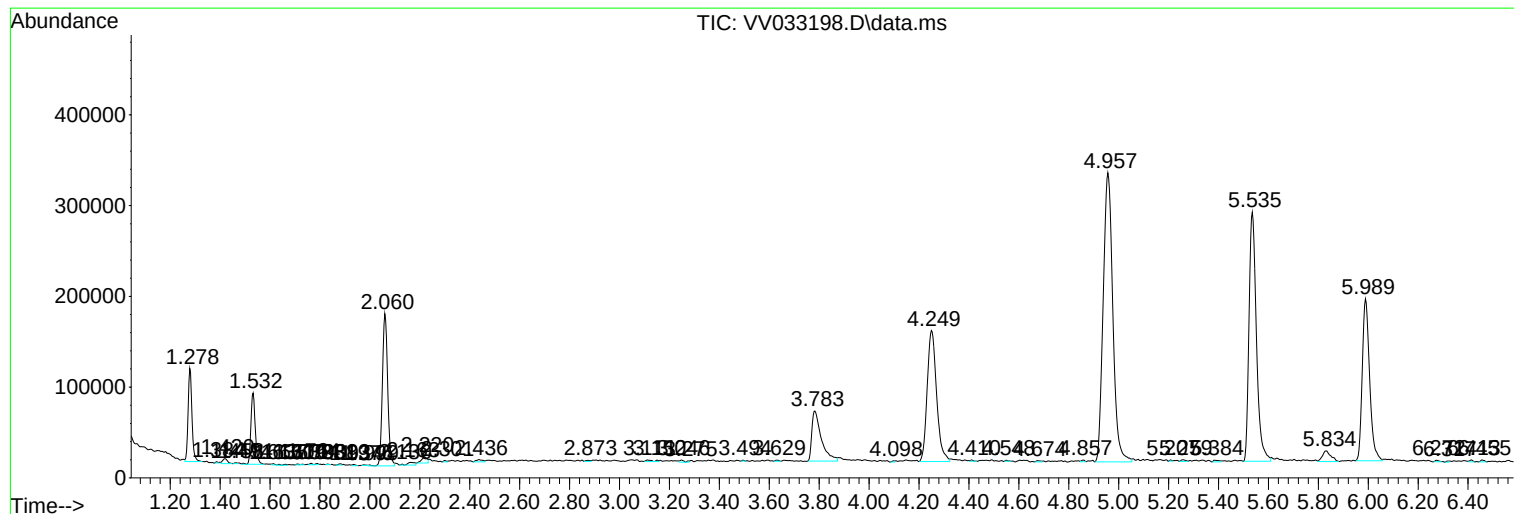

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033198.D
Acq On : 08 Dec 2023 18:12
Operator : SY/MD
Sample : 05689-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120823\
Data File : VV033198.D
Acq On : 08 Dec 2023 18:12
Operator : SY/MD
Sample : 05689-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GD6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc