




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120825\
Data File : VV039494.D
Acq On : 08 Dec 2025 15:41
Operator : SY/MD
Sample : Q3787-05MS
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-15B-42.5-120425-SIMMS

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 09 01:28:11 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

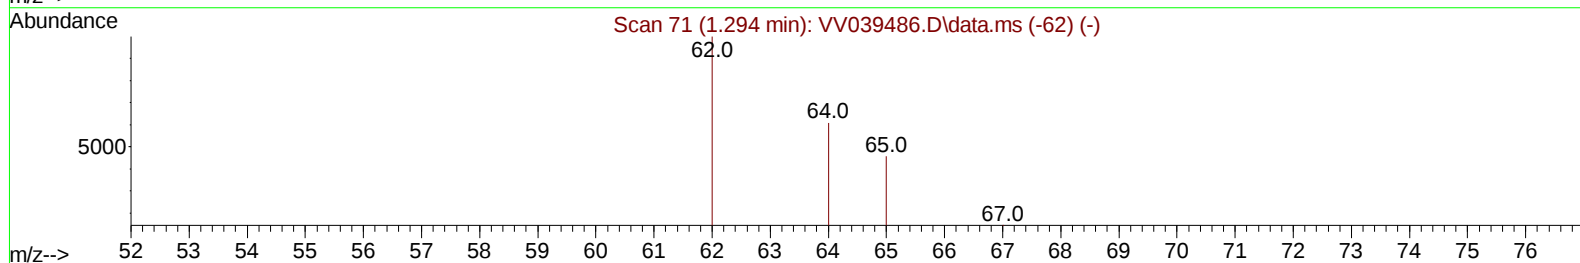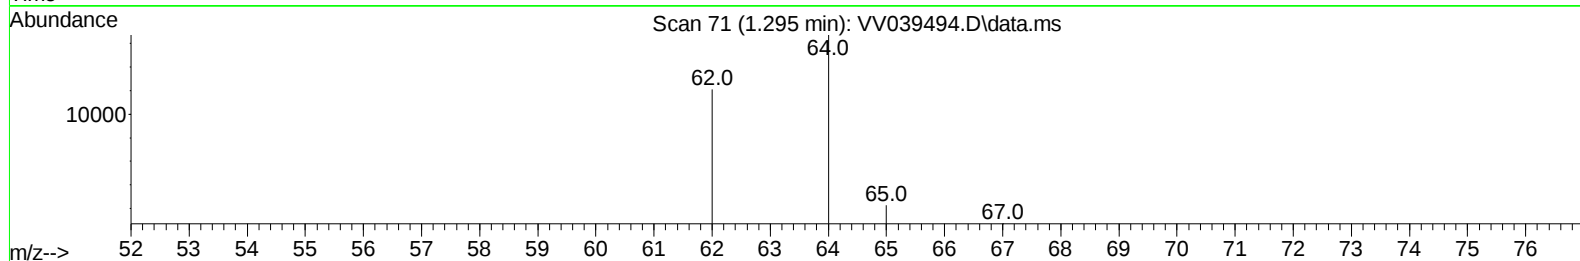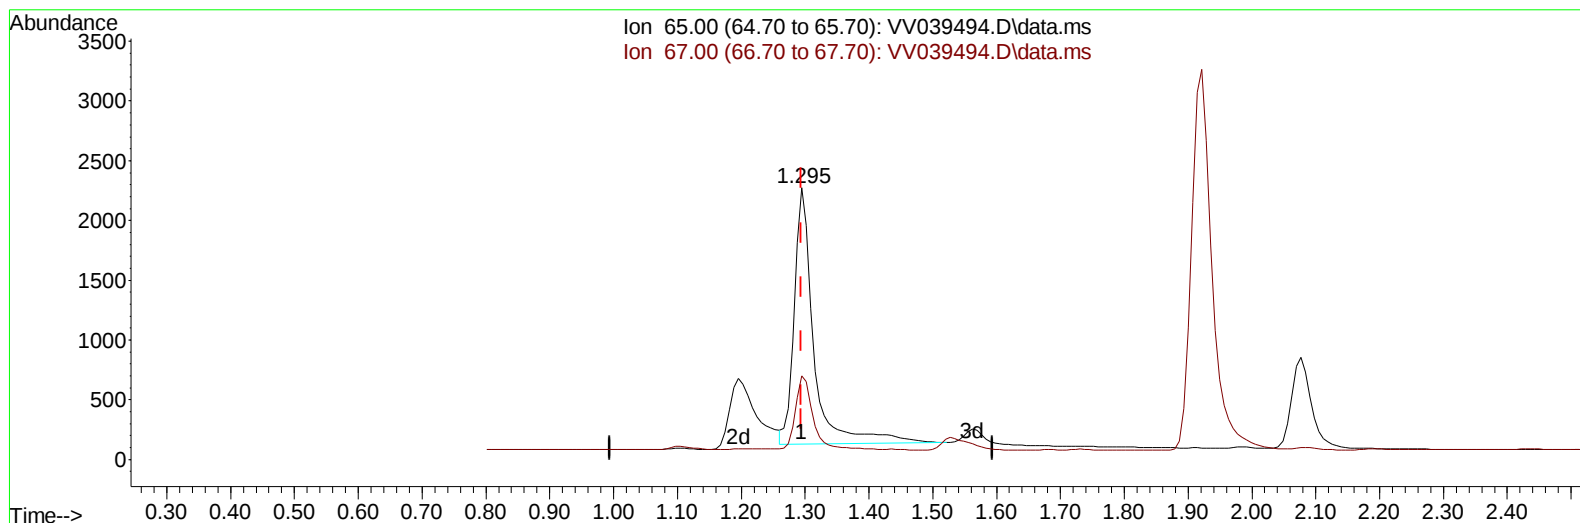

TIC: VV039494.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.295min (+ 0.001) 0.64 ug/L

response 4591

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	25.22
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120825\
Data File : VV039494.D
Acq On : 08 Dec 2025 15:41
Operator : SY/MD
Sample : Q3787-05MS
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-15B-42.5-120425-SIMMS

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 09 01:28:11 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

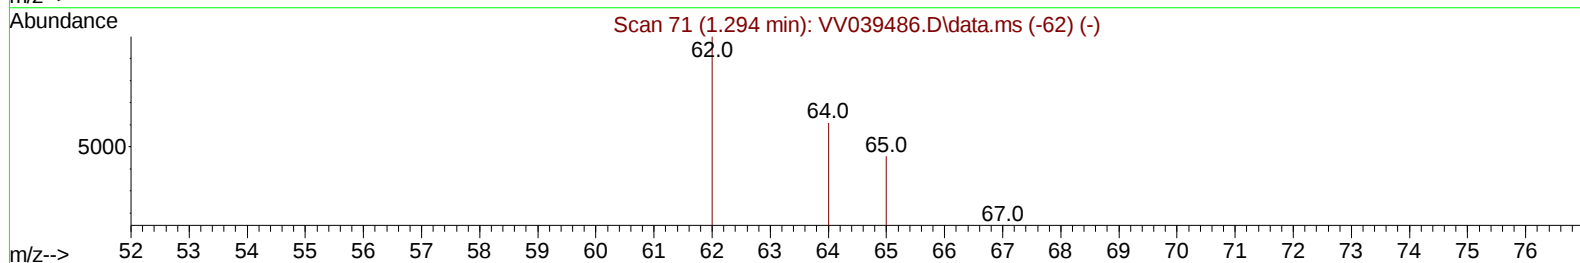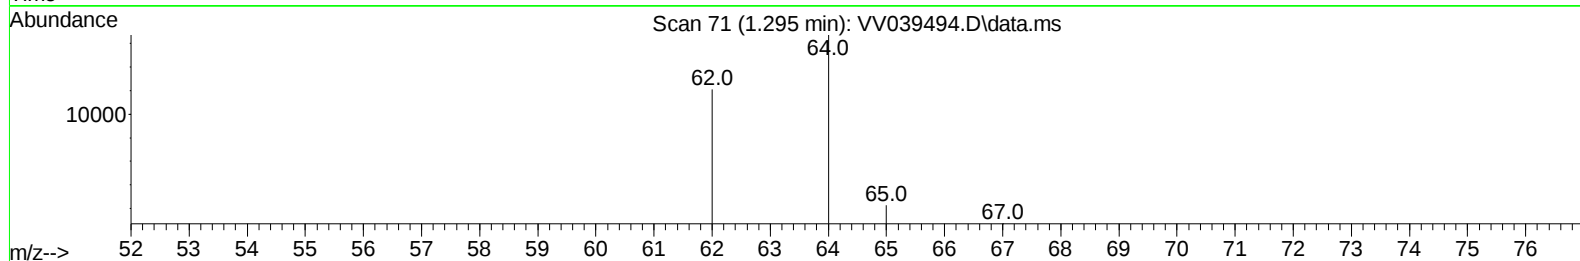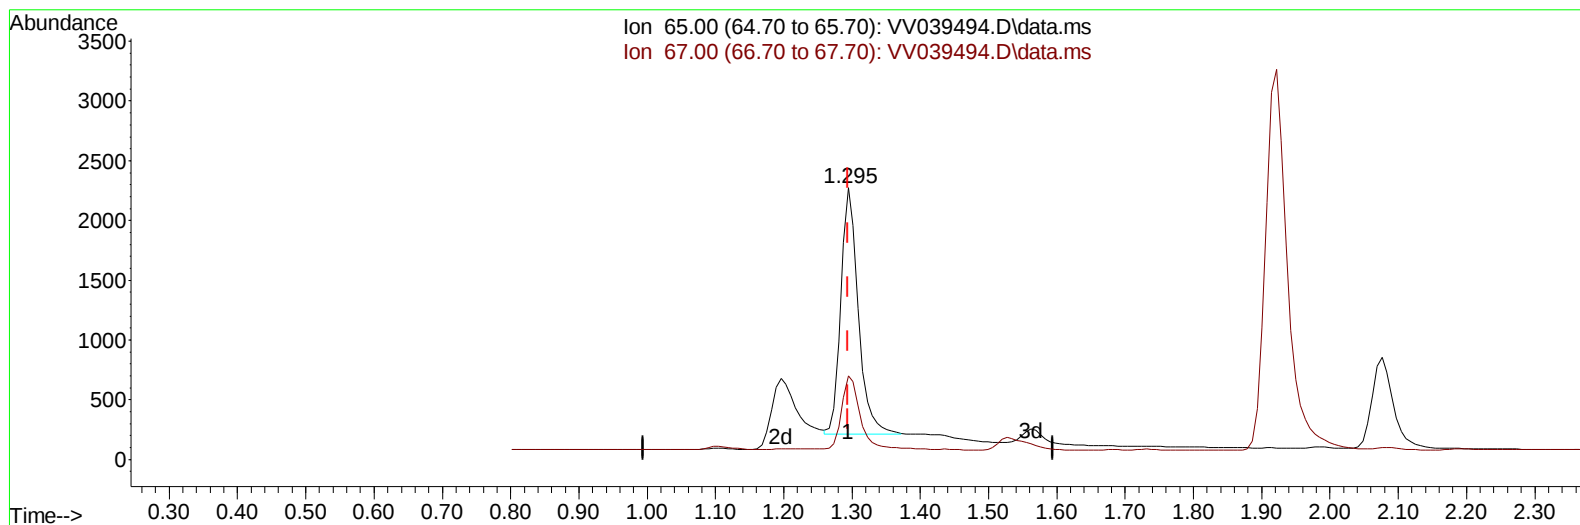

TIC: VV039494.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.295min (+ 0.001) 0.51 ug/L m

response 3660

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.90	31.64
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120825\
 Data File : VV039494.D
 Acq On : 08 Dec 2025 15:41
 Operator : SY/MD
 Sample : Q3787-05MS
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MW-15B-42.5-120425-SIMMS

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
 Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 09 01:28:11 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 04 00:58:46 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	7180	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.785	117	7469	0.500	ug/L	0.00
12) 1,4-Dichlorobenzene-d4	11.175	152	4203	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.295	65	3660m	0.507	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery =	102.000%		
4) 1,2-Dichloroethane-d4	4.970	65	2351	0.492	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery =	98.000%		
7) 1,2-Dichloropropane-d6	6.020	67	3440	0.546	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery =	110.000%		
8) Toluene-d8	7.254	98	5395	0.507	ug/L	0.02
Spiked Amount 0.500	Range 70 - 130		Recovery =	102.000%		
10) 1,1,2,2-Tetrachloroeth...	10.133	84	1962	0.552	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery =	110.000%		
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.295	62	21343	1.374	ug/L #	1
6) Trichloroethene	5.829	95	60422	6.527	ug/L	97
9) 1,2-Dibromoethane	8.290	107	2997	0.490	ug/L	98
11) 1,1,2,2-Tetrachloroethane	10.155	83	4045	0.540	ug/L	99
13) 1,2,3-Trichloropropane	10.199	75	2266	0.512	ug/L	98
14) 1,2-Dibromo-3-chloropr...	12.351	75	443	0.495	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120825\
Data File : VV039494.D
Acq On : 08 Dec 2025 15:41
Operator : SY/MD
Sample : Q3787-05MS
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MW-15B-42.5-120425-SIMMS

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 12/10/2025
Supervised By :Mahesh Dadoda 12/10/2025

Quant Time: Dec 09 01:28:11 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120325MA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 04 00:58:46 2025
Response via : Initial Calibration

