

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013953.D
 Acq On : 09 Dec 2019 11:10
 Operator : SY/MD
 Sample : VV1209WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	65	70	81	rVB	299655	291471	14.19%	1.787%
2	1.557	140	145	157	rVB	290893	329741	16.05%	2.021%
3	2.119	312	320	334	rVB	602926	828314	40.31%	5.078%
4	2.750	514	516	518	rBV3	568	167	0.01%	0.001%
5	2.782	518	526	530	rBV8	2478	3576	0.17%	0.022%
6	2.894	558	561	564	rBV4	1698	1291	0.06%	0.008%
7	2.991	589	591	594	rBV3	1158	766	0.04%	0.005%
8	3.036	602	605	608	rBV3	1153	754	0.04%	0.005%
9	3.097	620	624	627	rBV5	770	690	0.03%	0.004%
10	3.135	634	636	638	rBV3	1306	687	0.03%	0.004%
11	3.171	644	647	651	rBV6	1397	866	0.04%	0.005%
12	3.222	661	663	666	rBV2	981	498	0.02%	0.003%
13	3.258	671	674	676	rBV4	1018	591	0.03%	0.004%
14	3.287	682	683	684	rBV	969	230	0.01%	0.001%
15	3.351	701	703	704	rBV2	982	375	0.02%	0.002%
16	3.425	723	726	729	rBV4	828	671	0.03%	0.004%
17	3.505	750	751	753	rVB	991	293	0.01%	0.002%
18	3.518	753	755	757	rBV2	601	327	0.02%	0.002%
19	3.592	775	778	781	rBV4	1418	1076	0.05%	0.007%
20	3.643	791	794	795	rBV2	564	356	0.02%	0.002%
21	3.679	802	805	808	rBV3	1579	1041	0.05%	0.006%
22	3.708	812	814	816	rVV3	1157	680	0.03%	0.004%
23	3.730	819	821	822	rBV	728	220	0.01%	0.001%
24	3.743	822	825	826	rBV2	790	376	0.02%	0.002%
25	3.759	828	830	833	rVB2	1177	542	0.03%	0.003%
26	3.920	869	880	911	rBV	147072	403585	19.64%	2.474%
27	4.389	1012	1026	1048	rBV	342015	818705	39.84%	5.019%
28	4.785	1147	1149	1155	rVB5	1008	725	0.04%	0.004%
29	4.859	1168	1172	1175	rBV5	1396	1065	0.05%	0.007%
30	4.907	1183	1187	1190	rBV4	1518	1180	0.06%	0.007%
31	4.923	1190	1192	1197	rVV4	1335	1077	0.05%	0.007%
32	4.968	1202	1206	1208	rBV3	918	793	0.04%	0.005%
33	5.087	1225	1243	1269	rBV2	820594	2054730	100.00%	12.596%
34	5.656	1405	1420	1444	rBV	737772	1462921	71.20%	8.968%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013953.D
 Acq On : 09 Dec 2019 11:10
 Operator : SY/MD
 Sample : VV1209WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	5.939	1497	1508	1523	rBV2	50757	105085	5.11%	0.644%
36	6.110	1546	1561	1582	rBV	465368	932693	45.39%	5.717%
37	6.386	1644	1647	1652	rBV5	1542	1693	0.08%	0.010%
38	6.438	1661	1663	1667	rBV5	1403	1026	0.05%	0.006%
39	6.473	1671	1674	1679	rBV7	1331	1347	0.07%	0.008%
40	6.518	1686	1688	1690	rBV4	1183	482	0.02%	0.003%
41	6.556	1699	1700	1703	rBV	977	396	0.02%	0.002%
42	6.634	1721	1724	1725	rBV3	2209	1182	0.06%	0.007%
43	6.846	1788	1790	1791	rVB2	676	174	0.01%	0.001%
44	6.891	1802	1804	1807	rVB4	1246	697	0.03%	0.004%
45	6.936	1815	1818	1822	rVB5	1504	1008	0.05%	0.006%
46	6.974	1827	1830	1831	rBV2	1113	560	0.03%	0.003%
47	7.023	1833	1845	1863	rBV	240762	432143	21.03%	2.649%
48	7.354	1935	1948	1971	rBV	935807	1632393	79.45%	10.007%
49	7.656	2032	2042	2058	rBV	169753	289660	14.10%	1.776%
50	8.129	2178	2189	2222	rBV2	415520	922768	44.91%	5.657%
51	8.550	2317	2320	2321	rBV3	1641	810	0.04%	0.005%
52	8.614	2337	2340	2343	rBV2	1314	879	0.04%	0.005%
53	8.630	2343	2345	2347	rBV3	1683	1097	0.05%	0.007%
54	8.691	2360	2364	2368	rBV6	1615	1557	0.08%	0.010%
55	8.794	2395	2396	2399	rBV3	690	462	0.02%	0.003%
56	8.891	2414	2426	2451	rBV	1115876	1780240	86.64%	10.913%
57	9.286	2547	2549	2552	rVB3	1477	598	0.03%	0.004%
58	9.380	2576	2578	2580	rBV3	701	315	0.02%	0.002%
59	9.392	2580	2582	2584	rBV2	1309	645	0.03%	0.004%
60	9.447	2595	2599	2602	rBV4	633	524	0.03%	0.003%
61	9.463	2602	2604	2606	rBV3	874	364	0.02%	0.002%
62	9.515	2618	2620	2623	rVB2	931	295	0.01%	0.002%
63	9.537	2623	2627	2631	rBV6	1533	1511	0.07%	0.009%
64	9.572	2636	2638	2639	rBV2	1514	725	0.04%	0.004%
65	9.707	2678	2680	2682	rBV3	1111	508	0.02%	0.003%
66	9.785	2702	2704	2706	rBV3	1038	435	0.02%	0.003%
67	9.920	2744	2746	2749	rBV3	704	277	0.01%	0.002%
68	9.971	2759	2762	2763	rBV3	1614	939	0.05%	0.006%
69	10.010	2770	2774	2776	rBV4	1496	1226	0.06%	0.008%
70	10.254	2838	2850	2866	rBV	585675	924388	44.99%	5.667%
71	10.405	2894	2897	2898	rBV2	1646	1073	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013953.D
 Acq On : 09 Dec 2019 11:10
 Operator : SY/MD
 Sample : VV1209WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK87

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.550	2941	2942	2945	rBV2	834	434	0.02%	0.003%
73	10.566	2945	2947	2948	rBV2	1397	611	0.03%	0.004%
74	10.820	3021	3026	3028	rBV5	1365	1300	0.06%	0.008%
75	10.920	3054	3057	3060	rBV3	1028	597	0.03%	0.004%
76	10.955	3065	3068	3069	rBV2	1862	1179	0.06%	0.007%
77	11.023	3083	3089	3090	rBV5	1216	937	0.05%	0.006%
78	11.055	3097	3099	3101	rBV2	2064	1194	0.06%	0.007%
79	11.087	3105	3109	3111	rVV3	1244	986	0.05%	0.006%
80	11.174	3132	3136	3138	rBV4	1278	894	0.04%	0.005%
81	11.225	3145	3152	3159	rBV10	4920	8369	0.41%	0.051%
82	11.289	3160	3172	3193	rBV	1001619	1535048	74.71%	9.410%
83	11.666	3277	3289	3319	rBV	921143	1480932	72.07%	9.078%
84	12.029	3398	3402	3404	rBV4	1161	764	0.04%	0.005%
85	12.392	3512	3515	3519	rBV4	2353	1841	0.09%	0.011%
86	12.482	3541	3543	3546	rVB4	1342	685	0.03%	0.004%
87	12.958	3689	3691	3694	rBV4	1305	745	0.04%	0.005%
88	13.170	3755	3757	3758	rBV	723	314	0.02%	0.002%
89	13.257	3782	3784	3787	rBV2	1772	931	0.05%	0.006%
90	13.550	3869	3875	3885	rBV2	13272	21842	1.06%	0.134%
91	14.055	4028	4032	4033	rBV4	1277	878	0.04%	0.005%


Sum of corrected areas: 16313036

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120919\
Data File : VV013953.D
Acq On : 09 Dec 2019 11:10
Operator : SY/MD
Sample : VV1209WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK87

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

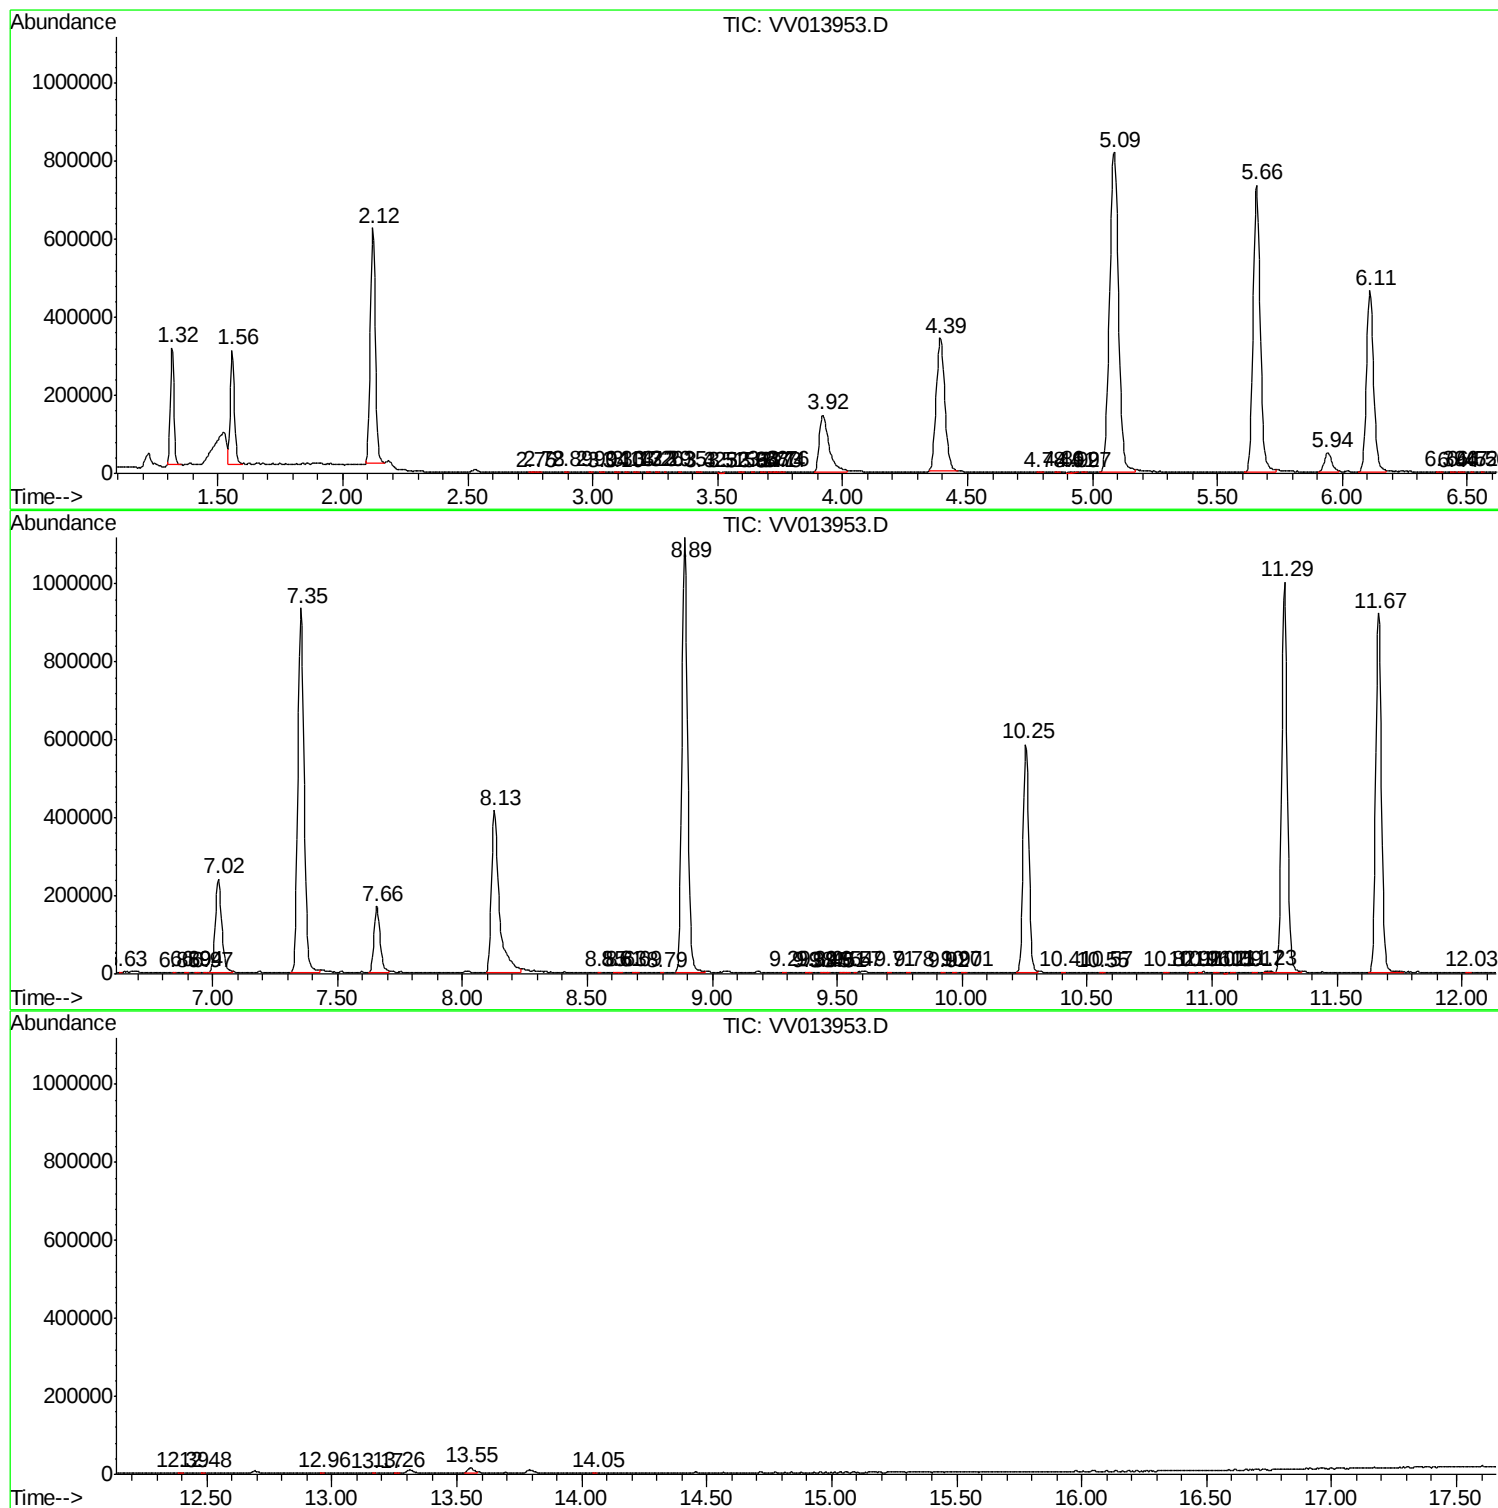

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120919\
Data File : VV013953.D
Acq On : 09 Dec 2019 11:10
Operator : SY/MD
Sample : VV1209WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK87

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120919\
Data File : VV013953.D
Acq On : 09 Dec 2019 11:10
Operator : SY/MD
Sample : VV1209WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK87

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc