

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013964.D
 Acq On : 09 Dec 2019 15:45
 Operator : SY/MD
 Sample : K6148-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.318	65	71	86	rVB	294653	283854	13.26%	1.731%
2	1.572	144	150	161	rVB	299142	346891	16.21%	2.116%
3	2.129	314	323	335	rVB	601346	827884	38.69%	5.049%
4	2.646	478	484	487	rBV8	3276	4052	0.19%	0.025%
5	2.711	501	504	507	rBV4	1595	1021	0.05%	0.006%
6	2.772	519	523	526	rBV4	1583	1601	0.07%	0.010%
7	2.810	533	535	538	rBV4	972	471	0.02%	0.003%
8	2.852	544	548	551	rBV3	2208	2045	0.10%	0.012%
9	2.913	565	567	568	rBV2	735	182	0.01%	0.001%
10	2.955	577	580	584	rVB4	2380	1844	0.09%	0.011%
11	2.994	587	592	593	rBV3	1150	918	0.04%	0.006%
12	3.016	597	599	601	rVV2	1018	457	0.02%	0.003%
13	3.116	628	630	632	rBV3	942	444	0.02%	0.003%
14	3.138	635	637	638	rBV2	877	327	0.02%	0.002%
15	3.148	638	640	644	rBV4	1215	920	0.04%	0.006%
16	3.270	674	678	681	rBV4	961	918	0.04%	0.006%
17	3.286	681	683	688	rVV4	583	473	0.02%	0.003%
18	3.354	699	704	708	rBV6	1222	1202	0.06%	0.007%
19	3.386	713	714	716	rBV	570	147	0.01%	0.001%
20	3.399	716	718	719	rBV	752	227	0.01%	0.001%
21	3.408	719	721	722	rVV2	874	275	0.01%	0.002%
22	3.418	722	724	727	rVB3	1052	517	0.02%	0.003%
23	3.441	727	731	732	rBV2	865	543	0.03%	0.003%
24	3.450	732	734	738	rVB3	1258	786	0.04%	0.005%
25	3.473	739	741	743	rVB3	926	343	0.02%	0.002%
26	3.537	754	761	764	rBV6	1118	1334	0.06%	0.008%
27	3.595	775	779	780	rBV3	874	505	0.02%	0.003%
28	3.640	790	793	796	rVB3	1092	773	0.04%	0.005%
29	3.656	796	798	801	rBV2	1075	810	0.04%	0.005%
30	3.698	804	811	813	rBV6	981	1043	0.05%	0.006%
31	3.711	813	815	816	rBV2	549	189	0.01%	0.001%
32	3.740	821	824	826	rBV5	575	357	0.02%	0.002%
33	3.775	833	835	838	rVB3	611	330	0.02%	0.002%
34	3.794	838	841	844	rBV3	691	536	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013964.D
 Acq On : 09 Dec 2019 15:45
 Operator : SY/MD
 Sample : K6148-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	3.830	851	852	856	rVB4	1226	629	0.03%	0.004%
36	3.852	856	859	862	rBV3	1097	959	0.04%	0.006%
37	3.920	869	880	913	rBV	160620	427890	19.99%	2.610%
38	4.396	1014	1028	1051	rVB2	360379	846245	39.54%	5.161%
39	4.772	1142	1145	1146	rBV2	787	441	0.02%	0.003%
40	4.801	1152	1154	1155	rBV	1033	461	0.02%	0.003%
41	4.878	1176	1178	1180	rBV3	1303	508	0.02%	0.003%
42	4.910	1185	1188	1191	rBV3	1471	895	0.04%	0.005%
43	4.932	1193	1195	1202	rBV6	1042	906	0.04%	0.006%
44	4.977	1207	1209	1214	rVB4	1210	847	0.04%	0.005%
45	5.010	1217	1219	1222	rVB3	1548	863	0.04%	0.005%
46	5.090	1224	1244	1269	rBV2	847311	2139987	100.00%	13.051%
47	5.492	1366	1369	1373	rBV6	1730	1606	0.08%	0.010%
48	5.585	1396	1398	1399	rBV2	1257	416	0.02%	0.003%
49	5.659	1401	1421	1438	rBV	760357	1566115	73.18%	9.551%
50	6.112	1551	1562	1587	rVB	505781	998984	46.68%	6.092%
51	7.026	1835	1846	1861	rBV	256466	447883	20.93%	2.731%
52	7.357	1935	1949	1969	rBV	932966	1625584	75.96%	9.914%
53	7.659	2034	2043	2062	rVB	173475	290849	13.59%	1.774%
54	8.125	2177	2188	2219	rBV	525120	965788	45.13%	5.890%
55	8.891	2414	2426	2452	rBV	1075557	1746561	81.62%	10.652%
56	9.173	2510	2514	2517	rBV5	2237	2203	0.10%	0.013%
57	9.251	2535	2538	2540	rBV3	1730	1234	0.06%	0.008%
58	9.357	2568	2571	2573	rBV4	1620	993	0.05%	0.006%
59	9.704	2677	2679	2681	rBV3	914	486	0.02%	0.003%
60	9.781	2701	2703	2704	rBV2	759	386	0.02%	0.002%
61	9.810	2710	2712	2713	rBV2	949	420	0.02%	0.003%
62	9.907	2740	2742	2744	rVB3	1110	308	0.01%	0.002%
63	9.968	2759	2761	2762	rBV2	1678	760	0.04%	0.005%
64	9.993	2767	2769	2773	rBV4	1385	1195	0.06%	0.007%
65	10.254	2836	2850	2868	rBV	667535	1053606	49.23%	6.426%
66	10.527	2933	2935	2939	rVB5	1539	819	0.04%	0.005%
67	10.665	2975	2978	2980	rBV3	1068	731	0.03%	0.004%
68	10.878	3041	3044	3045	rBV2	1611	743	0.03%	0.005%
69	11.035	3090	3093	3096	rBV3	1337	781	0.04%	0.005%
70	11.080	3104	3107	3108	rBV3	979	517	0.02%	0.003%
71	11.125	3118	3121	3122	rBV2	1269	806	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013964.D
 Acq On : 09 Dec 2019 15:45
 Operator : SY/MD
 Sample : K6148-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	11.212	3145	3148	3152	rBV5	2065	1821	0.09%	0.011%
73	11.289	3161	3172	3192	rBV	912884	1400981	65.47%	8.544%
74	11.665	3277	3289	3305	rBV	857403	1370454	64.04%	8.358%
75	11.948	3373	3377	3382	rBV7	1586	1541	0.07%	0.009%
76	11.971	3382	3384	3388	rBV4	1038	740	0.03%	0.005%
77	12.064	3411	3413	3416	rBV2	1429	851	0.04%	0.005%
78	12.157	3440	3442	3443	rBV2	1217	547	0.03%	0.003%
79	12.247	3467	3470	3473	rBV5	1583	1120	0.05%	0.007%
80	12.829	3646	3651	3655	rBV6	1715	2006	0.09%	0.012%
81	13.267	3785	3787	3788	rBV	1175	352	0.02%	0.002%
82	13.447	3841	3843	3846	rBV4	1164	765	0.04%	0.005%
83	13.517	3863	3865	3868	rBV4	1203	676	0.03%	0.004%
84	13.871	3973	3975	3976	rBV3	1631	661	0.03%	0.004%


Sum of corrected areas: 16397139

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120919\
Data File : VV013964.D
Acq On : 09 Dec 2019 15:45
Operator : SY/MD
Sample : K6148-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

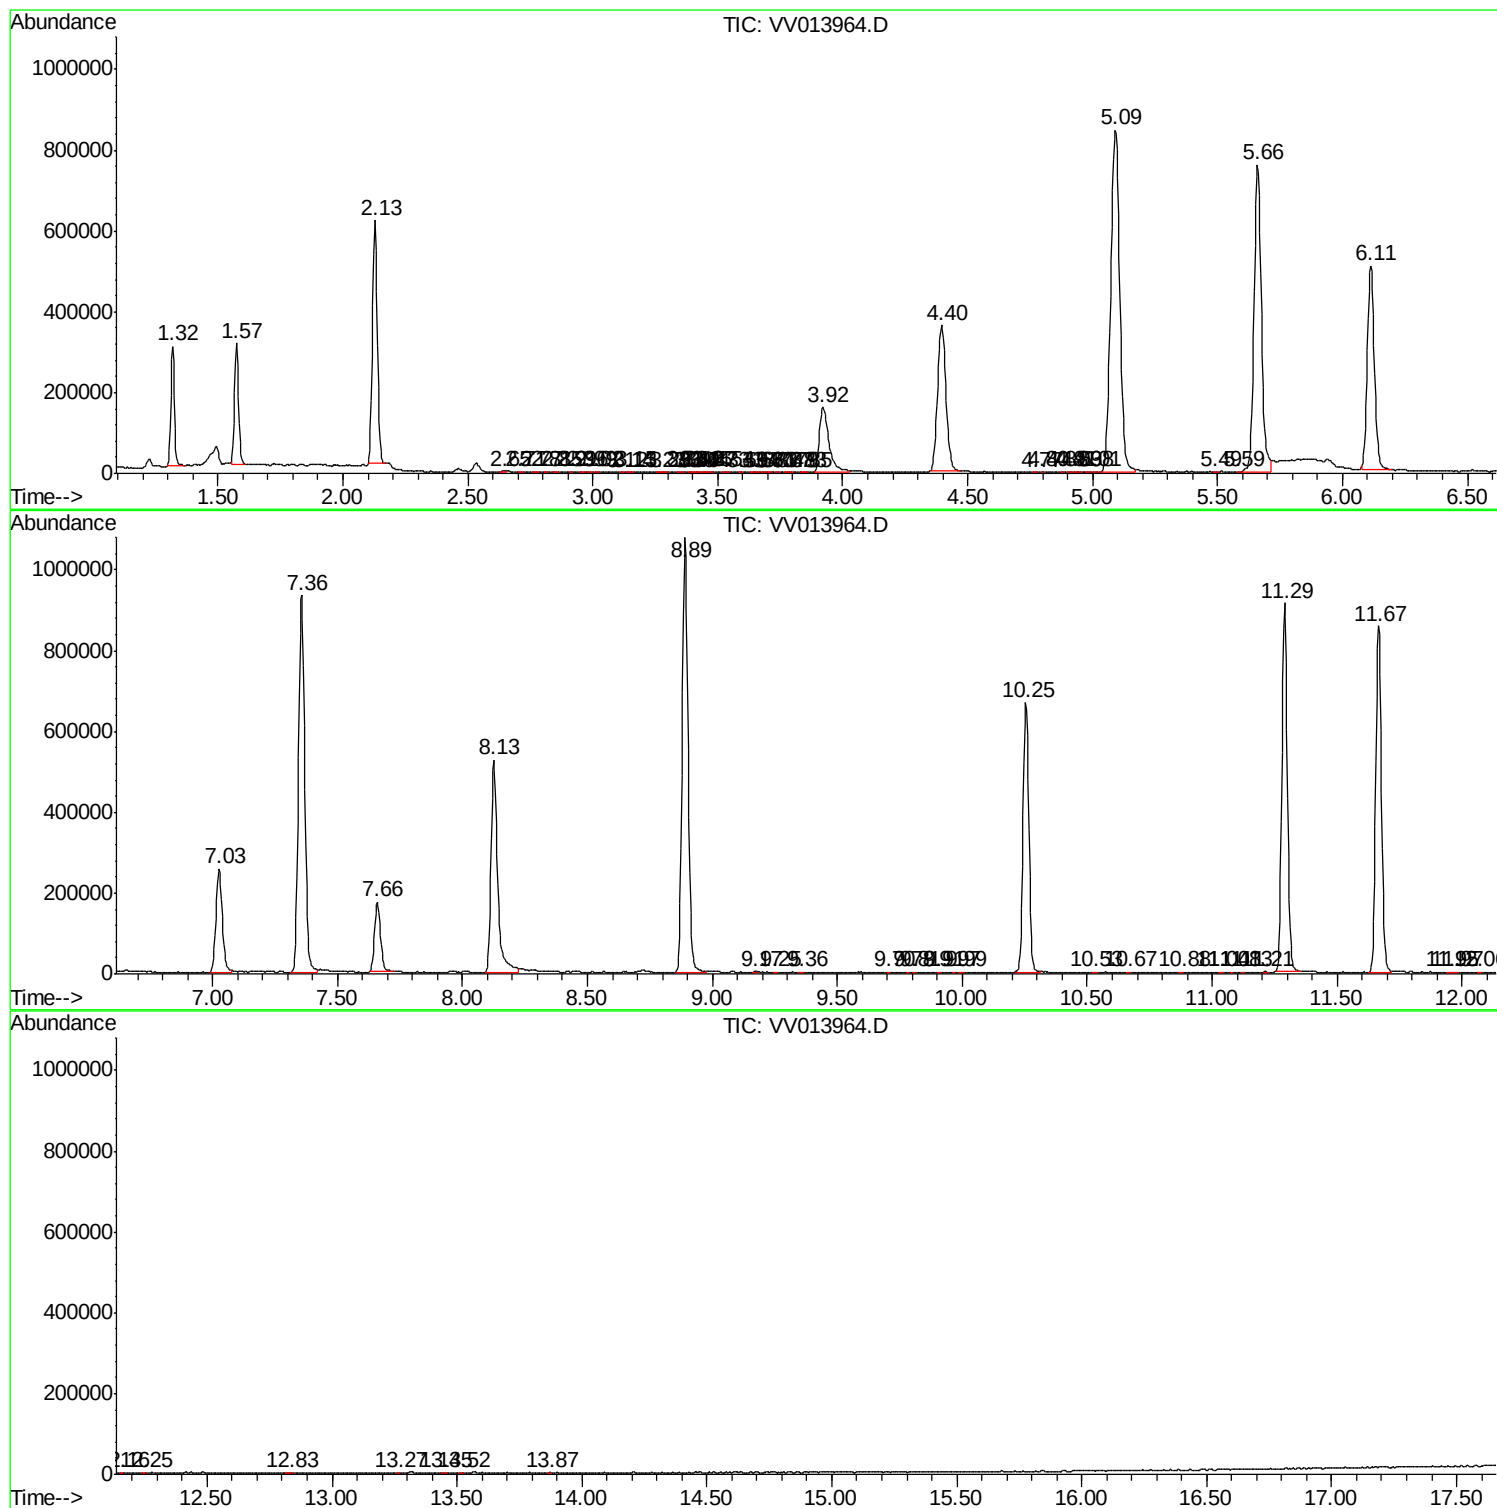

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120919\
Data File : VV013964.D
Acq On : 09 Dec 2019 15:45
Operator : SY/MD
Sample : K6148-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV120919\
Data File : VV013964.D
Acq On : 09 Dec 2019 15:45
Operator : SY/MD
Sample : K6148-01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
DBBL2

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc