

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013968.D
 Acq On : 09 Dec 2019 17:48
 Operator : SY/MD
 Sample : K6148-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBT1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	82	rVB	297842	287851	13.57%	1.750%
2	1.573	144	150	163	rVB	312825	361974	17.07%	2.201%
3	2.126	314	322	339	rVB	588150	842455	39.73%	5.122%
4	2.534	439	449	461	rBV2	34838	58002	2.74%	0.353%
5	2.611	470	473	475	rBV3	1747	918	0.04%	0.006%
6	2.646	479	484	492	rBV4	4354	7007	0.33%	0.043%
7	2.833	540	542	545	rVB4	1325	655	0.03%	0.004%
8	2.846	545	546	549	rBV2	666	256	0.01%	0.002%
9	2.862	549	551	556	rBV5	1131	971	0.05%	0.006%
10	2.913	565	567	568	rVB2	723	160	0.01%	0.001%
11	2.971	581	585	586	rBV2	1299	710	0.03%	0.004%
12	3.097	622	624	627	rBV3	1313	812	0.04%	0.005%
13	3.122	630	632	634	rBV2	946	560	0.03%	0.003%
14	3.177	647	649	654	rBV4	1330	847	0.04%	0.005%
15	3.219	660	662	665	rVB3	842	454	0.02%	0.003%
16	3.244	669	670	671	rBV	1020	234	0.01%	0.001%
17	3.261	671	675	677	rVB3	1633	1067	0.05%	0.006%
18	3.280	677	681	685	rBV6	1473	1318	0.06%	0.008%
19	3.299	685	687	689	rBV3	789	357	0.02%	0.002%
20	3.335	696	698	699	rBV	453	178	0.01%	0.001%
21	3.373	708	710	713	rBV2	770	530	0.02%	0.003%
22	3.421	722	725	727	rBV2	1038	482	0.02%	0.003%
23	3.431	727	728	730	rBV2	911	359	0.02%	0.002%
24	3.444	730	732	733	rVV2	857	400	0.02%	0.002%
25	3.466	737	739	741	rVV3	1564	739	0.03%	0.004%
26	3.489	744	746	750	rVB2	1004	639	0.03%	0.004%
27	3.524	755	757	760	rBV3	854	502	0.02%	0.003%
28	3.540	760	762	764	rVV3	993	449	0.02%	0.003%
29	3.553	764	766	770	rVB4	1217	716	0.03%	0.004%
30	3.598	779	780	782	rBV	542	237	0.01%	0.001%
31	3.611	782	784	789	rVB3	1136	890	0.04%	0.005%
32	3.637	789	792	795	rBV4	534	513	0.02%	0.003%
33	3.656	795	798	801	rVV3	696	519	0.02%	0.003%
34	3.701	810	812	816	rBV5	789	433	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013968.D
 Acq On : 09 Dec 2019 17:48
 Operator : SY/MD
 Sample : K6148-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBT1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	3.720	816	818	820	rVB2	1209	483	0.02%	0.003%
36	3.733	820	822	825	rVB4	759	409	0.02%	0.002%
37	3.756	825	829	831	rVB3	1171	688	0.03%	0.004%
38	3.765	831	832	834	rBV2	771	279	0.01%	0.002%
39	3.781	834	837	839	rBV4	1035	742	0.03%	0.005%
40	3.814	845	847	850	rVB3	1010	514	0.02%	0.003%
41	3.830	850	852	853	rBV3	637	282	0.01%	0.002%
42	3.846	853	857	859	rBV3	1000	783	0.04%	0.005%
43	3.920	868	880	916	rBV2	162999	448333	21.14%	2.726%
44	4.396	1012	1028	1053	rBV	349639	847070	39.95%	5.150%
45	4.691	1118	1120	1121	rBV2	1001	341	0.02%	0.002%
46	4.830	1160	1163	1166	rBV4	1156	888	0.04%	0.005%
47	4.894	1181	1183	1185	rBV2	987	487	0.02%	0.003%
48	4.949	1197	1200	1202	rBV4	957	638	0.03%	0.004%
49	4.971	1205	1207	1211	rVB3	1355	883	0.04%	0.005%
50	5.090	1225	1244	1270	rBV2	845924	2120570	100.00%	12.893%
51	5.659	1407	1421	1441	rBV	781704	1531464	72.22%	9.311%
52	6.113	1550	1562	1584	rVB	475491	951700	44.88%	5.786%
53	6.785	1769	1771	1775	rBV5	1138	800	0.04%	0.005%
54	6.974	1828	1830	1831	rBV2	1079	425	0.02%	0.003%
55	7.026	1835	1846	1863	rVV	246521	441267	20.81%	2.683%
56	7.357	1936	1949	1967	rBV	956185	1626938	76.72%	9.892%
57	7.659	2033	2043	2067	rBV	168223	286555	13.51%	1.742%
58	8.125	2177	2188	2218	rBV	497168	929751	43.84%	5.653%
59	8.891	2414	2426	2452	rBV	1092415	1748463	82.45%	10.631%
60	9.177	2510	2515	2518	rBV7	2057	2154	0.10%	0.013%
61	9.386	2577	2580	2581	rBV3	1233	707	0.03%	0.004%
62	9.556	2631	2633	2634	rBV2	967	412	0.02%	0.003%
63	9.646	2659	2661	2663	rBV2	1148	658	0.03%	0.004%
64	9.727	2684	2686	2692	rBV6	1291	1116	0.05%	0.007%
65	9.778	2700	2702	2705	rBV4	1244	1035	0.05%	0.006%
66	10.055	2786	2788	2790	rVB2	850	280	0.01%	0.002%
67	10.180	2825	2827	2831	rBV4	909	552	0.03%	0.003%
68	10.254	2835	2850	2872	rBV	609413	964406	45.48%	5.864%
69	10.360	2881	2883	2887	rBV4	1137	951	0.04%	0.006%
70	10.411	2897	2899	2902	rBV4	1237	690	0.03%	0.004%
71	10.530	2934	2936	2939	rVB3	1393	583	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013968.D
 Acq On : 09 Dec 2019 17:48
 Operator : SY/MD
 Sample : K6148-05
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBT1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

72	10.582	2946	2952	2956	rBV7	1829	2486	0.12%	0.015%
73	10.640	2968	2970	2974	rVB3	902	541	0.03%	0.003%
74	10.669	2978	2979	2984	rVB5	1868	1238	0.06%	0.008%
75	10.784	3013	3015	3017	rBV3	1227	520	0.02%	0.003%
76	10.842	3031	3033	3036	rVB2	1464	600	0.03%	0.004%
77	10.890	3045	3048	3050	rBV2	1506	962	0.05%	0.006%
78	10.952	3063	3067	3069	rBV3	2409	1983	0.09%	0.012%
79	11.289	3159	3172	3192	rBV	981407	1502391	70.85%	9.135%
80	11.665	3277	3289	3305	rBV	915400	1436165	67.73%	8.732%
81	12.344	3498	3500	3503	rVB4	2107	1008	0.05%	0.006%
82	12.366	3503	3507	3509	rBV4	1589	1369	0.06%	0.008%
83	12.839	3652	3654	3656	rBV3	1004	447	0.02%	0.003%
84	12.939	3682	3685	3686	rBV2	1167	516	0.02%	0.003%
85	13.109	3735	3738	3740	rBV3	1250	794	0.04%	0.005%
86	13.318	3795	3803	3809	rBV3	2827	4812	0.23%	0.029%
87	13.505	3859	3861	3862	rBV2	1406	730	0.03%	0.004%
88	13.643	3902	3904	3908	rVB2	1508	646	0.03%	0.004%
89	13.955	3998	4001	4004	rBV2	2224	1513	0.07%	0.009%


Sum of corrected areas: 16447212

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120919\
Data File : VV013968.D
Acq On : 09 Dec 2019 17:48
Operator : SY/MD
Sample : K6148-05
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBT1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

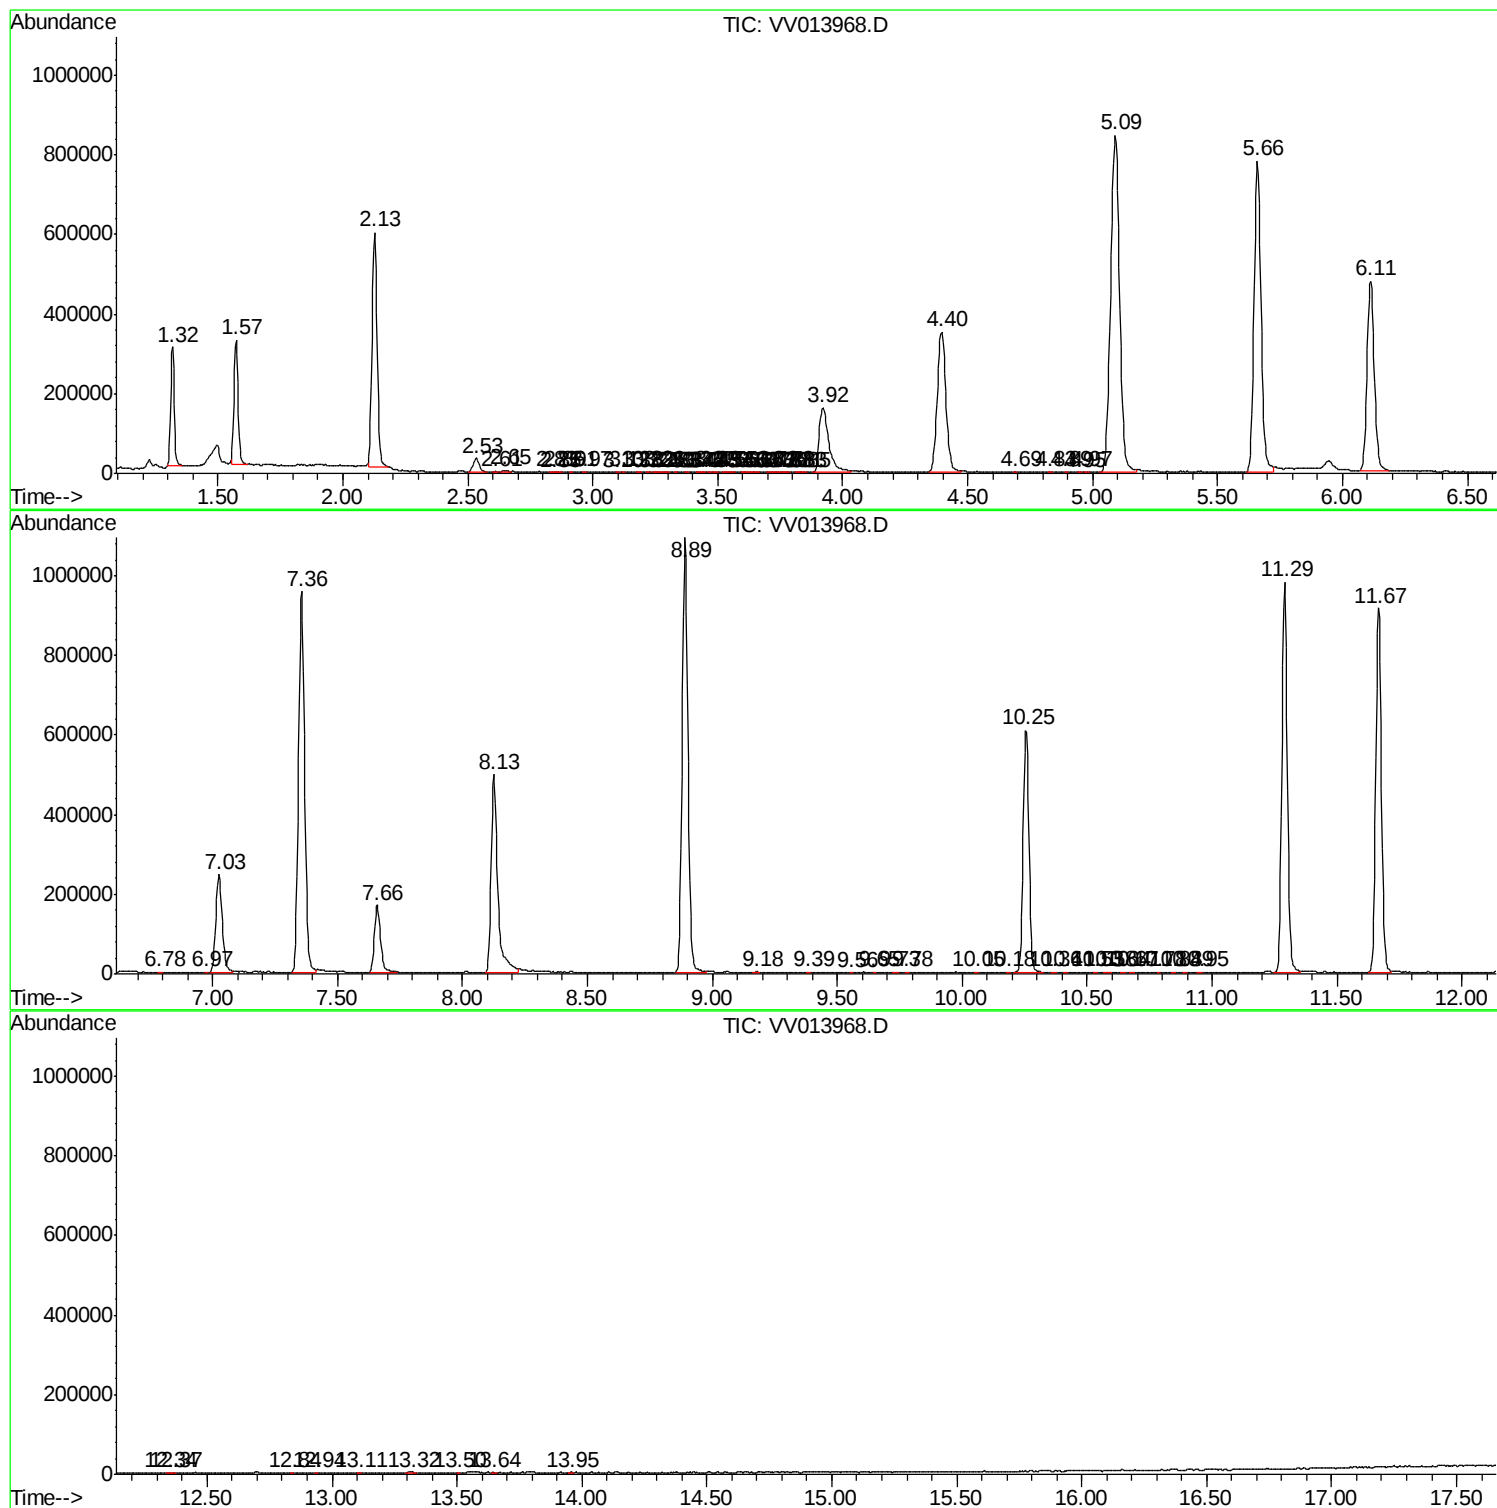

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120919\
Data File : VV013968.D
Acq On : 09 Dec 2019 17:48
Operator : SY/MD
Sample : K6148-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBT1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120919\
Data File : VV013968.D
Acq On : 09 Dec 2019 17:48
Operator : SY/MD
Sample : K6148-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBT1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc