

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013970.D
 Acq On : 09 Dec 2019 18:36
 Operator : SY/MD
 Sample : K6148-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBW0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	80	rVB	294009	285919	13.25%	1.741%
2	1.573	143	150	159	rVB	304775	353417	16.37%	2.151%
3	2.126	314	322	335	rVB	610845	849593	39.36%	5.172%
4	2.534	442	449	463	rVB2	31134	50638	2.35%	0.308%
5	2.647	476	484	492	rBV8	4445	8240	0.38%	0.050%
6	2.762	518	520	521	rBV3	851	288	0.01%	0.002%
7	2.846	542	546	549	rVB4	1286	833	0.04%	0.005%
8	2.923	566	570	572	rBV3	1147	1110	0.05%	0.007%
9	3.036	603	605	610	rBV4	1642	896	0.04%	0.005%
10	3.106	622	627	631	rBV6	1288	1183	0.05%	0.007%
11	3.126	631	633	634	rBV2	384	168	0.01%	0.001%
12	3.145	638	639	640	rBV2	598	150	0.01%	0.001%
13	3.187	650	652	656	rBV4	915	583	0.03%	0.004%
14	3.216	659	661	665	rVB4	1358	957	0.04%	0.006%
15	3.238	665	668	672	rBV3	1100	1075	0.05%	0.007%
16	3.277	675	680	681	rBV3	1608	1082	0.05%	0.007%
17	3.312	690	691	692	rBV	665	225	0.01%	0.001%
18	3.332	695	697	698	rVB2	581	221	0.01%	0.001%
19	3.373	708	710	712	rBV3	1256	629	0.03%	0.004%
20	3.422	723	725	726	rBV	1087	500	0.02%	0.003%
21	3.447	731	733	737	rVB3	2115	1108	0.05%	0.007%
22	3.463	737	738	740	rBV2	906	397	0.02%	0.002%
23	3.524	752	757	758	rBV2	1074	943	0.04%	0.006%
24	3.627	787	789	790	rBV2	741	318	0.01%	0.002%
25	3.692	805	809	813	rBV7	1325	1003	0.05%	0.006%
26	3.711	813	815	818	rVB3	682	241	0.01%	0.001%
27	3.733	818	822	824	rBV5	1265	979	0.05%	0.006%
28	3.778	833	836	840	rBV	775	565	0.03%	0.003%
29	3.804	842	844	849	rVV4	917	716	0.03%	0.004%
30	3.849	856	858	859	rBV2	630	236	0.01%	0.001%
31	3.920	869	880	907	rBV	164064	433145	20.07%	2.637%
32	4.322	1002	1005	1009	rVB4	1497	866	0.04%	0.005%
33	4.396	1010	1028	1051	rBV	360494	880602	40.80%	5.361%
34	4.666	1110	1112	1114	rVV3	892	235	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013970.D
 Acq On : 09 Dec 2019 18:36
 Operator : SY/MD
 Sample : K6148-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBBW0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	4.682	1114	1117	1120	rVB4	1196	809	0.04%	0.005%
36	4.836	1163	1165	1168	rBV4	725	404	0.02%	0.002%
37	4.894	1178	1183	1185	rBV5	1086	1023	0.05%	0.006%
38	4.926	1189	1193	1198	rVB6	1278	1370	0.06%	0.008%
39	4.955	1199	1202	1203	rBV2	608	347	0.02%	0.002%
40	4.984	1207	1211	1215	rVB5	1603	1161	0.05%	0.007%
41	5.020	1220	1222	1225	rVB2	945	300	0.01%	0.002%
42	5.090	1225	1244	1274	rBV2	846450	2158514	100.00%	13.140%
43	5.659	1405	1421	1443	rBV	745283	1466672	67.95%	8.929%
44	6.113	1549	1562	1585	rVB	476731	967343	44.82%	5.889%
45	7.026	1835	1846	1869	rBV	250588	445828	20.65%	2.714%
46	7.354	1935	1948	1968	rBV	991250	1708918	79.17%	10.403%
47	7.659	2032	2043	2063	rBV	174732	299660	13.88%	1.824%
48	8.126	2178	2188	2223	rBV	493822	944239	43.74%	5.748%
49	8.775	2387	2390	2393	rBV4	1068	827	0.04%	0.005%
50	8.891	2414	2426	2444	rBV	1045643	1695154	78.53%	10.320%
51	9.235	2529	2533	2535	rBV4	1407	934	0.04%	0.006%
52	9.576	2637	2639	2641	rBV3	1011	432	0.02%	0.003%
53	9.801	2707	2709	2712	rBV4	1609	1079	0.05%	0.007%
54	9.846	2720	2723	2727	rBV5	791	517	0.02%	0.003%
55	10.026	2775	2779	2781	rBV3	1132	700	0.03%	0.004%
56	10.190	2827	2830	2834	rBV4	1151	1070	0.05%	0.007%
57	10.254	2840	2850	2870	rVB	615545	963068	44.62%	5.863%
58	10.495	2922	2925	2927	rVB3	1217	591	0.03%	0.004%
59	10.611	2959	2961	2963	rBV3	1085	502	0.02%	0.003%
60	10.656	2973	2975	2976	rBV2	937	349	0.02%	0.002%
61	10.714	2990	2993	2998	rVB7	1022	803	0.04%	0.005%
62	10.736	2998	3000	3002	rBV3	1041	485	0.02%	0.003%
63	10.836	3029	3031	3034	rVB3	1319	767	0.04%	0.005%
64	10.855	3034	3037	3038	rBV2	893	499	0.02%	0.003%
65	10.987	3075	3078	3080	rBV4	1131	929	0.04%	0.006%
66	11.080	3104	3107	3112	rBV6	1702	1575	0.07%	0.010%
67	11.170	3132	3135	3138	rBV3	1047	779	0.04%	0.005%
68	11.190	3138	3141	3142	rBV3	1034	579	0.03%	0.004%
69	11.289	3160	3172	3191	rBV	925540	1449495	67.15%	8.824%
70	11.666	3277	3289	3307	rBV	902558	1417212	65.66%	8.628%
71	11.875	3350	3354	3357	rBV6	1294	1362	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
Data File : VV013970.D
Acq On : 09 Dec 2019 18:36
Operator : SY/MD
Sample : K6148-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBW0

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis

72	11.952	3376	3378	3379	rBV3	1015	368	0.02%	0.002%
73	12.151	3437	3440	3442	rBV3	867	592	0.03%	0.004%
74	12.315	3489	3491	3492	rBV2	1073	287	0.01%	0.002%
75	12.360	3503	3505	3508	rBV4	1098	975	0.05%	0.006%
76	12.585	3573	3575	3578	rBV3	1337	878	0.04%	0.005%
77	12.662	3598	3599	3600	rBV2	918	301	0.01%	0.002%
78	12.839	3653	3654	3656	rBV2	892	416	0.02%	0.003%
79	12.875	3660	3665	3667	rBV5	1262	1399	0.06%	0.009%
80	13.035	3713	3715	3716	rBV2	835	310	0.01%	0.002%
81	13.112	3737	3739	3744	rBV3	1281	901	0.04%	0.005%
82	13.161	3752	3754	3755	rBV2	994	455	0.02%	0.003%
83	13.347	3810	3812	3813	rBV2	729	403	0.02%	0.002%
84	13.711	3921	3925	3928	rBV4	1928	1513	0.07%	0.009%
85	13.865	3970	3973	3974	rBV3	1729	899	0.04%	0.005%
86	13.974	4005	4007	4008	rBV2	1228	573	0.03%	0.003%
87	14.428	4146	4148	4152	rBV4	1698	964	0.04%	0.006%


Sum of corrected areas: 16426591

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120919\
Data File : VV013970.D
Acq On : 09 Dec 2019 18:36
Operator : SY/MD
Sample : K6148-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBW0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

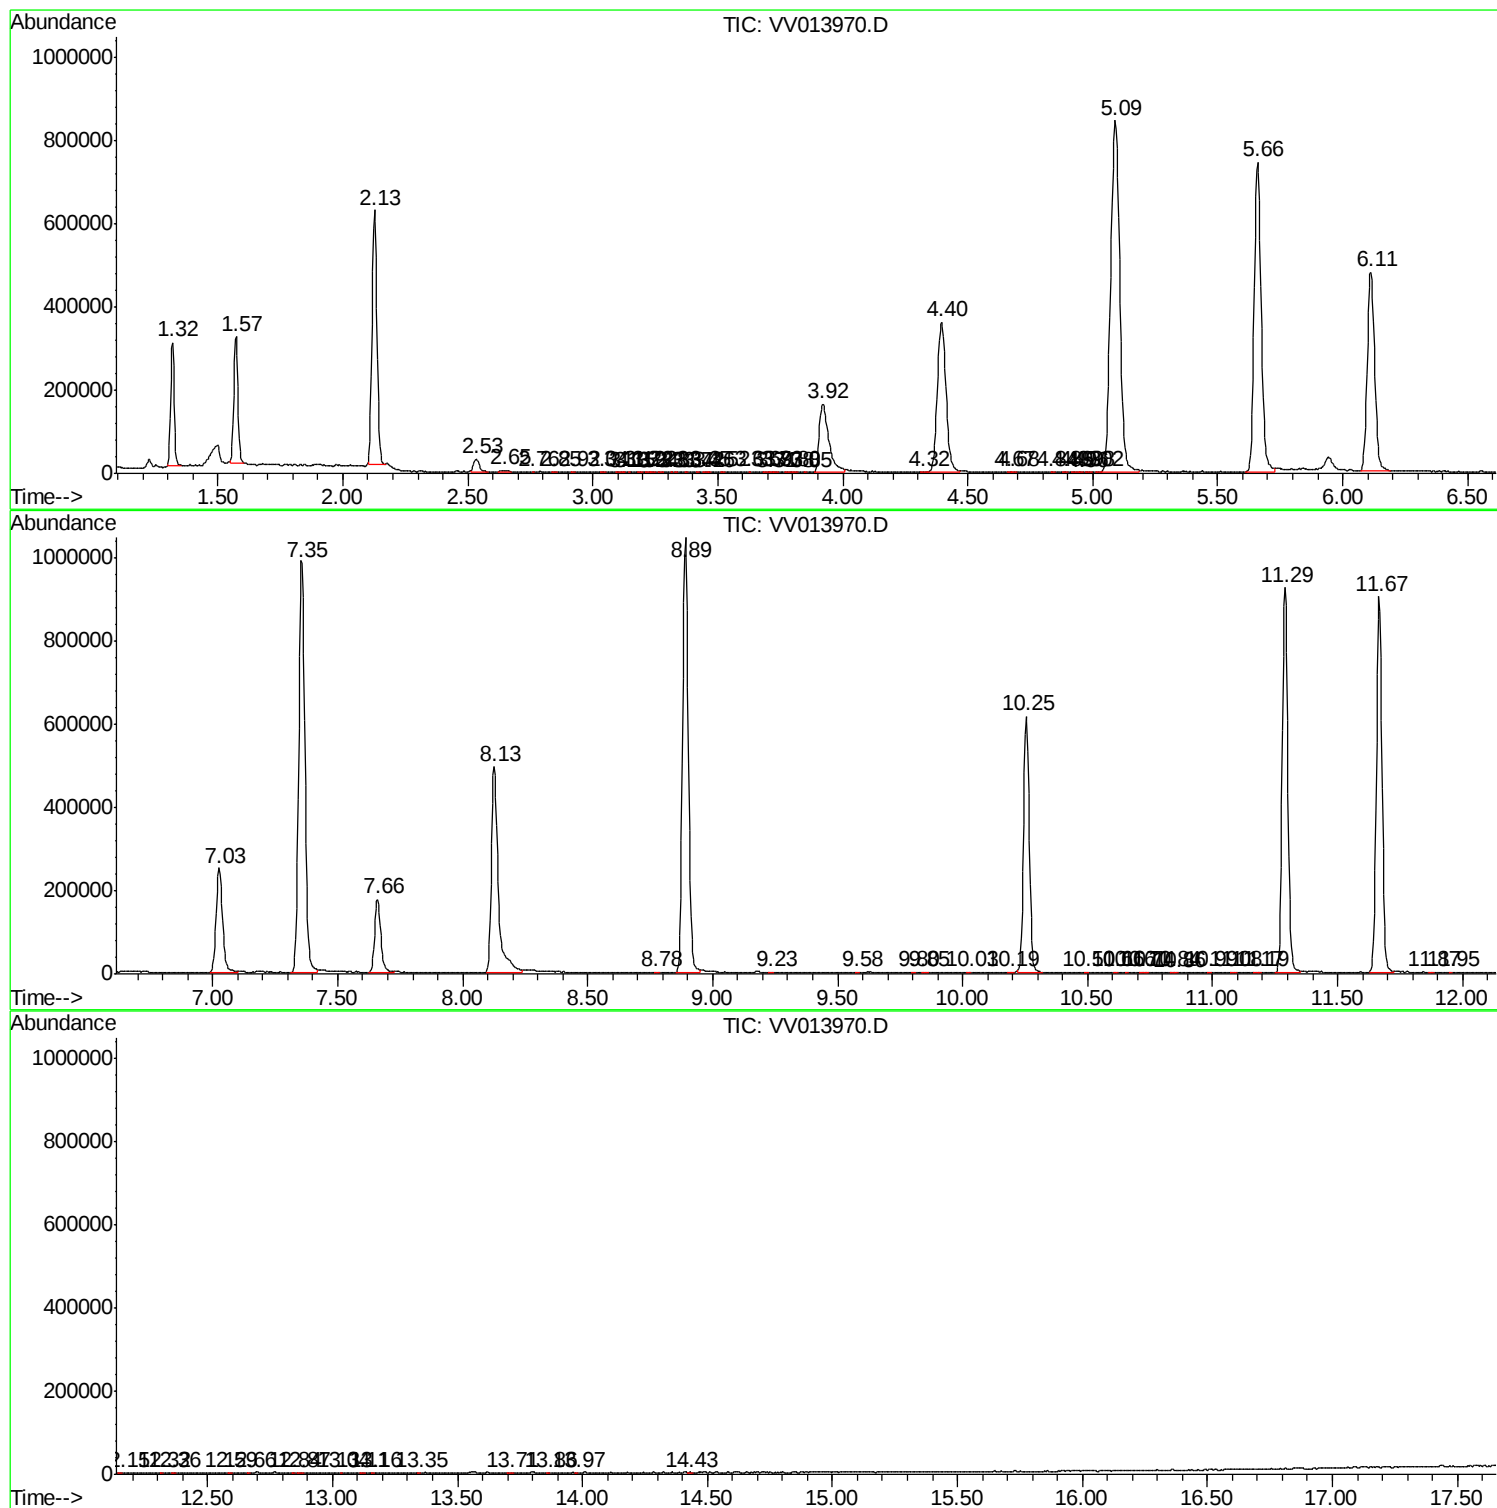

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120919\
Data File : VV013970.D
Acq On : 09 Dec 2019 18:36
Operator : SY/MD
Sample : K6148-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBW0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120919\
Data File : VV013970.D
Acq On : 09 Dec 2019 18:36
Operator : SY/MD
Sample : K6148-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBBW0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc