

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013973.D
 Acq On : 09 Dec 2019 19:49
 Operator : SY/MD
 Sample : K6200-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	81	rVB	282078	268916	13.37%	1.755%
2	1.573	144	150	162	rVB	297029	339157	16.86%	2.214%
3	2.126	314	322	335	rVB	570619	796837	39.61%	5.201%
4	2.621	475	476	477	rBV	818	218	0.01%	0.001%
5	2.717	503	506	513	rBV8	1644	1410	0.07%	0.009%
6	2.775	522	524	526	rBV3	1446	748	0.04%	0.005%
7	2.978	581	587	590	rBV7	1648	1512	0.08%	0.010%
8	3.016	596	599	601	rBV3	1253	876	0.04%	0.006%
9	3.097	621	624	625	rBV3	1265	658	0.03%	0.004%
10	3.203	654	657	661	rVB4	1651	1091	0.05%	0.007%
11	3.232	663	666	668	rBV3	1605	995	0.05%	0.006%
12	3.341	698	700	702	rVB3	802	226	0.01%	0.001%
13	3.351	702	703	706	rBV	681	349	0.02%	0.002%
14	3.428	722	727	728	rBV4	1339	1056	0.05%	0.007%
15	3.460	735	737	739	rBV3	903	458	0.02%	0.003%
16	3.492	745	747	749	rBV2	642	368	0.02%	0.002%
17	3.518	753	755	758	rVV4	874	460	0.02%	0.003%
18	3.566	767	770	773	rBV3	710	598	0.03%	0.004%
19	3.627	785	789	791	rBV4	1156	1098	0.05%	0.007%
20	3.650	794	796	799	rVV3	885	512	0.03%	0.003%
21	3.666	799	801	806	rVB4	1502	1332	0.07%	0.009%
22	3.695	806	810	815	rBV6	1863	1974	0.10%	0.013%
23	3.717	815	817	820	rBV4	698	501	0.02%	0.003%
24	3.740	822	824	827	rBV3	889	409	0.02%	0.003%
25	3.920	869	880	905	rBV	156067	404456	20.11%	2.640%
26	4.396	1012	1028	1049	rBV	341753	814879	40.51%	5.319%
27	4.955	1199	1202	1207	rBV7	1616	1596	0.08%	0.010%
28	5.090	1222	1244	1270	rBV2	780284	2011675	100.00%	13.131%
29	5.576	1389	1395	1400	rBV8	2210	2480	0.12%	0.016%
30	5.659	1408	1421	1447	rBV	722177	1431591	71.16%	9.345%
31	6.113	1550	1562	1580	rVB	450139	878929	43.69%	5.737%
32	6.888	1800	1803	1804	rBV4	1651	680	0.03%	0.004%
33	6.949	1820	1822	1824	rBV3	1266	809	0.04%	0.005%
34	7.026	1834	1846	1862	rBV	237091	413320	20.55%	2.698%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV120919\
 Data File : VV013973.D
 Acq On : 09 Dec 2019 19:49
 Operator : SY/MD
 Sample : K6200-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFF07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
 Title : VOC Analysis

35	7.357	1936	1949	1970	rBV	896387	1539726	76.54%	10.051%
36	7.659	2032	2043	2064	rBV	170903	292351	14.53%	1.908%
37	8.125	2178	2188	2224	rBV2	452546	905172	45.00%	5.908%
38	8.521	2308	2311	2312	rBV	1022	578	0.03%	0.004%
39	8.891	2414	2426	2449	rBV	1031159	1661823	82.61%	10.848%
40	9.225	2527	2530	2532	rBV4	1114	710	0.04%	0.005%
41	9.260	2539	2541	2544	rVB2	1432	574	0.03%	0.004%
42	9.280	2545	2547	2552	rVV4	1400	1235	0.06%	0.008%
43	9.550	2629	2631	2633	rBV4	1231	605	0.03%	0.004%
44	9.675	2667	2670	2672	rBV4	994	747	0.04%	0.005%
45	9.723	2683	2685	2687	rBV3	1869	1068	0.05%	0.007%
46	9.820	2713	2715	2717	rBV3	883	328	0.02%	0.002%
47	9.836	2717	2720	2725	rVB4	1390	1211	0.06%	0.008%
48	9.862	2725	2728	2731	rBV3	987	816	0.04%	0.005%
49	9.897	2736	2739	2744	rVB6	2626	2250	0.11%	0.015%
50	9.936	2744	2751	2752	rBV5	1460	1898	0.09%	0.012%
51	10.071	2790	2793	2794	rBV3	1429	680	0.03%	0.004%
52	10.257	2838	2851	2867	rBV	609294	950999	47.27%	6.208%
53	10.839	3030	3032	3034	rBV	1792	1071	0.05%	0.007%
54	11.122	3118	3120	3123	rBV3	1170	677	0.03%	0.004%
55	11.199	3142	3144	3146	rBV3	1322	726	0.04%	0.005%
56	11.289	3159	3172	3188	rBV	839812	1311139	65.18%	8.558%
57	11.666	3278	3289	3307	rBV	791395	1251740	62.22%	8.171%
58	11.948	3372	3377	3378	rBV3	1324	1098	0.05%	0.007%
59	12.116	3427	3429	3431	rBV4	1612	871	0.04%	0.006%
60	12.247	3468	3470	3473	rBV4	1330	774	0.04%	0.005%
61	12.604	3578	3581	3583	rBV3	1261	784	0.04%	0.005%
62	12.868	3659	3663	3665	rBV2	1247	947	0.05%	0.006%
63	12.907	3672	3675	3676	rBV2	1498	847	0.04%	0.006%
64	13.148	3748	3750	3752	rBV2	889	536	0.03%	0.003%
65	13.495	3855	3858	3859	rBV2	1123	682	0.03%	0.004%
66	13.743	3932	3935	3937	rBV3	1642	1242	0.06%	0.008%
67	13.958	4000	4002	4006	rBV3	2390	1773	0.09%	0.012%


Sum of corrected areas: 15319852

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV120919\
Data File : VV013973.D
Acq On : 09 Dec 2019 19:49
Operator : SY/MD
Sample : K6200-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF07

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

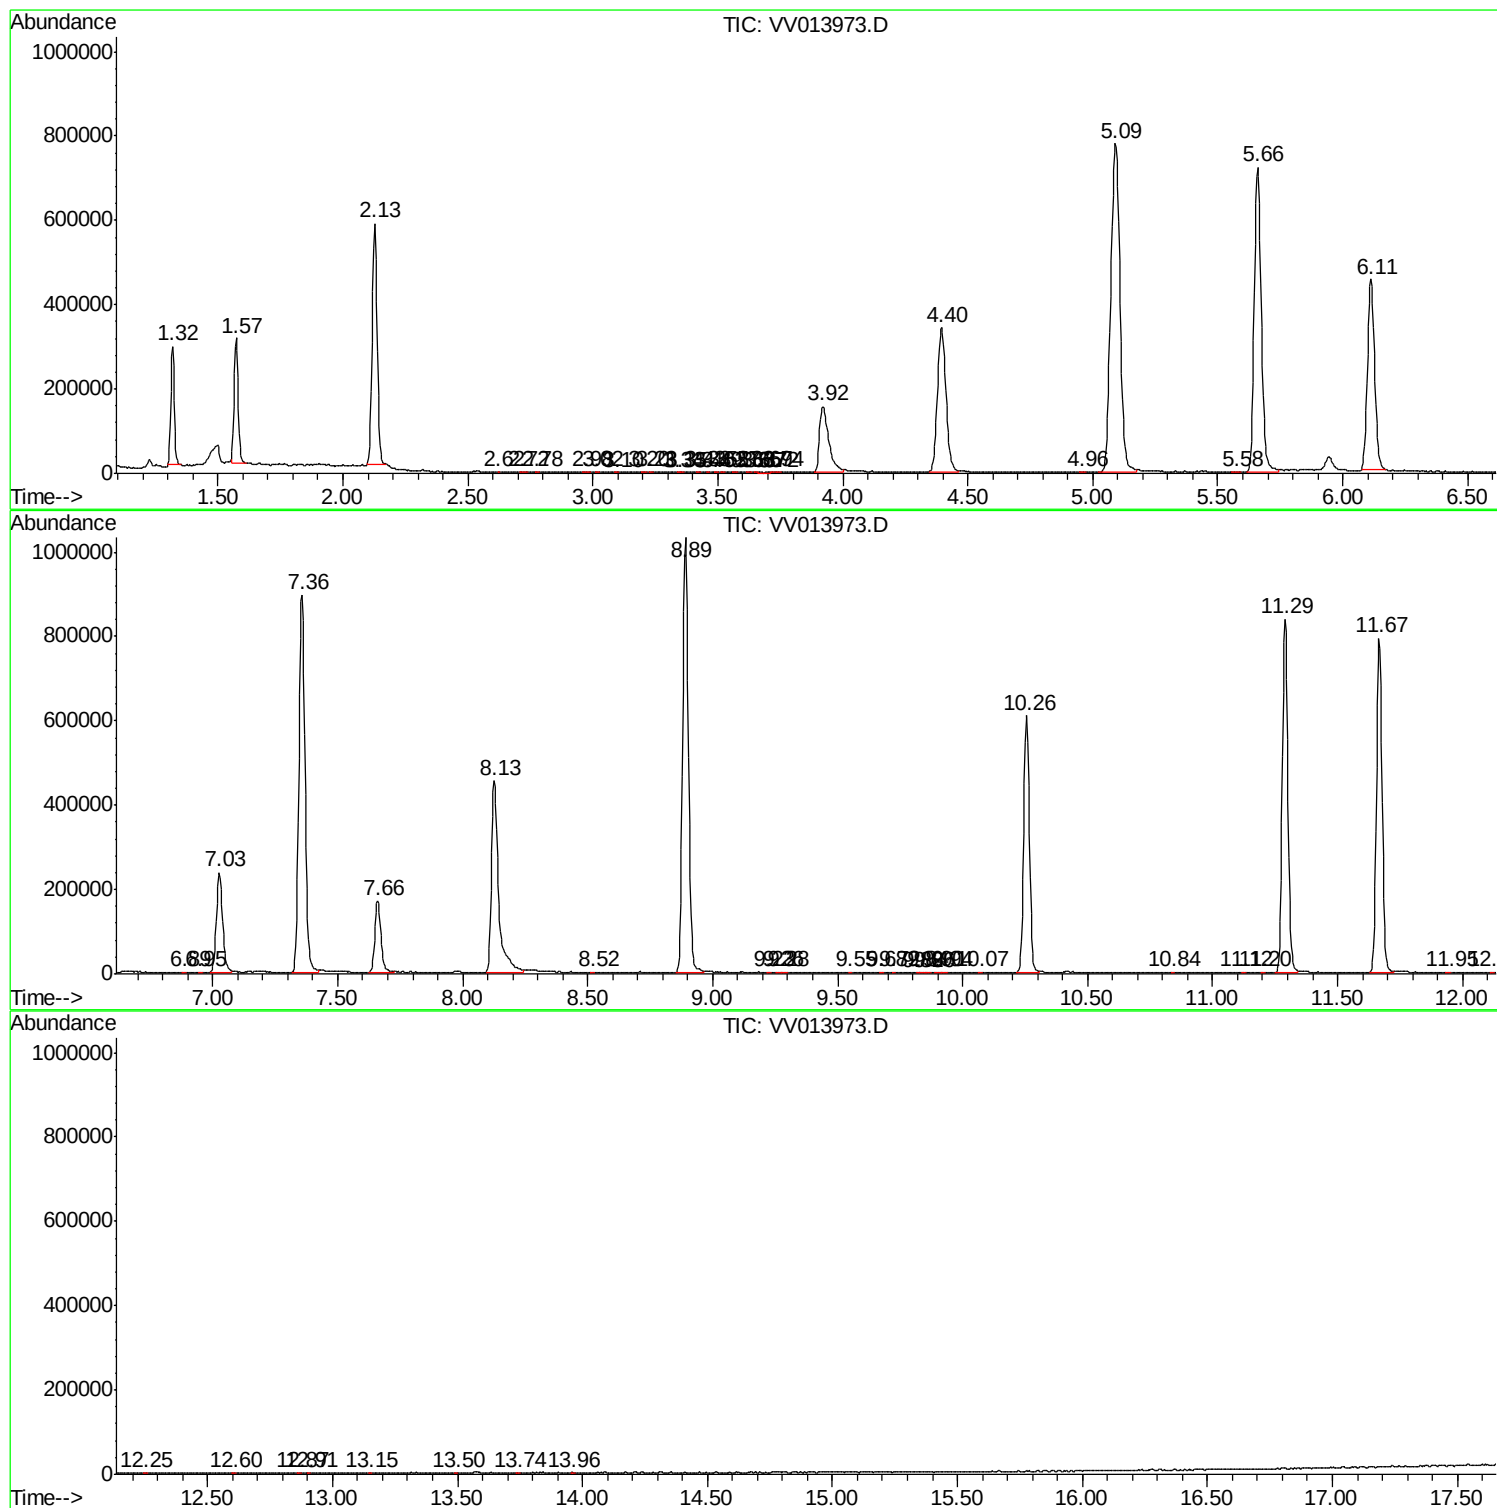

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV120919\
Data File : VV013973.D
Acq On : 09 Dec 2019 19:49
Operator : SY/MD
Sample : K6200-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF07

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV120919\
Data File : VV013973.D
Acq On : 09 Dec 2019 19:49
Operator : SY/MD
Sample : K6200-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFF07

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc