


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV120919\
Data File : VV013951.D
Acq On : 09 Dec 2019 09:05
Operator : SY/MD
Sample : BFB78
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB78

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM120219WMA.M
Title : VOC Analysis
Last Update : Tue Dec 10 11:57:03 2019

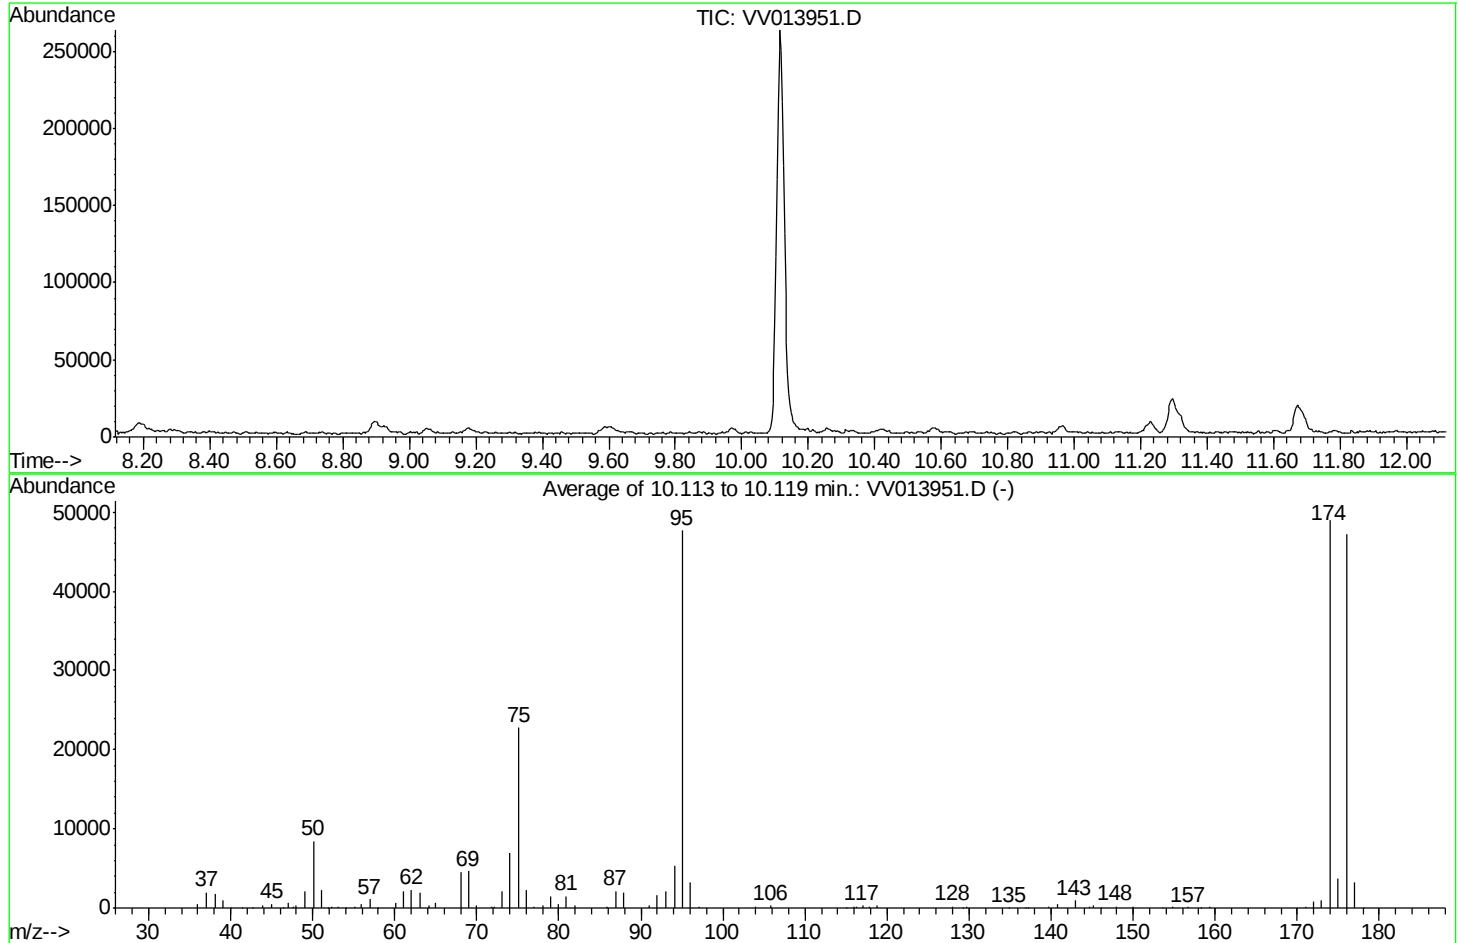

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	8427	PASS
75	95	30	80	47.7	22762	PASS
95	95	100	100	100.0	47674	PASS
96	95	5	9	6.6	3166	PASS
173	174	0.00	2	1.8	901	PASS
174	95	50	120	102.7	48962	PASS
175	174	5	9	7.7	3763	PASS
176	174	95	101	96.4	47186	PASS
177	176	5	9	6.8	3207	PASS

m/z	Abundance
36.00	405.0
37.10	1975.0
38.10	1780.0
39.10	1046.0
39.90	697.0
42.70	135.0
44.00	938.0
45.10	521.0
47.00	679.0
47.70	328.0
48.00	361.0
49.00	2041.0
50.10	8307.0
51.00	2427.0
52.20	120.0
53.20	117.0
55.10	164.0
56.00	656.0
57.00	1082.0
58.00	131.0
60.00	691.0
61.00	2083.0
62.10	2482.0
63.00	1850.0
64.10	373.0
65.00	624.0
68.00	4550.0
69.00	4678.0
70.00	375.0
72.20	241.0
73.00	2062.0
74.00	6767.0
75.10	22480.0
76.10	2169.0
76.90	200.0
78.00	261.0
78.90	1475.0
80.00	529.0
80.90	1615.0
82.10	436.0
86.90	2223.0
87.90	2259.0
90.90	323.0
91.90	1580.0
93.00	2091.0
94.10	5485.0
95.00	47976.0
96.00	3327.0
97.00	152.0
103.90	210.0
105.90	316.0
115.90	262.0
117.00	304.0
117.80	279.0
118.90	365.0
128.00	263.0
129.80	211.0
137.00	125.0
139.60	161.0
140.80	505.0
142.90	886.0
145.10	386.0
147.80	205.0
149.90	160.0
153.60	101.0
156.80	118.0
159.40	146.0
170.90	224.0
171.90	839.0
172.90	942.0
174.00	46696.0
175.00	3806.0
176.00	45384.0
177.00	3156.0
178.00	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.90	471.0
37.00	2098.0
38.10	1867.0
39.10	1020.0
39.90	638.0
41.30	101.0
44.00	819.0
45.00	488.0
46.40	116.0
46.90	621.0
48.00	411.0
49.00	2112.0
50.00	8737.0
51.00	2395.0
52.30	116.0
53.20	139.0
54.00	101.0
55.10	208.0
55.90	557.0
56.90	1102.0
60.10	579.0
61.00	2117.0
62.10	2303.0
63.00	1933.0
64.10	378.0
65.00	599.0
65.70	109.0
68.10	4934.0
69.00	4970.0
69.90	366.0
71.80	187.0
72.10	195.0
73.00	2167.0
74.10	6963.0
75.10	23376.0
76.10	2425.0
77.00	201.0
78.00	216.0
78.90	1513.0
80.00	571.0
80.90	1597.0
82.00	386.0
85.80	159.0
86.90	2237.0
87.90	2140.0
90.90	358.0
91.90	1671.0
93.00	2131.0
94.10	5473.0
95.00	49288.0
96.00	3244.0
97.00	174.0
104.00	240.0
105.90	283.0
115.10	108.0
115.90	236.0
116.40	184.0
117.00	302.0
117.80	232.0
118.90	261.0
128.00	233.0
129.10	110.0
129.70	247.0
134.90	115.0
137.20	124.0
139.70	171.0
140.90	557.0
143.00	895.0
145.10	392.0
146.00	107.0
147.90	242.0
149.90	135.0
154.80	126.0
156.70	137.0
159.40	139.0
171.00	214.0
171.90	830.0
172.90	947.0
174.00	50944.0
175.00	3898.0
176.00	48784.0
177.00	3347.0
178.10	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.90	452.0
37.00	1989.0
38.10	1598.0
39.10	925.0
40.00	613.0
41.40	113.0
44.00	721.0
44.90	471.0
46.30	115.0
47.00	583.0
48.00	366.0
49.00	1928.0
50.00	8237.0
51.00	2173.0
51.90	127.0
52.30	137.0
53.10	177.0
54.00	114.0
55.10	201.0
56.00	470.0
56.90	1016.0
60.10	475.0
61.00	1920.0
62.00	2091.0
63.00	1874.0
64.10	369.0
65.00	526.0
65.80	160.0
68.10	4732.0
69.00	4586.0
69.90	347.0
71.80	186.0
72.10	182.0
73.00	2077.0
74.10	6962.0
75.10	22432.0
76.10	2253.0
77.00	242.0
78.00	299.0
79.00	1418.0
80.00	505.0
80.90	1350.0
81.90	378.0
85.80	175.0
86.90	2004.0
87.90	2011.0
91.00	384.0
92.00	1559.0
93.00	2059.0
94.10	4984.0
95.00	45760.0
96.00	2927.0
97.10	146.0
104.00	233.0
105.90	235.0
115.10	117.0
115.90	216.0
116.30	181.0
117.00	302.0
117.80	172.0
118.80	227.0
128.00	192.0
129.20	138.0
129.70	207.0
134.90	129.0
136.90	107.0
137.20	106.0
139.70	126.0
140.90	586.0
143.00	913.0
144.70	260.0
145.10	303.0
146.00	146.0
148.00	287.0
154.80	145.0
156.70	138.0
158.20	104.0
171.10	229.0
171.90	852.0
172.90	816.0
174.00	49248.0
175.00	3587.0
176.00	47392.0
177.00	3119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78

m/z	Abundance
35.60	103.0
40.00	616.0
43.90	470.0
48.50	104.0
51.40	116.0
65.70	135.0
68.10	185.0
68.80	123.0
83.70	113.0
87.70	196.0
92.20	125.0
171.10	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB78