

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120921\
 Data File : VW023859.D
 Acq On : 09 Dec 2021 14:20
 Operator : SY/MD
 Sample : M4984-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW5S0

Quant Time: Dec 10 00:42:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 02 02:08:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	98930	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	97608	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	48663	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	27615	3.400	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	68.000%	
7) Chloroethane-d5	1.568	69	25369	3.974	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	79.400%	
11) 1,1-Dichloroethene-d2	2.108	63	42941	3.000	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	60.000%	
20) 2-Butanone-d5	3.908	46	70872	72.592	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	145.180%#	
24) Chloroform-d	4.349	84	69796	4.935	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.800%	
26) 1,2-Dichloroethane-d4	5.034	65	33472	5.066	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.400%	
32) Benzene-d6	5.050	84	127486	4.795	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.800%	
36) 1,2-Dichloropropane-d6	6.069	67	38180	5.122	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.400%	
41) Toluene-d8	7.316	98	113058	4.551	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.000%	
43) trans-1,3-Dichloroprop...	7.625	79	14226	4.735	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	94.600%	
46) 2-Hexanone-d5	8.091	63	60828	60.932	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	121.860%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	27103	5.053	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	47126	5.478	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	109.600%	
Target Compounds					Qvalue	
42) Toluene	7.400	91	2185	0.072	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023859.D
Acq On : 09 Dec 2021 14:20
Operator : SY/MD
Sample : M4984-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW5S0

Quant Time: Dec 10 00:42:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 02 02:08:23 2021
Response via : Initial Calibration

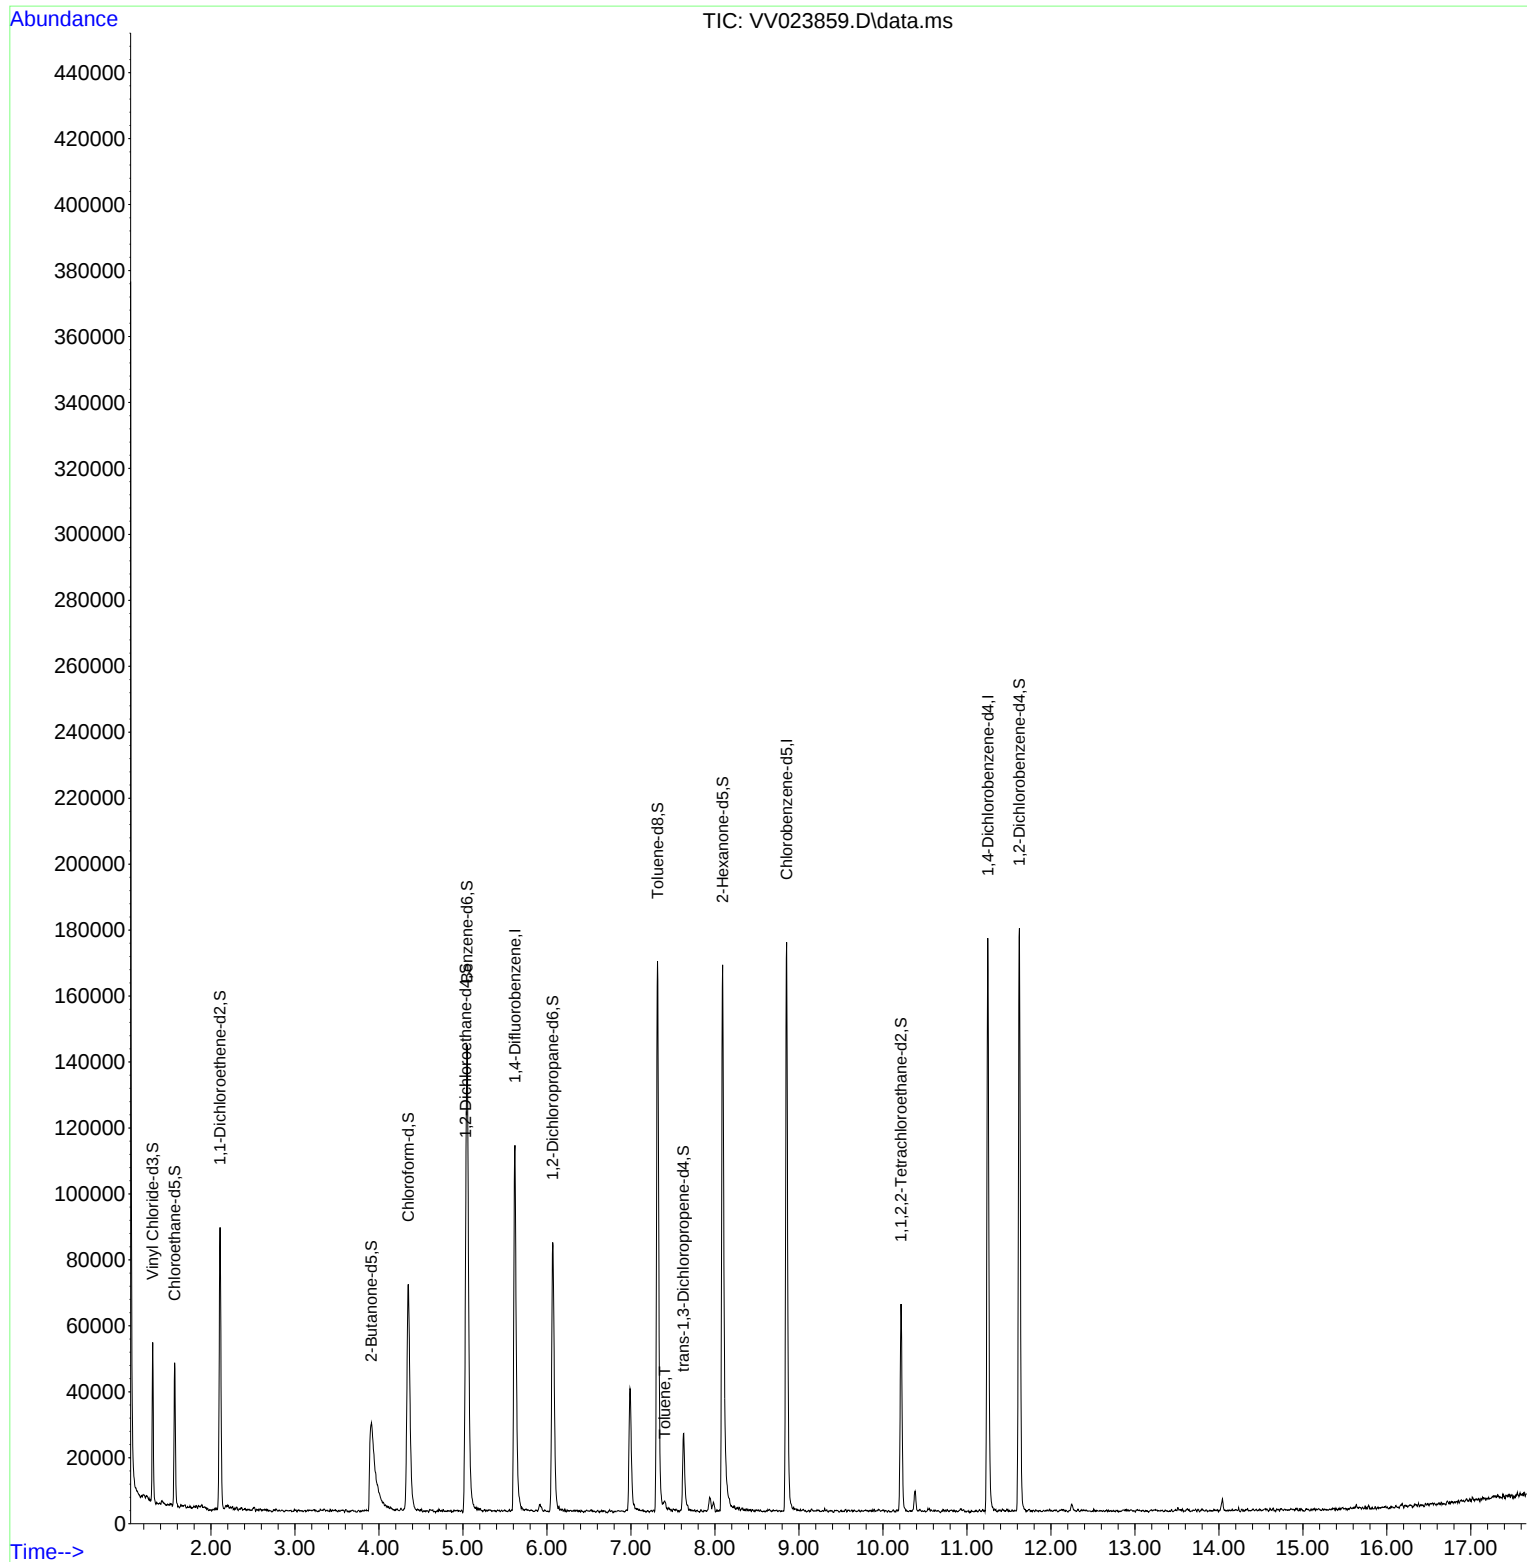

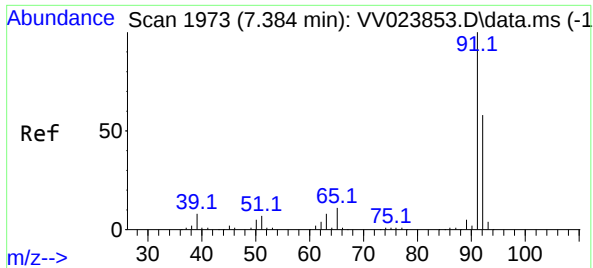

#42
Toluene
Concen: 0.072 ug/L
RT: 7.400 min Scan# 19
Delta R.T. 0.016 min
Lab File: VV023859.D
Acq: 09 Dec 2021 14:20

Instrument :
MSVOA_V
ClientSampleId :
EW5S0

Tgt Ion:	91	Resp:	2185
Ion	Ratio	Lower	Upper
91	100		
92	63.4	41.5	77.1

