

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120921\
 Data File : VW023871.D
 Acq On : 09 Dec 2021 19:05
 Operator : SY/MD
 Sample : M5003-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COCT2

Quant Time: Dec 10 00:44:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 02 02:08:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	105036	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	101254	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	49696	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	26427	3.065	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	61.200%
7) Chloroethane-d5	1.568	69	24996	3.688	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	73.800%
11) 1,1-Dichloroethene-d2	2.108	63	41242	2.714	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.200%#
20) 2-Butanone-d5	3.908	46	69719	67.259	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	134.520%#
24) Chloroform-d	4.352	84	67203	4.476	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.600%
26) 1,2-Dichloroethane-d4	5.034	65	33458	4.770	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.400%
32) Benzene-d6	5.053	84	122334	4.435	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.800%
36) 1,2-Dichloropropane-d6	6.069	67	37365	4.832	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.600%
41) Toluene-d8	7.317	98	106894	4.148	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.000%
43) trans-1,3-Dichloroprop...	7.625	79	14162	4.544	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.800%
46) 2-Hexanone-d5	8.091	63	60574	58.493	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	116.980%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	27511	4.944	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.800%
66) 1,2-Dichlorobenzene-d4	11.625	152	45815	5.214	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.200%
Target Compounds					Qvalue	
42) Toluene	7.397	91	2173	0.069	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023871.D
Acq On : 09 Dec 2021 19:05
Operator : SY/MD
Sample : M5003-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CT2

Quant Time: Dec 10 00:44:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 02 02:08:23 2021
Response via : Initial Calibration

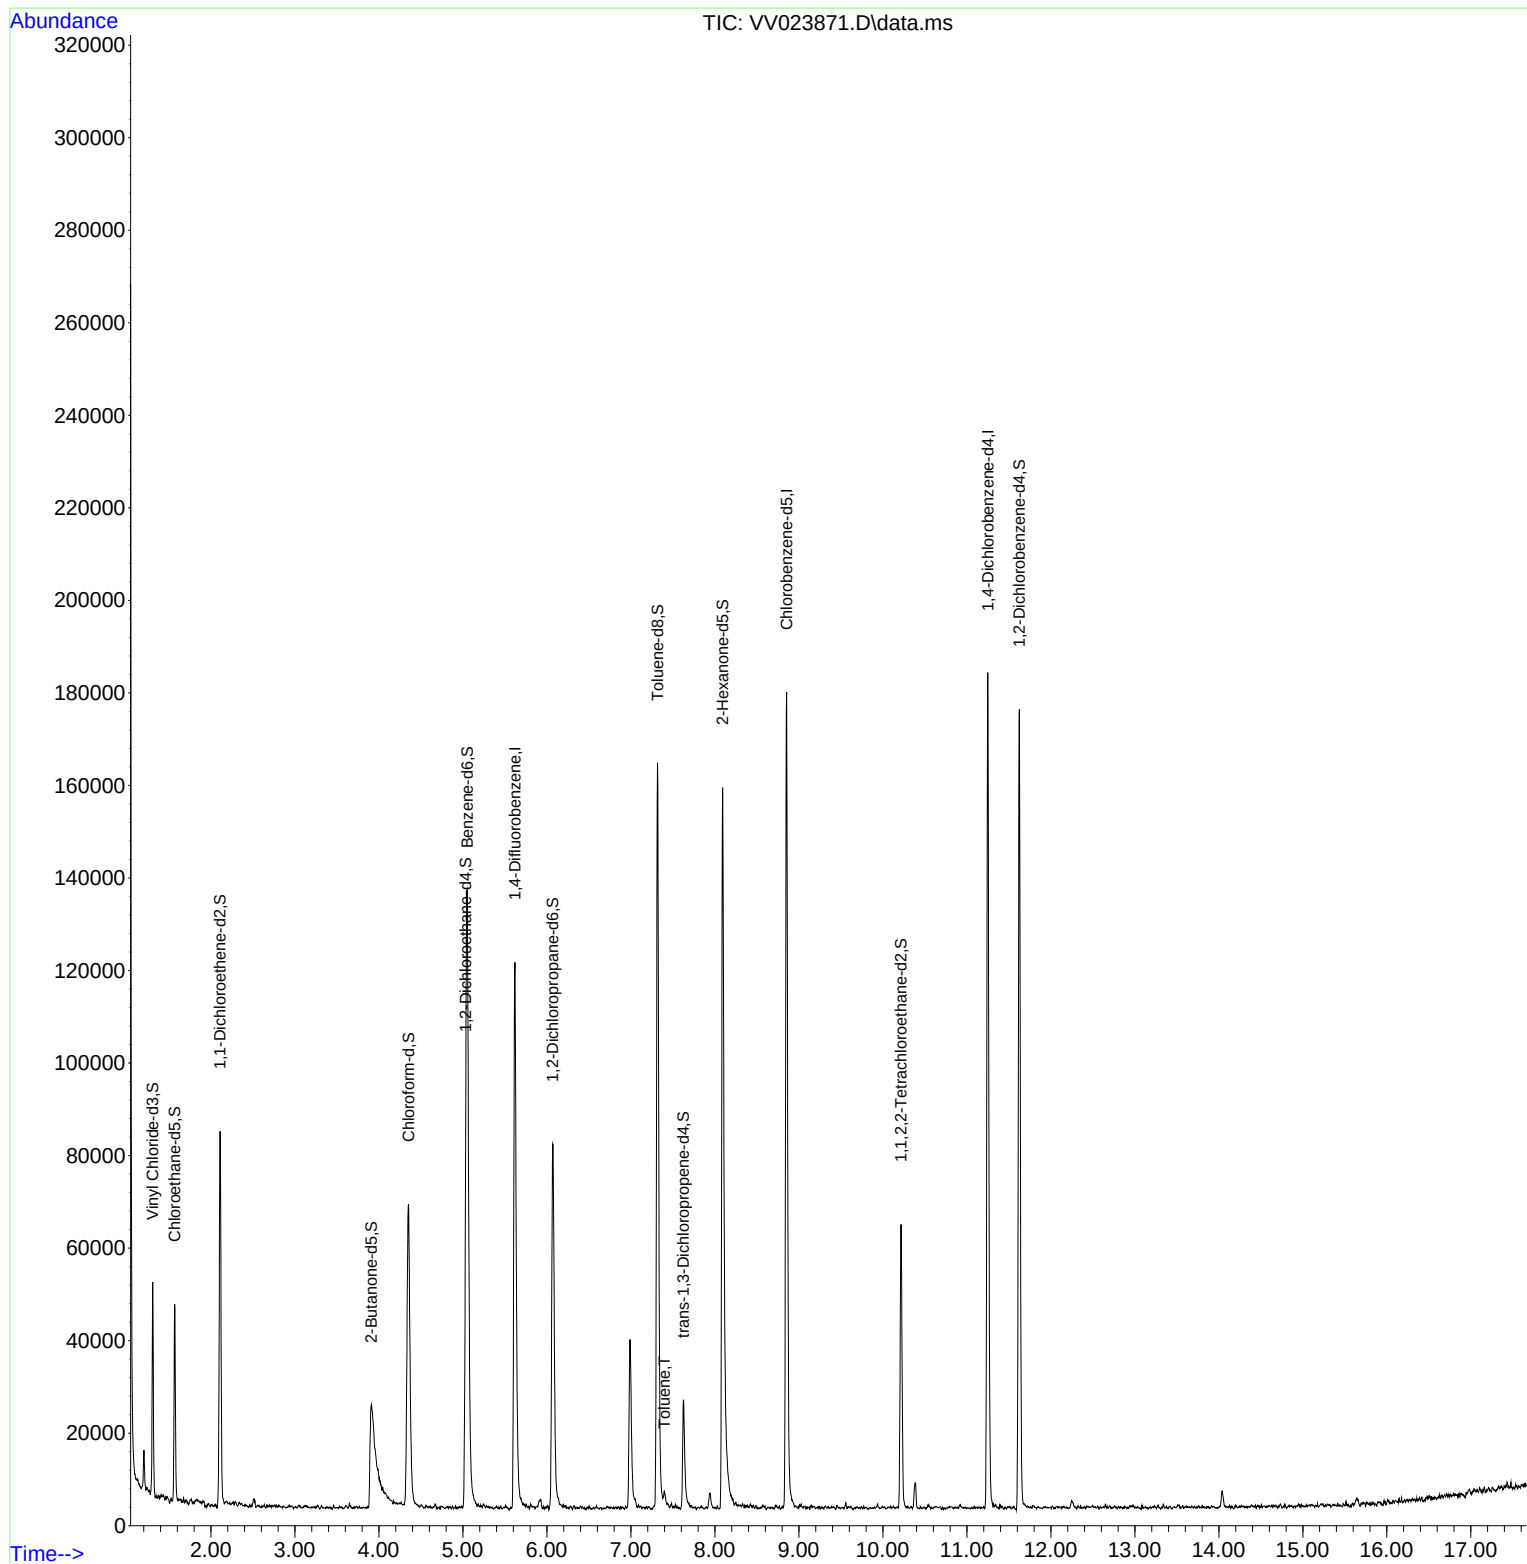

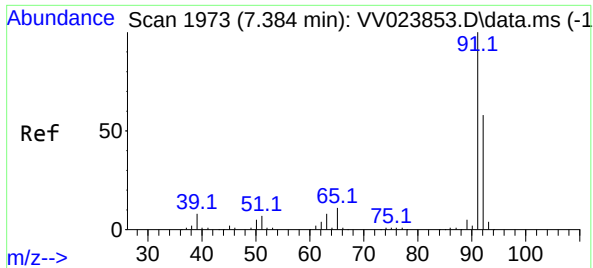

#42
Toluene
Concen: 0.069 ug/L
RT: 7.397 min Scan# 19
Delta R.T. 0.013 min
Lab File: VV023871.D
Acq: 09 Dec 2021 19:05

Instrument :
MSVOA_V
ClientSampleId :
C0CT2

Tgt Ion: 91 Resp: 2173

Ion	Ratio	Lower	Upper
91	100		
92	54.4	41.5	77.1

