

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
 Data File : VV023864.D
 Acq On : 09 Dec 2021 16:19
 Operator : SY/MD
 Sample : M5002-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CT7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	45813	47569	13.98%	1.525%
2	1.568	157	164	172	rBV	42751	48927	14.38%	1.568%
3	1.937	270	279	286	rVB4	3221	5044	1.48%	0.162%
4	2.111	323	333	348	rBV2	84295	126596	37.21%	4.058%
5	3.908	878	892	912	rBV	18030	62911	18.49%	2.016%
6	4.352	1012	1030	1057	rVB	64998	166841	49.04%	5.348%
7	5.050	1232	1247	1273	rBV3	134054	340230	100.00%	10.905%
8	5.619	1412	1424	1449	rBV	117335	241903	71.10%	7.753%
9	5.915	1504	1516	1531	rBV	125247	247667	72.79%	7.938%
10	6.072	1553	1565	1581	rBV3	77080	159675	46.93%	5.118%
11	6.989	1839	1850	1873	rBV	36826	72887	21.42%	2.336%
12	7.316	1938	1952	1974	rBV	156565	279802	82.24%	8.968%
13	7.403	1975	1979	1987	rVB5	2594	3712	1.09%	0.119%
14	7.625	2039	2048	2065	rBV2	21003	40395	11.87%	1.295%
15	7.937	2131	2145	2156	rBV3	6255	11354	3.34%	0.364%
16	8.091	2184	2193	2225	rBV	125181	298973	87.87%	9.583%
17	8.853	2418	2430	2457	rBV	181182	301051	88.48%	9.649%
18	10.217	2842	2854	2873	rVB2	59853	96788	28.45%	3.102%
19	10.381	2893	2905	2915	rBV3	8130	13975	4.11%	0.448%
20	11.249	3164	3175	3192	rBV	183312	285542	83.93%	9.152%
21	11.625	3276	3292	3312	rBV	166588	268124	78.81%	8.594%




Sum of corrected areas: 3119966

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023864.D
Acq On : 09 Dec 2021 16:19
Operator : SY/MD
Sample : M5002-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

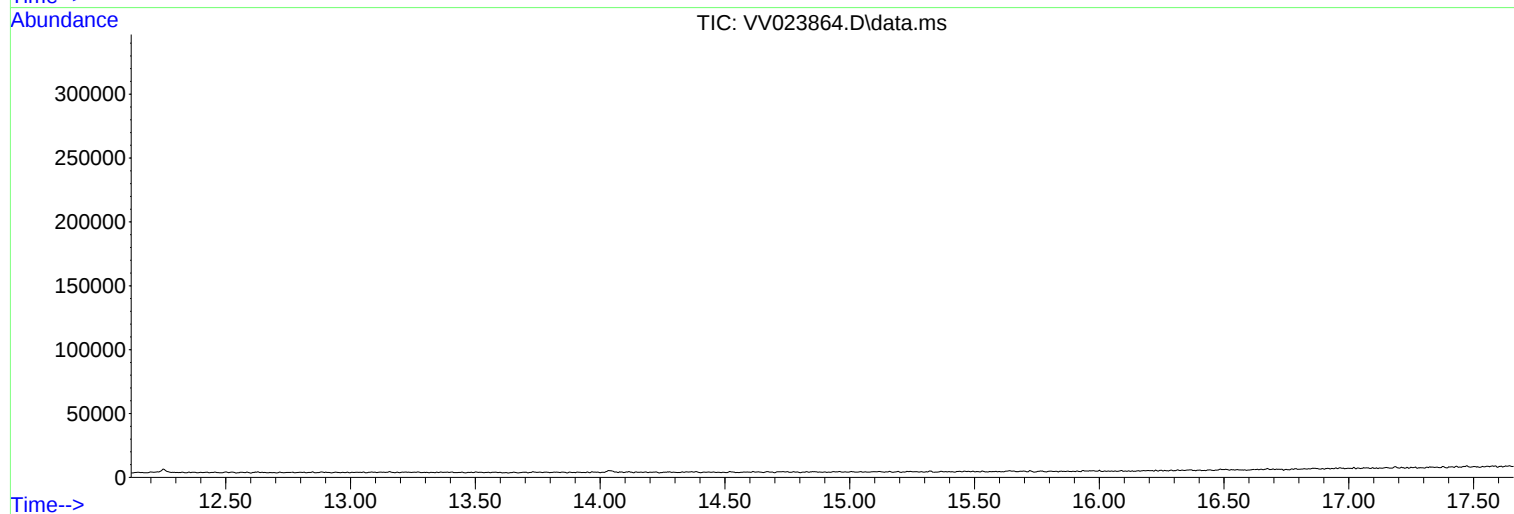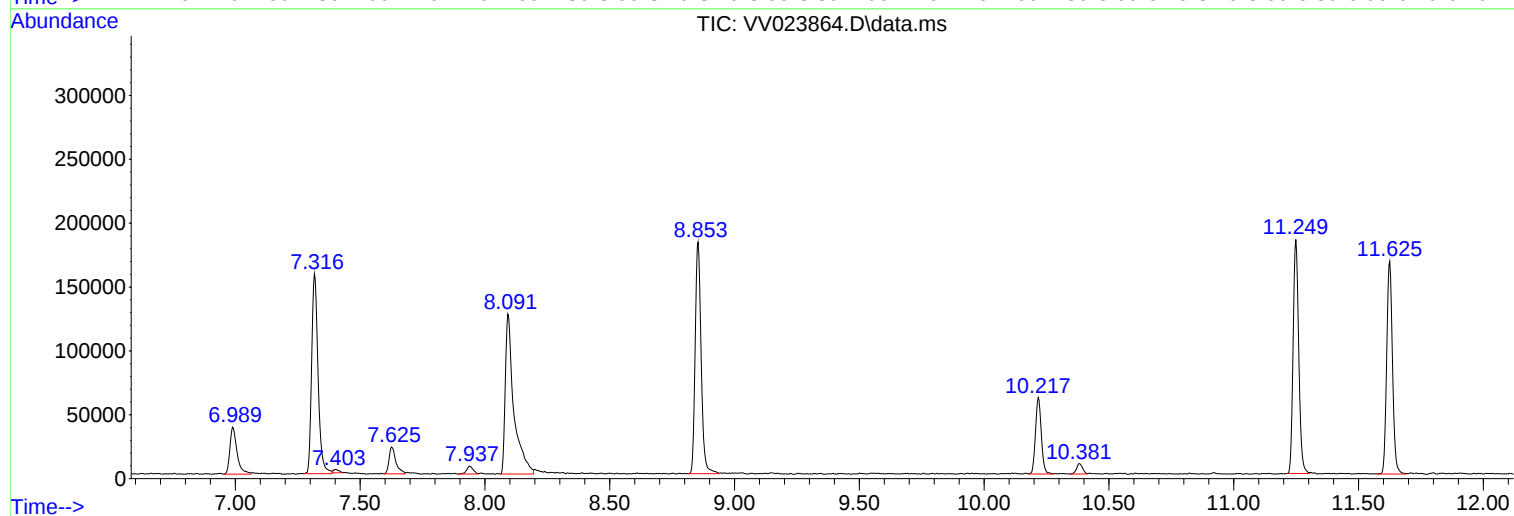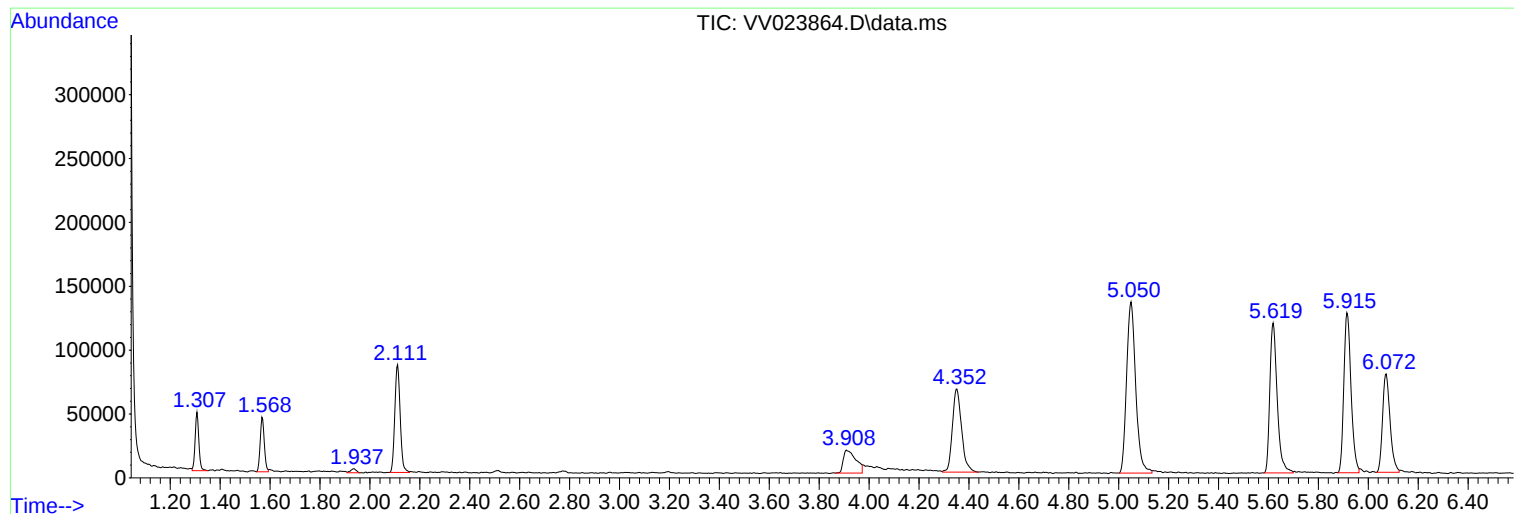

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023864.D
Acq On : 09 Dec 2021 16:19
Operator : SY/MD
Sample : M5002-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023864.D
Acq On : 09 Dec 2021 16:19
Operator : SY/MD
Sample : M5002-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CT7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
