

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
 Data File : VV023865.D
 Acq On : 09 Dec 2021 16:42
 Operator : SY/MD
 Sample : M5002-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CW2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	46973	47887	13.94%	1.639%
2	1.568	157	164	177	rVB	42732	47867	13.93%	1.638%
3	2.108	322	332	348	rBV2	84692	130132	37.87%	4.454%
4	3.195	656	670	681	rBV3	4547	8855	2.58%	0.303%
5	3.915	882	894	921	rBV3	27744	98641	28.71%	3.376%
6	4.349	1014	1029	1060	rVB	67480	180523	52.54%	6.178%
7	5.050	1226	1247	1271	rBV3	136521	343591	100.00%	11.760%
8	5.619	1412	1424	1444	rBV	111138	226453	65.91%	7.750%
9	5.918	1507	1517	1533	rBV7	12735	27128	7.90%	0.928%
10	6.069	1552	1564	1587	rBV	78505	167488	48.75%	5.732%
11	6.989	1840	1850	1868	rBV2	35971	69245	20.15%	2.370%
12	7.317	1940	1952	1972	rBV	157047	283630	82.55%	9.707%
13	7.625	2040	2048	2060	rBV2	21384	38610	11.24%	1.321%
14	7.940	2136	2146	2157	rBV2	5206	9448	2.75%	0.323%
15	8.091	2183	2193	2235	rBV	124838	309385	90.04%	10.589%
16	8.853	2418	2430	2452	rBV	172345	287653	83.72%	9.845%
17	10.217	2843	2854	2870	rVB	60540	97874	28.49%	3.350%
18	10.384	2898	2906	2917	rVB4	5677	9529	2.77%	0.326%
19	11.249	3163	3175	3191	rBV	174415	269760	78.51%	9.233%
20	11.625	3281	3292	3310	rBV	169298	268116	78.03%	9.176%




Sum of corrected areas: 2921815

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023865.D
Acq On : 09 Dec 2021 16:42
Operator : SY/MD
Sample : M5002-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

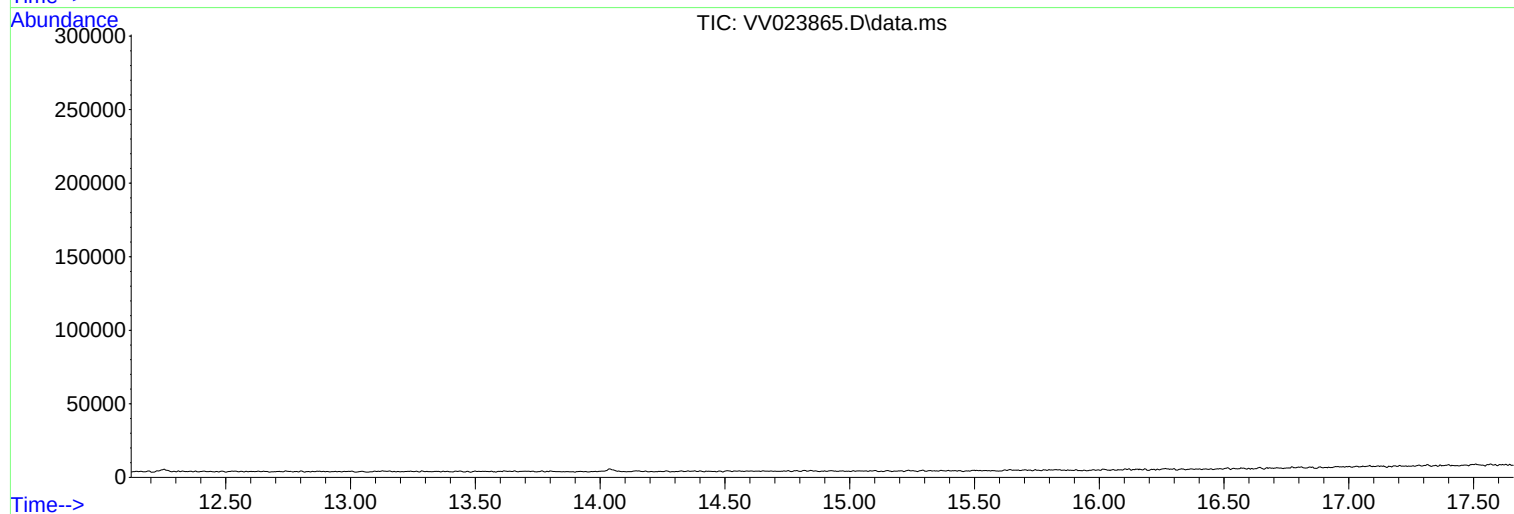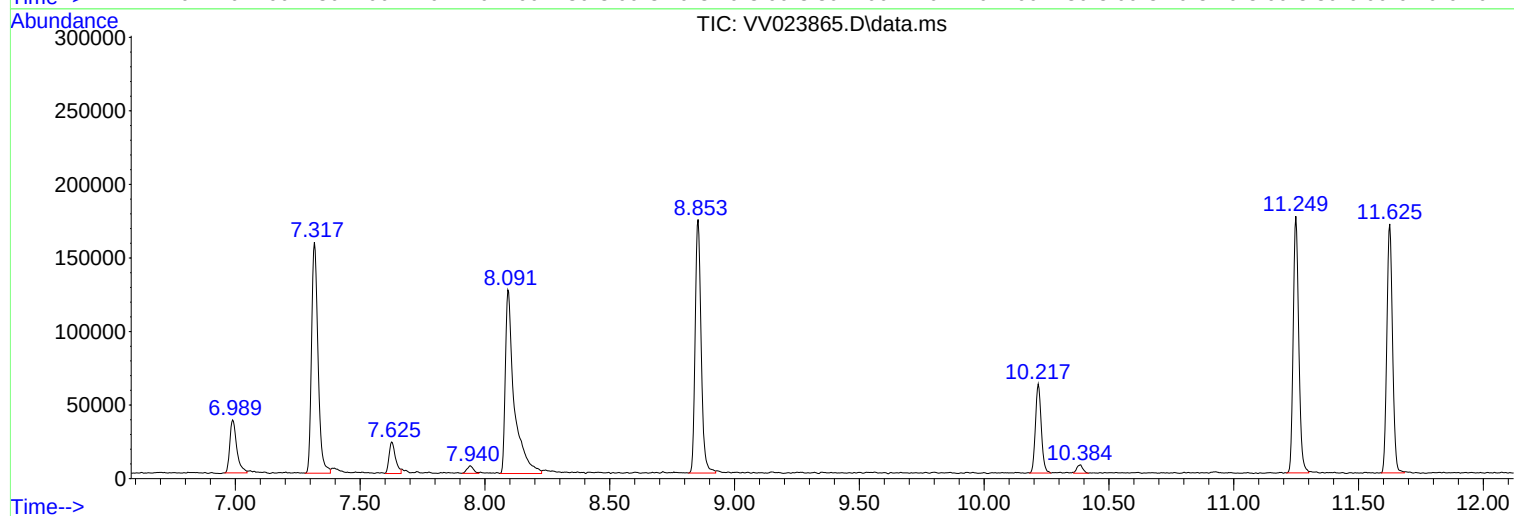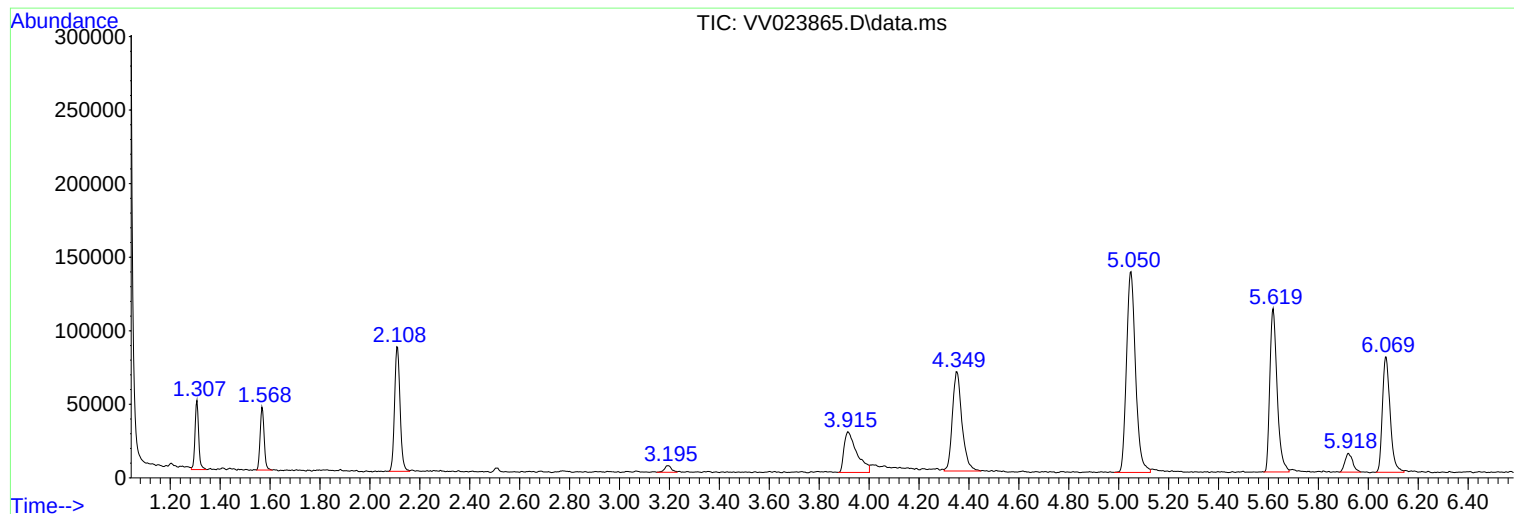

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023865.D
Acq On : 09 Dec 2021 16:42
Operator : SY/MD
Sample : M5002-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023865.D
Acq On : 09 Dec 2021 16:42
Operator : SY/MD
Sample : M5002-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
