

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
 Data File : VV023870.D
 Acq On : 09 Dec 2021 18:41
 Operator : SY/MD
 Sample : M5003-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CS6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	33	rVB	6820	7790	2.24%	0.261%
2	1.204	45	51	60	rBV	12794	12566	3.61%	0.422%
3	1.307	76	83	98	rVB	45574	49201	14.15%	1.651%
4	1.571	156	165	174	rBV	42632	49438	14.22%	1.659%
5	2.111	322	333	349	rVB	82194	121026	34.82%	4.062%
6	2.700	513	516	521	rBV	5053	3498	1.01%	0.117%
7	3.905	879	891	927	rBV	28333	124419	35.79%	4.176%
8	4.352	1013	1030	1051	rBV2	67970	169316	48.71%	5.683%
9	5.050	1229	1247	1278	rBV3	133685	347621	100.00%	11.668%
10	5.619	1413	1424	1450	rBV	113443	234543	67.47%	7.872%
11	6.069	1552	1564	1589	rBV	81035	169406	48.73%	5.686%
12	6.989	1840	1850	1865	rBV	40356	73583	21.17%	2.470%
13	7.317	1939	1952	1972	rBV	165340	290297	83.51%	9.744%
14	7.629	2039	2049	2066	rBV2	23175	43793	12.60%	1.470%
15	7.940	2137	2146	2156	rBV4	2222	4533	1.30%	0.152%
16	8.092	2181	2193	2228	rBV	165745	316335	91.00%	10.618%
17	8.854	2414	2430	2450	rBV	176796	295846	85.11%	9.930%
18	10.217	2843	2854	2868	rBV2	64175	99878	28.73%	3.352%
19	10.378	2898	2904	2914	rVB3	3868	6005	1.73%	0.202%
20	11.249	3163	3175	3192	rBV	180506	283774	81.63%	9.525%
21	11.625	3279	3292	3308	rBV	175543	276466	79.53%	9.279%




Sum of corrected areas: 2979334

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023870.D
Acq On : 09 Dec 2021 18:41
Operator : SY/MD
Sample : M5003-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

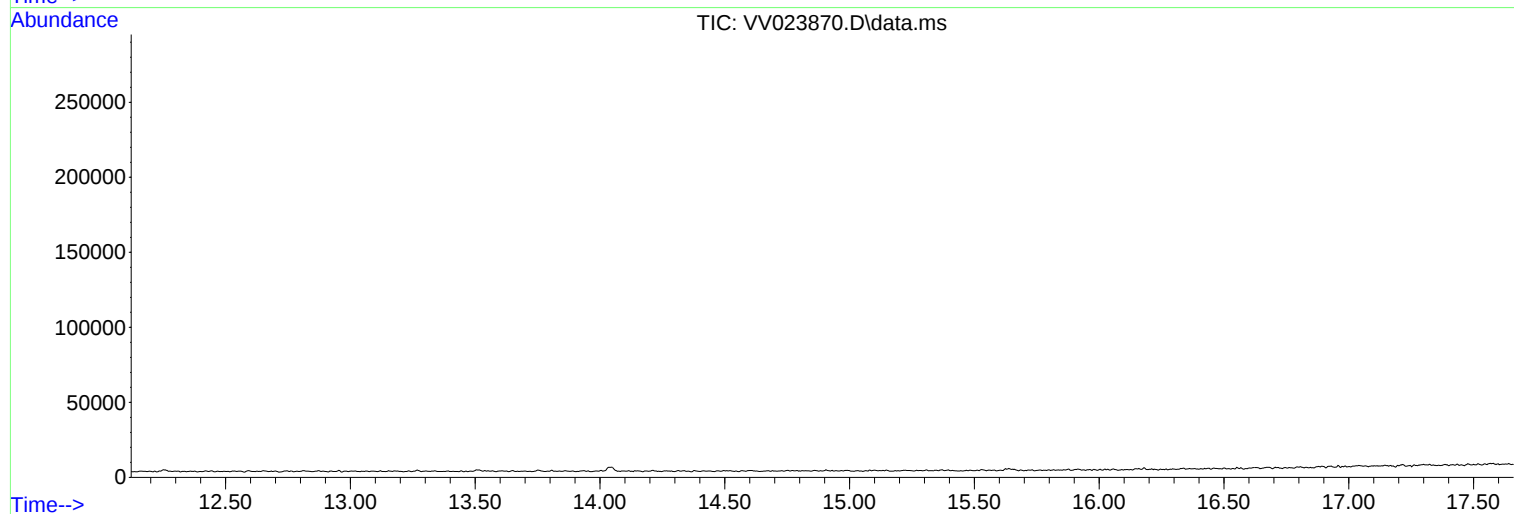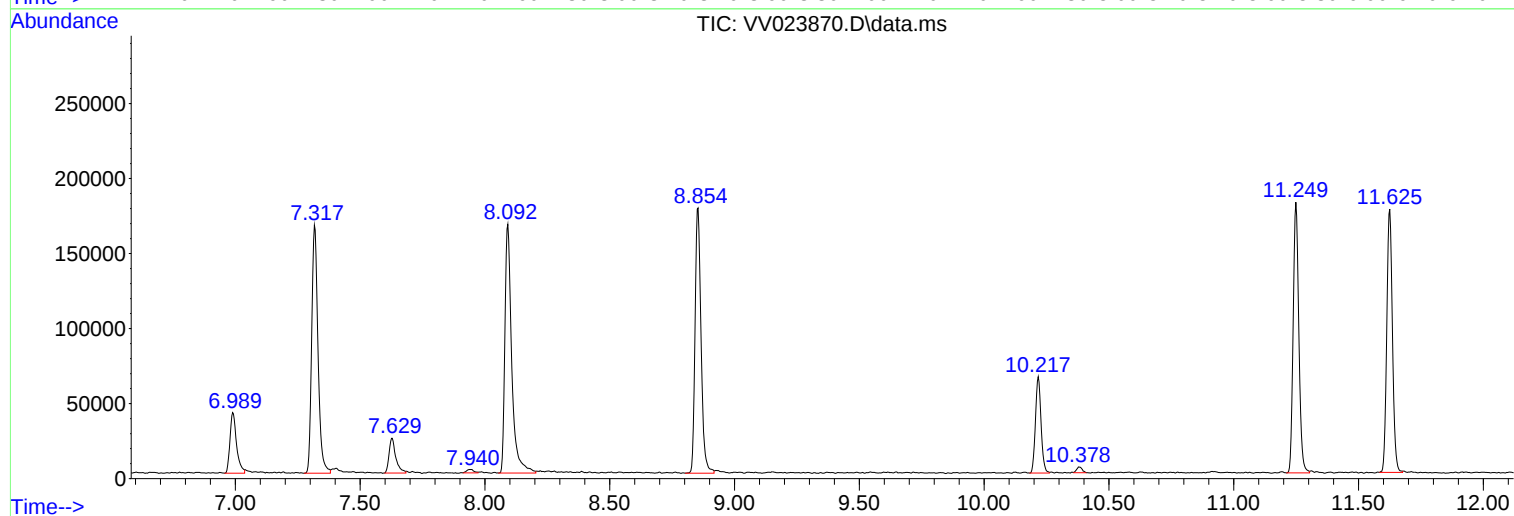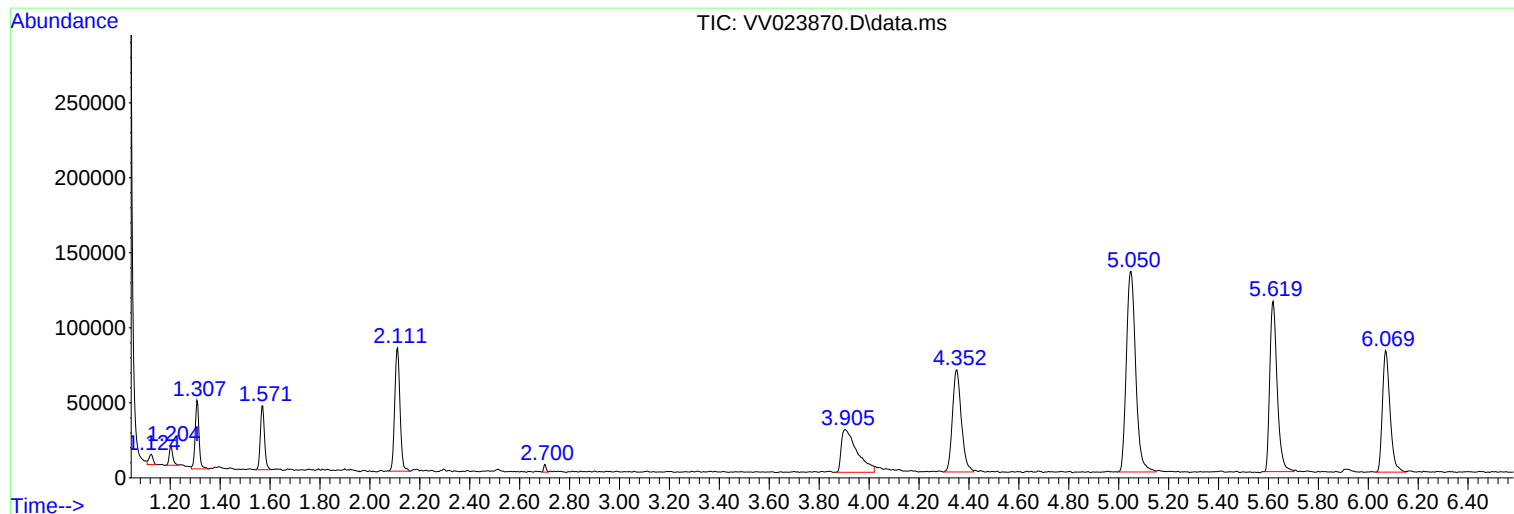

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023870.D
Acq On : 09 Dec 2021 18:41
Operator : SY/MD
Sample : M5003-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023870.D
Acq On : 09 Dec 2021 18:41
Operator : SY/MD
Sample : M5003-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
