

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
 Data File : VV023871.D
 Acq On : 09 Dec 2021 19:05
 Operator : SY/MD
 Sample : M5003-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CT2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023871.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	58	rVB2	8671	8686	2.51%	0.297%
2	1.307	74	83	92	rVB	46488	47759	13.79%	1.630%
3	1.568	156	164	175	rBV	42513	48611	14.04%	1.659%
4	2.108	322	332	348	rBV	81339	120706	34.85%	4.120%
5	3.912	882	893	925	rBV2	22258	101427	29.29%	3.462%
6	4.352	1014	1030	1053	rBV2	64924	160694	46.40%	5.486%
7	5.050	1230	1247	1279	rBV3	133639	346337	100.00%	11.823%
8	5.619	1413	1424	1445	rBV	117796	236740	68.36%	8.082%
9	6.069	1550	1564	1591	rBV2	79064	170331	49.18%	5.815%
10	6.989	1838	1850	1869	rBV2	36510	72660	20.98%	2.480%
11	7.317	1941	1952	1971	rBV	160669	279917	80.82%	9.555%
12	7.397	1974	1977	1988	rVB4	2942	3903	1.13%	0.133%
13	7.625	2037	2048	2064	rBV2	23642	43267	12.49%	1.477%
14	7.940	2136	2146	2158	rBV5	3370	6113	1.77%	0.209%
15	8.091	2183	2193	2229	rBV	155764	313919	90.64%	10.716%
16	8.853	2417	2430	2460	rBV	176280	295331	85.27%	10.082%
17	10.217	2844	2854	2871	rBV	61308	96897	27.98%	3.308%
18	10.387	2896	2907	2915	rBV4	5593	9198	2.66%	0.314%
19	11.249	3163	3175	3193	rBV	180768	285089	82.32%	9.732%
20	11.625	3281	3292	3307	rBV	173045	275893	79.66%	9.418%
21	14.040	4033	4043	4054	rBV3	3502	5927	1.71%	0.202%




Sum of corrected areas: 2929405

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023871.D
Acq On : 09 Dec 2021 19:05
Operator : SY/MD
Sample : M5003-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

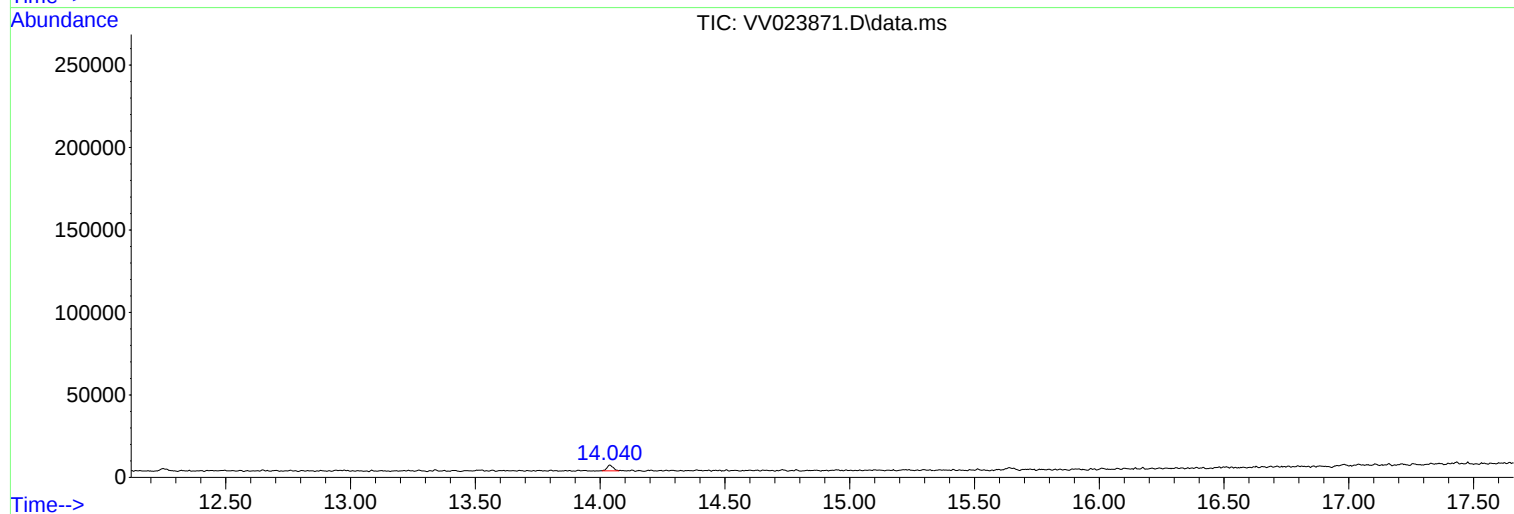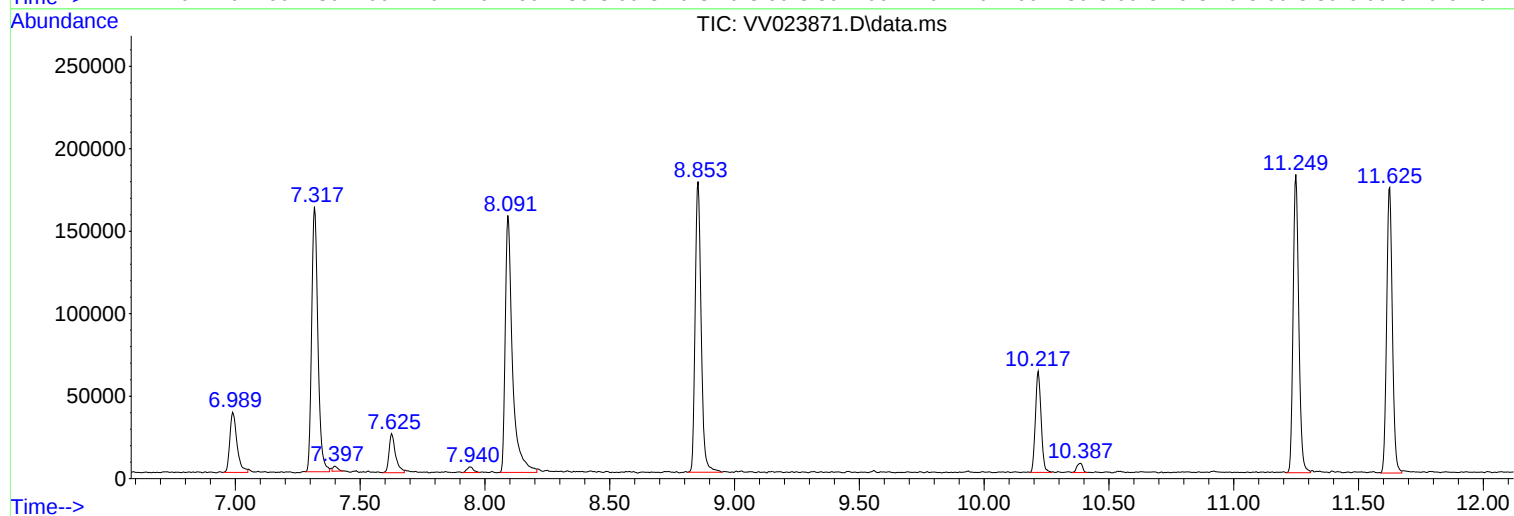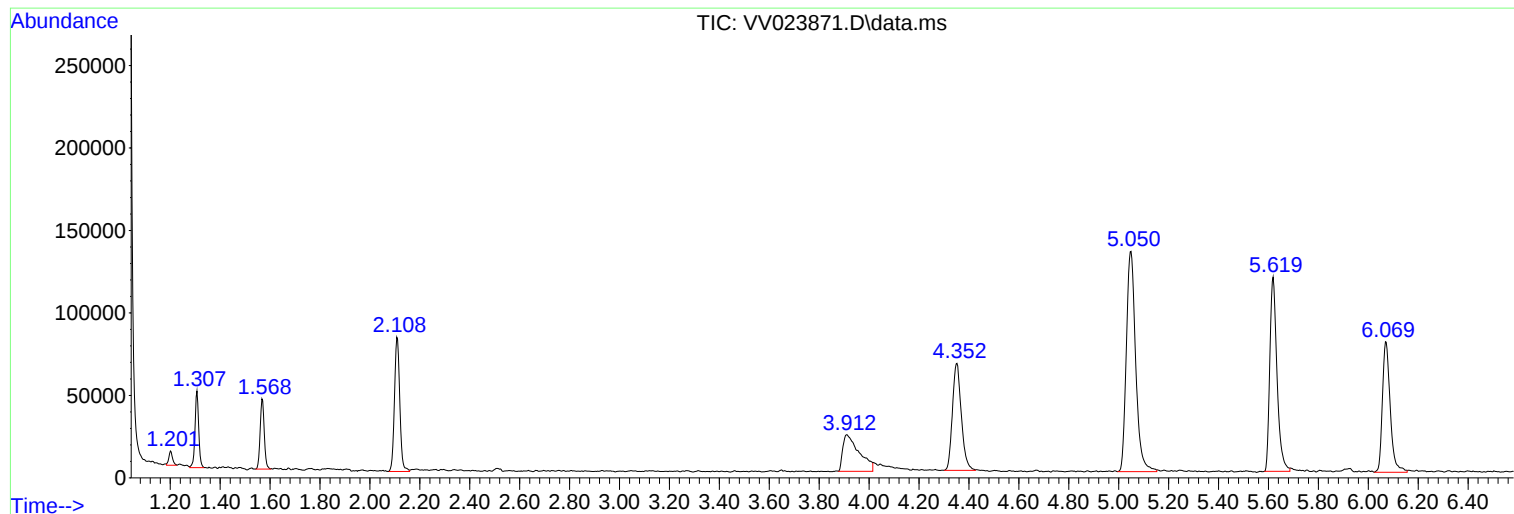

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023871.D
Acq On : 09 Dec 2021 19:05
Operator : SY/MD
Sample : M5003-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023871.D
Acq On : 09 Dec 2021 19:05
Operator : SY/MD
Sample : M5003-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc