

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
 Data File : VV023872.D
 Acq On : 09 Dec 2021 19:29
 Operator : SY/MD
 Sample : M5003-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0CT5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023872.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	44	50	59	rVB	63773	56095	16.77%	1.969%
2	1.307	75	83	96	rVB	45178	46551	13.92%	1.634%
3	1.568	155	164	179	rVB	41854	49363	14.76%	1.733%
4	2.108	321	332	344	rBV	79581	114521	34.24%	4.020%
5	3.912	883	893	910	rBV	17042	55469	16.58%	1.947%
6	4.349	1014	1029	1048	rVB	65641	158387	47.35%	5.559%
7	5.047	1228	1246	1272	rBV2	132276	334481	100.00%	11.740%
8	5.616	1413	1423	1444	rBV	111377	229586	68.64%	8.058%
9	6.072	1551	1565	1579	rBV	78686	160296	47.92%	5.626%
10	6.989	1840	1850	1874	rBV	37024	72336	21.63%	2.539%
11	7.317	1938	1952	1972	rBV	156464	276685	82.72%	9.711%
12	7.397	1973	1977	1988	rVB7	3050	4846	1.45%	0.170%
13	7.625	2040	2048	2065	rBV3	20917	40884	12.22%	1.435%
14	7.941	2135	2146	2155	rVB3	3782	6960	2.08%	0.244%
15	8.092	2183	2193	2231	rBV	126650	302424	90.42%	10.615%
16	8.854	2417	2430	2452	rBV	174347	286603	85.69%	10.060%
17	10.217	2842	2854	2871	rBV2	60675	98650	29.49%	3.463%
18	10.381	2894	2905	2916	rVB3	5696	9678	2.89%	0.340%
19	11.249	3163	3175	3194	rBV	177128	277974	83.11%	9.757%
20	11.625	3281	3292	3308	rBV	166382	261728	78.25%	9.186%
21	14.040	4033	4043	4052	rBV2	3800	5545	1.66%	0.195%




Sum of corrected areas: 2849062

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023872.D
Acq On : 09 Dec 2021 19:29
Operator : SY/MD
Sample : M5003-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

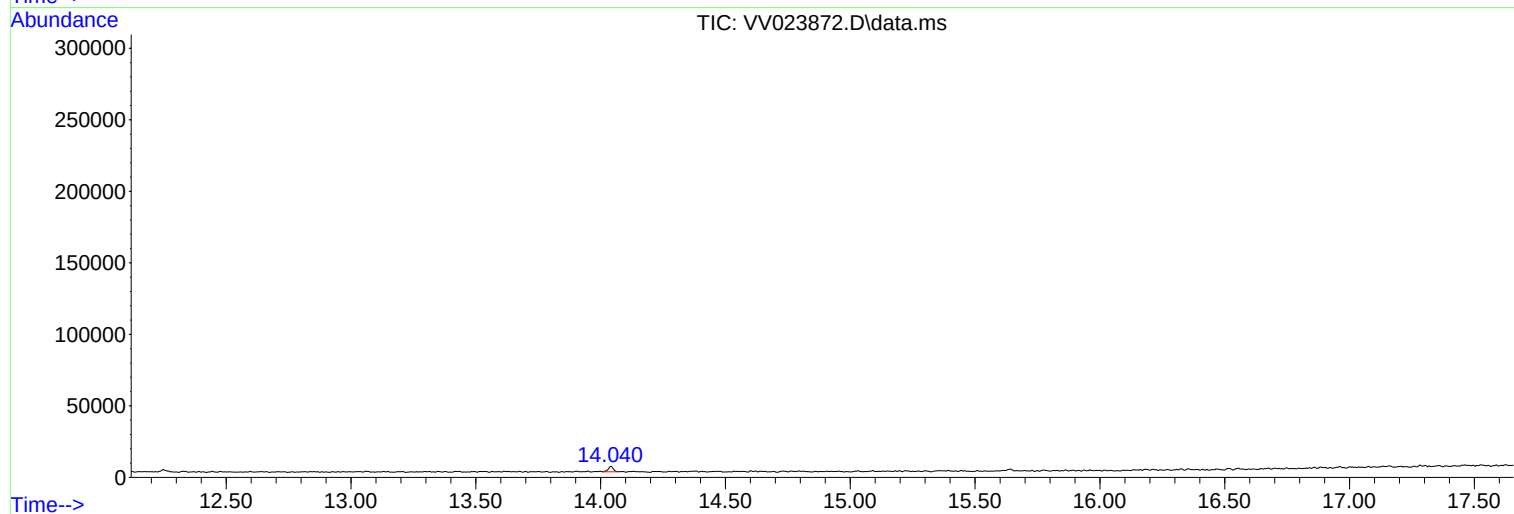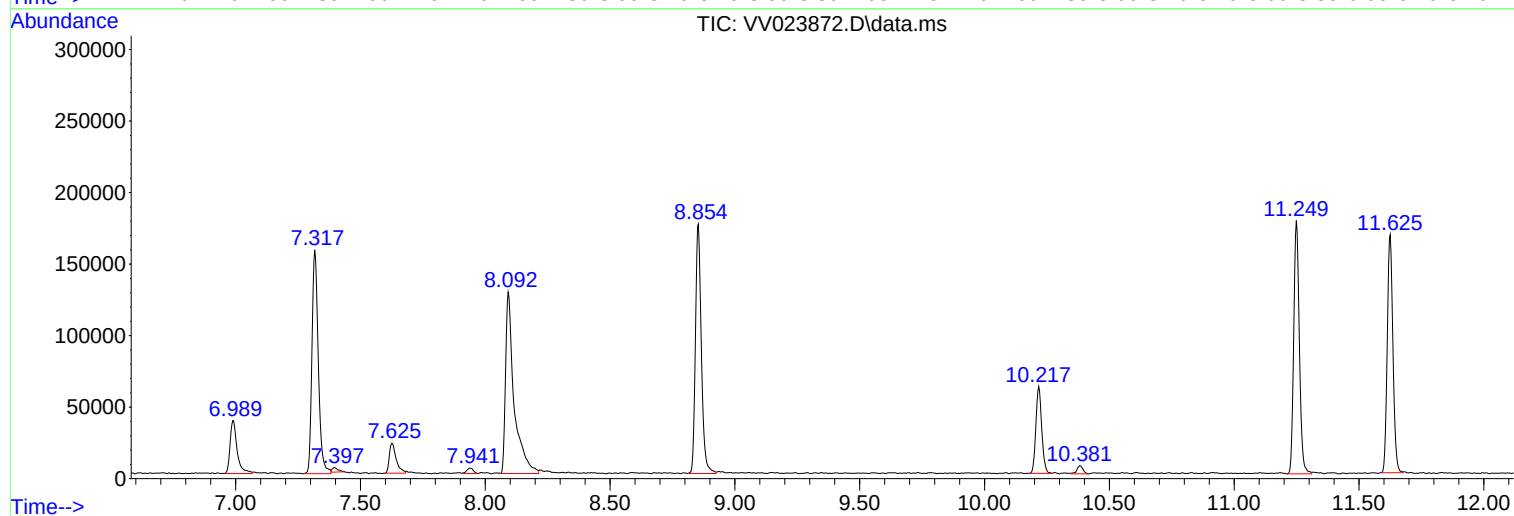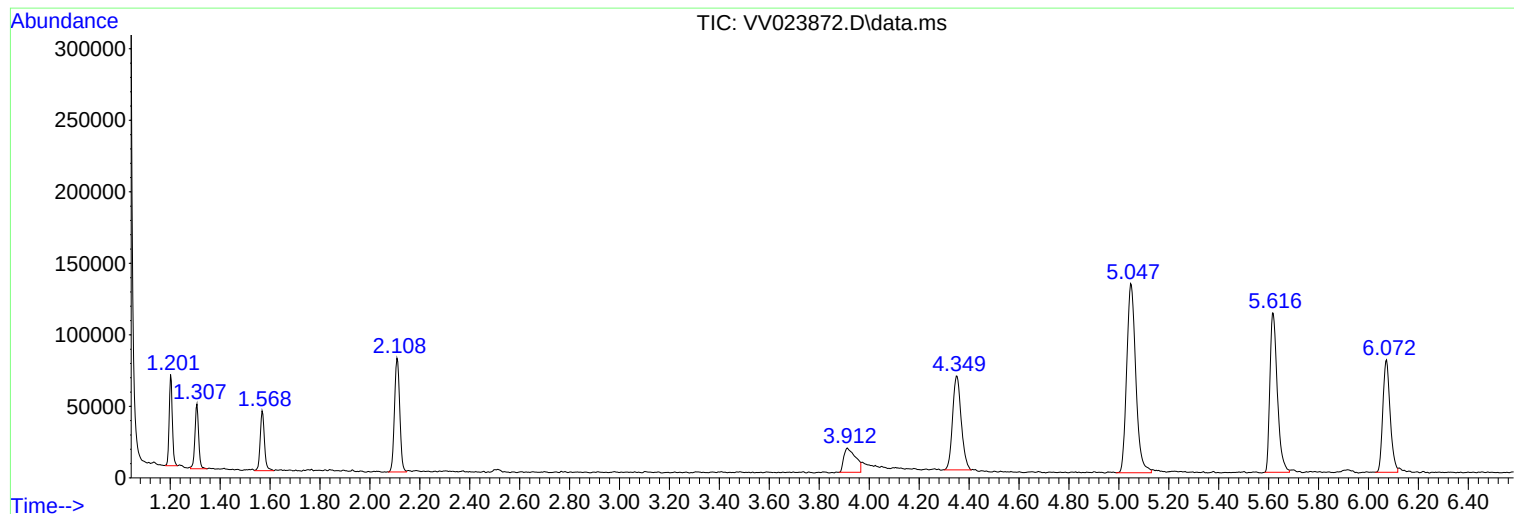

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023872.D
Acq On : 09 Dec 2021 19:29
Operator : SY/MD
Sample : M5003-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
Data File : VV023872.D
Acq On : 09 Dec 2021 19:29
Operator : SY/MD
Sample : M5003-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0CT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------