
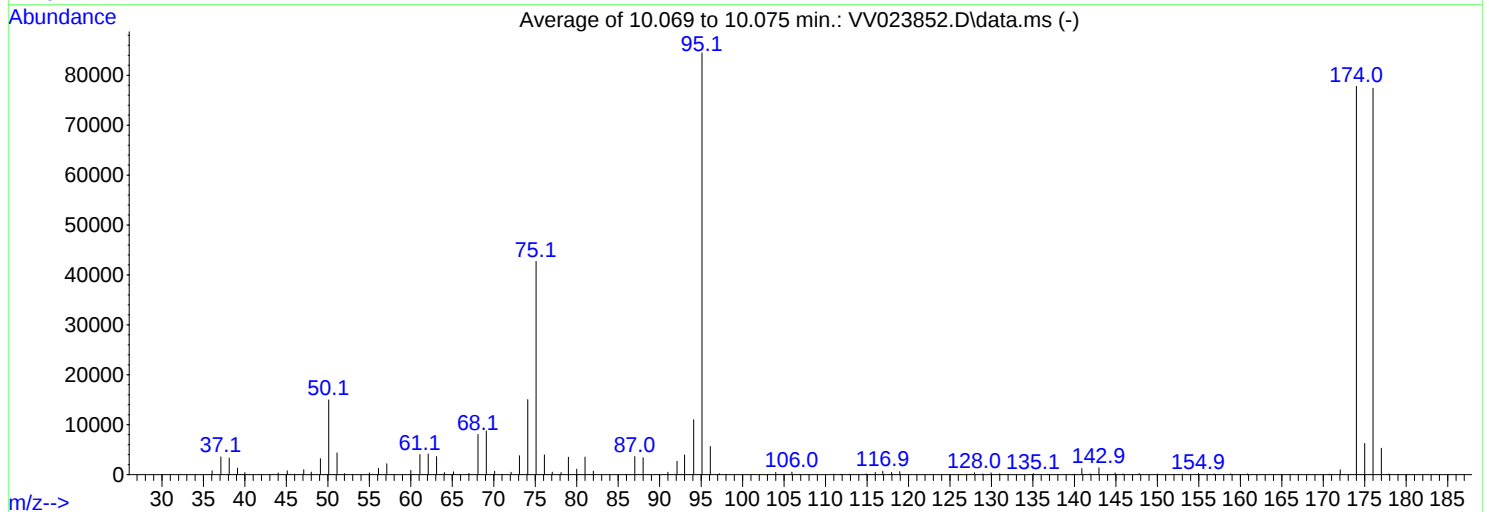


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120921\
 Data File : VV023852.D
 Acq On : 09 Dec 2021 09:20
 Operator : SY/MD
 Sample : BFB248
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB248

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR112321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Dec 02 02:08:23 2021

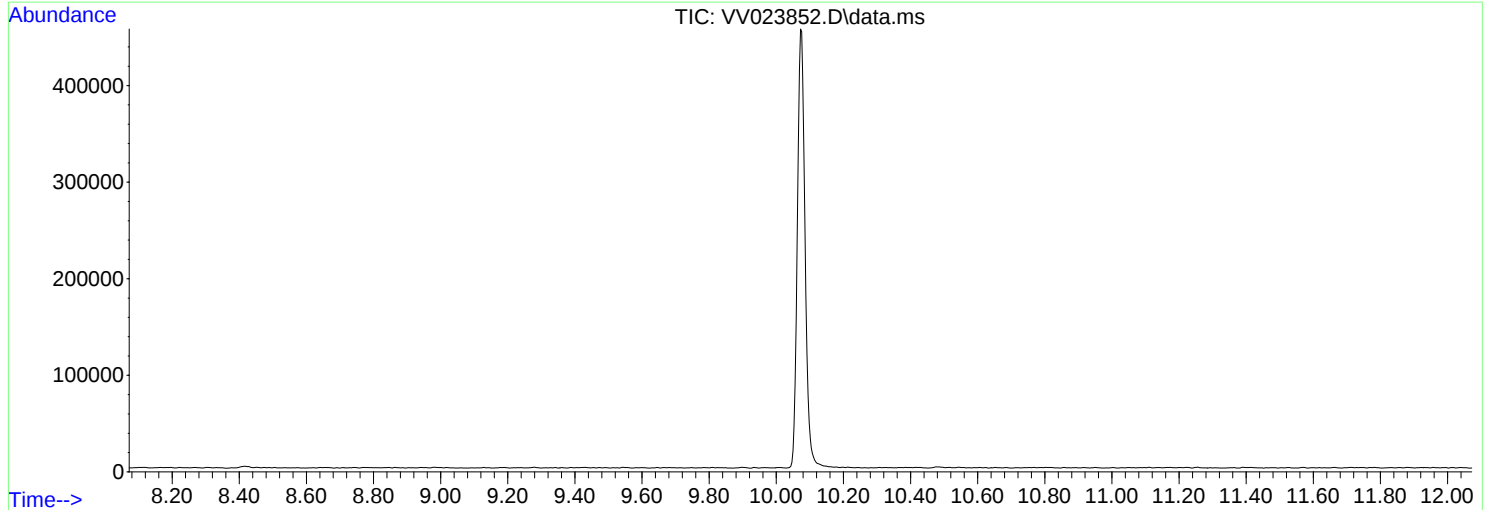

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	14974	PASS
75	95	30	80	50.6	42709	PASS
95	95	100	100	100.0	84483	PASS
96	95	5	9	6.7	5628	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.1	77771	PASS
175	174	5	9	8.0	6249	PASS
176	174	95	105	99.5	77411	PASS
177	176	5	10	6.8	5300	PASS

Scan 2796 (10.030 min): VV023852.D\data.ms
BFB248

m/z	Abundance
40.00	3799.0
44.00	223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248

m/z	Abundance
36.10	765.0
37.10	3688.0
38.10	3475.0
39.10	1342.0
40.00	4245.0
44.00	569.0
45.10	814.0
46.00	134.0
47.10	1063.0
48.00	559.0
49.10	3276.0
50.10	15470.0
51.10	4506.0
52.00	241.0
53.00	106.0
55.00	367.0
56.10	1293.0
57.10	2261.0
60.00	878.0
61.10	4128.0
62.10	4295.0
63.10	3715.0
64.10	449.0
65.10	596.0
67.00	254.0
68.10	8199.0
69.10	9117.0
70.10	703.0
72.10	461.0
73.10	3929.0
74.10	15521.0
75.10	44408.0
76.10	4140.0
77.00	541.0
78.10	442.0
79.00	3647.0
80.00	1134.0
81.00	3666.0
82.00	692.0
85.90	100.0
87.00	3712.0
88.00	3561.0
91.00	501.0
92.10	2791.0
93.00	4069.0
94.10	11337.0
95.10	87672.0
96.10	5791.0
97.20	196.0
104.00	473.0
105.00	130.0
105.90	535.0
111.00	127.0
111.90	118.0
112.90	112.0
114.90	170.0
116.00	444.0
116.90	671.0
117.90	457.0
118.90	632.0
127.90	395.0
128.90	152.0
129.90	386.0
131.00	202.0
135.10	236.0
136.80	159.0
140.00	120.0
140.90	1256.0
141.90	177.0
143.00	1436.0
144.90	359.0
145.80	157.0
147.80	247.0
150.00	149.0
153.00	145.0
154.90	245.0
156.90	158.0
158.80	167.0
160.80	169.0
170.70	164.0
172.10	974.0
174.00	80152.0
175.00	6469.0
176.00	80152.0
177.00	5529.0
177.90	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248

m/z	Abundance
36.00	757.0
37.10	3616.0
38.10	3446.0
39.10	1408.0
40.00	4201.0
44.00	575.0
45.10	758.0
45.90	153.0
47.10	1003.0
48.00	486.0
49.10	3407.0
50.10	15197.0
51.10	4455.0
52.00	248.0
55.00	356.0
56.10	1293.0
57.10	2194.0
60.00	876.0
61.10	3917.0
62.10	4116.0
63.10	3780.0
64.00	406.0
65.10	564.0
65.90	127.0
67.00	262.0
68.10	8307.0
69.10	8709.0
70.10	629.0
72.10	465.0
73.10	3830.0
74.10	15246.0
75.10	43384.0
76.10	3768.0
77.10	492.0
78.10	408.0
79.00	3561.0
80.00	1103.0
81.00	3478.0
82.00	743.0
87.00	3676.0
88.00	3638.0
91.00	430.0
92.10	2771.0
93.00	4076.0
94.10	11328.0
95.10	86392.0
96.10	5720.0
97.20	205.0
103.90	505.0
105.00	156.0
106.00	515.0
110.90	109.0
111.80	112.0
112.90	106.0
114.90	161.0
116.00	448.0
116.90	686.0
117.90	483.0
118.90	693.0
127.90	438.0
129.00	191.0
129.90	351.0
131.00	154.0
135.10	227.0
137.00	170.0
140.10	145.0
140.90	1220.0
141.90	187.0
143.00	1457.0
144.20	104.0
144.90	372.0
145.90	161.0
147.80	201.0
150.00	134.0
153.00	131.0
154.90	264.0
156.90	202.0
158.90	166.0
160.80	167.0
170.90	157.0
172.00	958.0
174.00	81408.0
175.00	6591.0
176.00	81040.0
177.00	5217.0
177.90	159.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248

m/z	Abundance
36.00	758.0
37.10	3382.0
38.10	3117.0
39.10	1184.0
40.00	4162.0
44.00	607.0
45.10	697.0
46.10	115.0
47.10	958.0
48.00	525.0
49.10	2954.0
50.10	14254.0
51.10	4164.0
52.00	206.0
53.00	102.0
55.00	306.0
56.10	1214.0
57.10	2091.0
58.00	102.0
60.00	830.0
61.10	4063.0
62.10	4019.0
63.10	3358.0
64.10	429.0
65.20	607.0
67.00	219.0
68.10	7616.0
69.10	8412.0
70.10	703.0
72.10	492.0
73.10	3598.0
74.10	14348.0
75.10	40336.0
76.10	3979.0
77.00	531.0
78.10	435.0
79.00	3274.0
80.00	1020.0
81.00	3402.0
82.00	703.0
85.90	105.0
87.00	3452.0
88.00	3042.0
91.00	477.0
92.10	2493.0
93.00	3647.0
94.10	10305.0
95.10	79384.0
96.10	5373.0
97.20	175.0
103.00	108.0
104.10	409.0
105.90	480.0
106.90	104.0
111.00	144.0
111.80	111.0
112.80	122.0
114.90	158.0
116.00	423.0
116.90	645.0
118.00	380.0
119.00	513.0
128.00	339.0
129.00	129.0
130.00	366.0
131.00	208.0
135.00	221.0
136.80	151.0
139.80	115.0
140.90	1177.0
141.90	131.0
142.90	1251.0
144.90	318.0
145.80	148.0
147.80	246.0
150.00	122.0
153.00	116.0
155.00	224.0
156.80	150.0
158.80	144.0
160.90	155.0
170.70	111.0
172.10	956.0
174.00	71752.0
175.00	5688.0
176.00	71040.0
177.00	5155.0
177.90	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB248