

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029515.D
 Acq On : 09 Dec 2022 12:49
 Operator : SY/MD
 Sample : N5919-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Dec 09 23:50:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 09 23:48:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	463333	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	424368	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	222211	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	150221	52.946	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	105.900%
7) Chloroethane-d5	1.564	69	118545	54.793	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	109.580%
11) 1,1-Dichloroethene-d2	2.105	63	184066	41.594	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.180%
21) 2-Butanone-d5	3.870	46	192538	111.242	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	111.240%
24) Chloroform-d	4.339	84	267733	50.145	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.280%
26) 1,2-Dichloroethane-d4	5.024	65	164450	53.929	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.860%
32) Benzene-d6	5.043	84	586676	52.320	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.640%
36) 1,2-Dichloropropane-d6	6.063	67	176916	51.652	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	103.300%
41) Toluene-d8	7.307	98	528715	50.042	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.080%
43) trans-1,3-Dichloroprop...	7.612	79	74051	42.815	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.620%
47) 2-Hexanone-d5	8.082	63	170169	116.346	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	116.350%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	250386	51.157	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	102.320%
66) 1,2-Dichlorobenzene-d4	11.612	152	213502	50.473	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.940%
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.616	75	3156	0.702	ug/L	# 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029515.D
Acq On : 09 Dec 2022 12:49
Operator : SY/MD
Sample : N5919-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Dec 09 23:50:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 09 23:48:53 2022
Response via : Initial Calibration

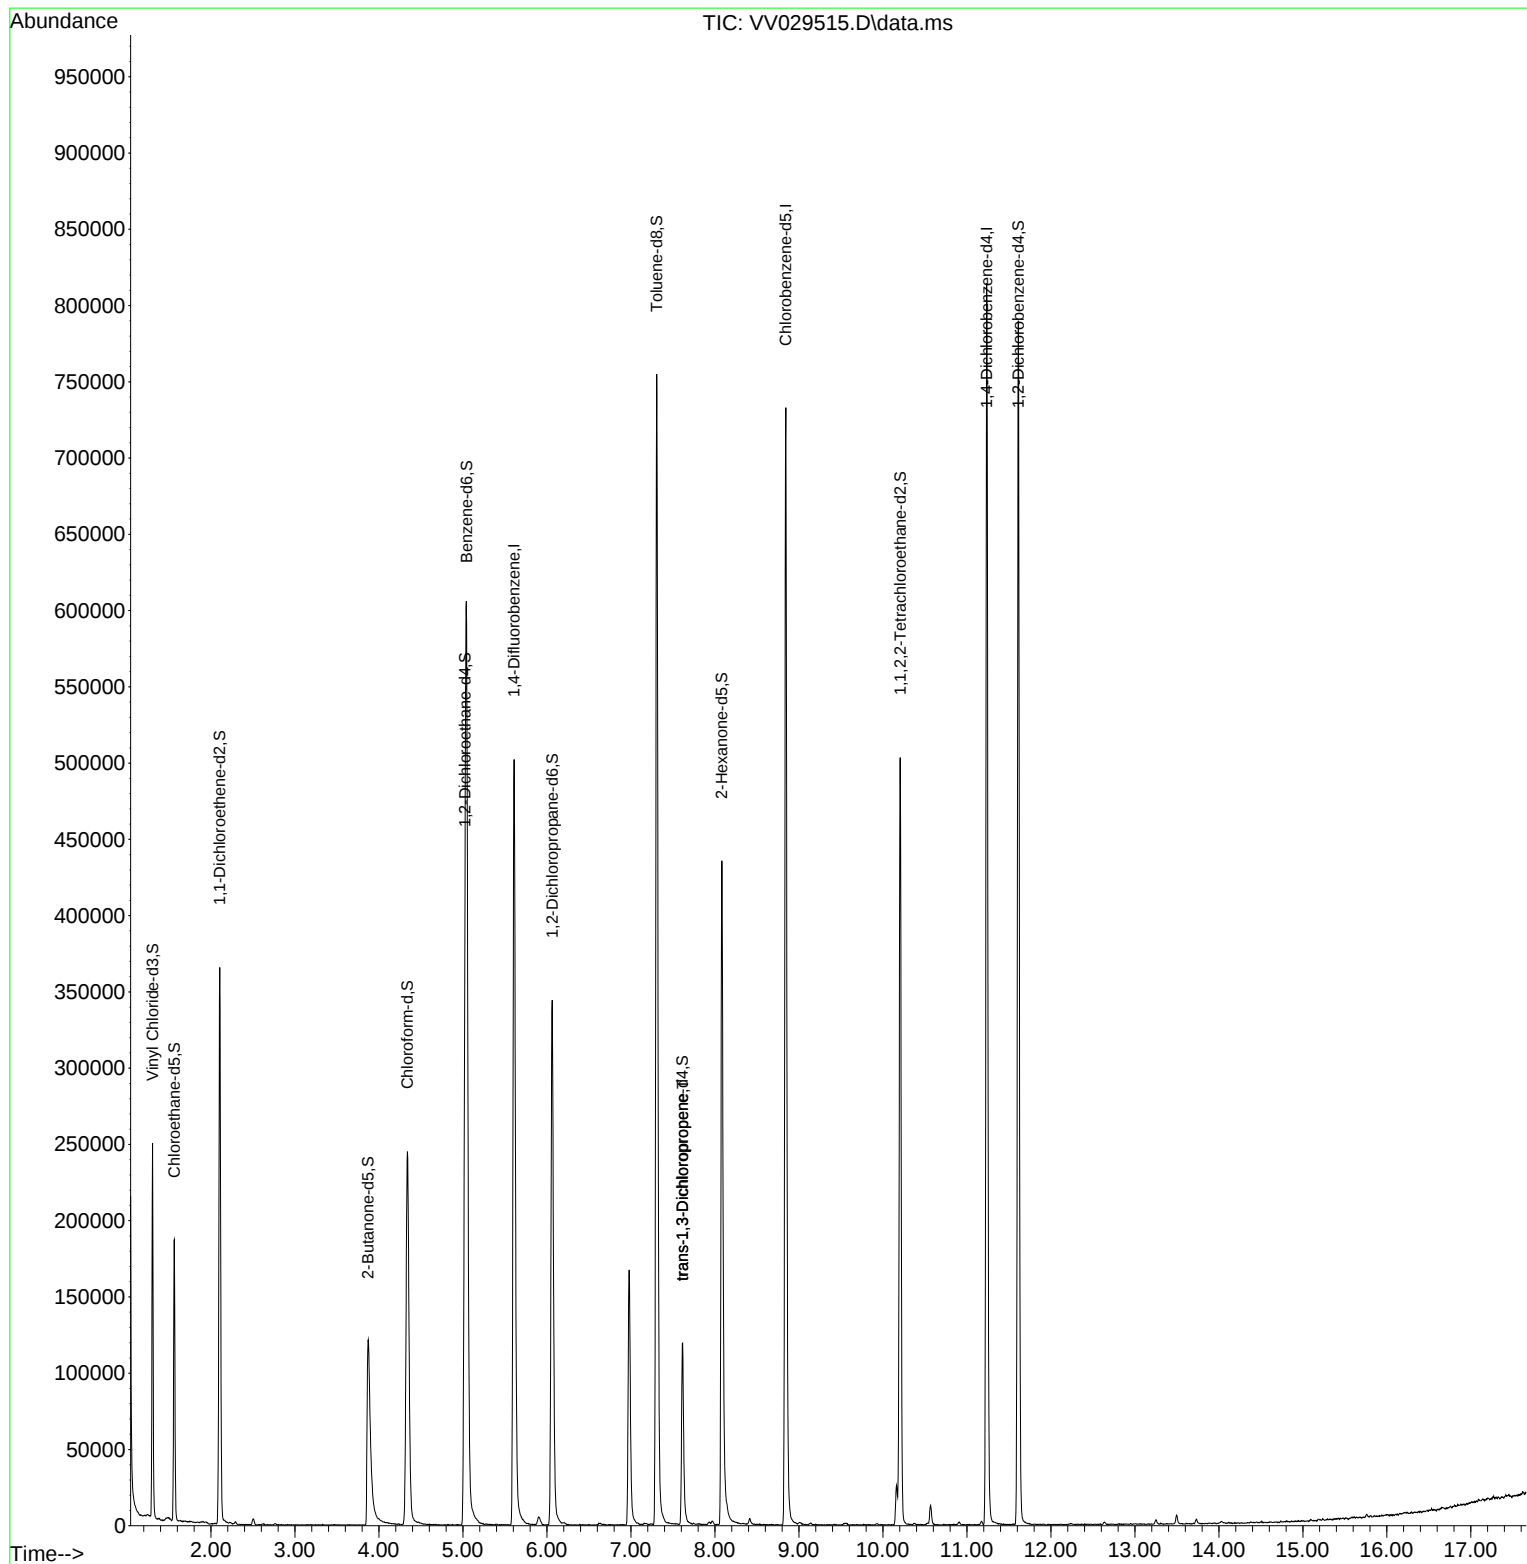

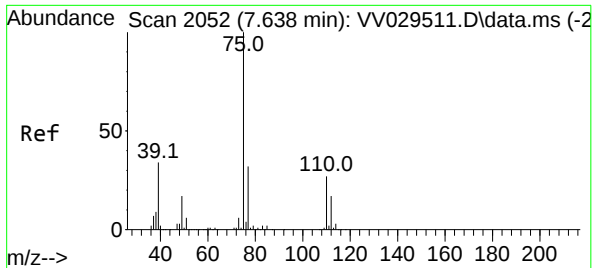

#44
 trans-1,3-Dichloropropene
 Concen: 0.702 ug/L
 RT: 7.616 min Scan# 2045
 Delta R.T. -0.023 min
 Lab File: VV029515.D
 Acq: 09 Dec 2022 12:49

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 3156
 Ion Ratio Lower Upper
 75 100
 77 45.4 22.3 41.5#

