

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029545.D
 Acq On : 10 Dec 2022 00:45
 Operator : SY/MD
 Sample : N5915-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N05

Quant Time: Dec 10 01:11:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 10 00:41:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	498924	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	458770	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	241321	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	134107	43.895	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	87.780%		
7) Chloroethane-d5	1.565	69	114698	49.233	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	98.460%		
11) 1,1-Dichloroethene-d2	2.105	63	177121	37.169	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.340%		
21) 2-Butanone-d5	3.870	46	207265	111.208	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	111.210%		
24) Chloroform-d	4.339	84	260286	45.273	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.540%		
26) 1,2-Dichloroethane-d4	5.024	65	154155	46.946	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.900%		
32) Benzene-d6	5.043	84	562552	46.406	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.820%		
36) 1,2-Dichloropropane-d6	6.063	67	171191	46.233	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.460%		
41) Toluene-d8	7.307	98	504672	44.185	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.360%		
43) trans-1,3-Dichloroprop...	7.612	79	67243	35.963	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.920%		
47) 2-Hexanone-d5	8.082	63	184800	116.875	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	116.870%		
56) 1,1,2,2-Tetrachloroeth...	10.204	84	250572	47.356	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.720%		
66) 1,2-Dichlorobenzene-d4	11.612	152	208264	45.336	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.680%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.979	75	3881	0.756	ug/L	# 57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029545.D
Acq On : 10 Dec 2022 00:45
Operator : SY/MD
Sample : N5915-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N05

Quant Time: Dec 10 01:11:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 10 00:41:04 2022
Response via : Initial Calibration

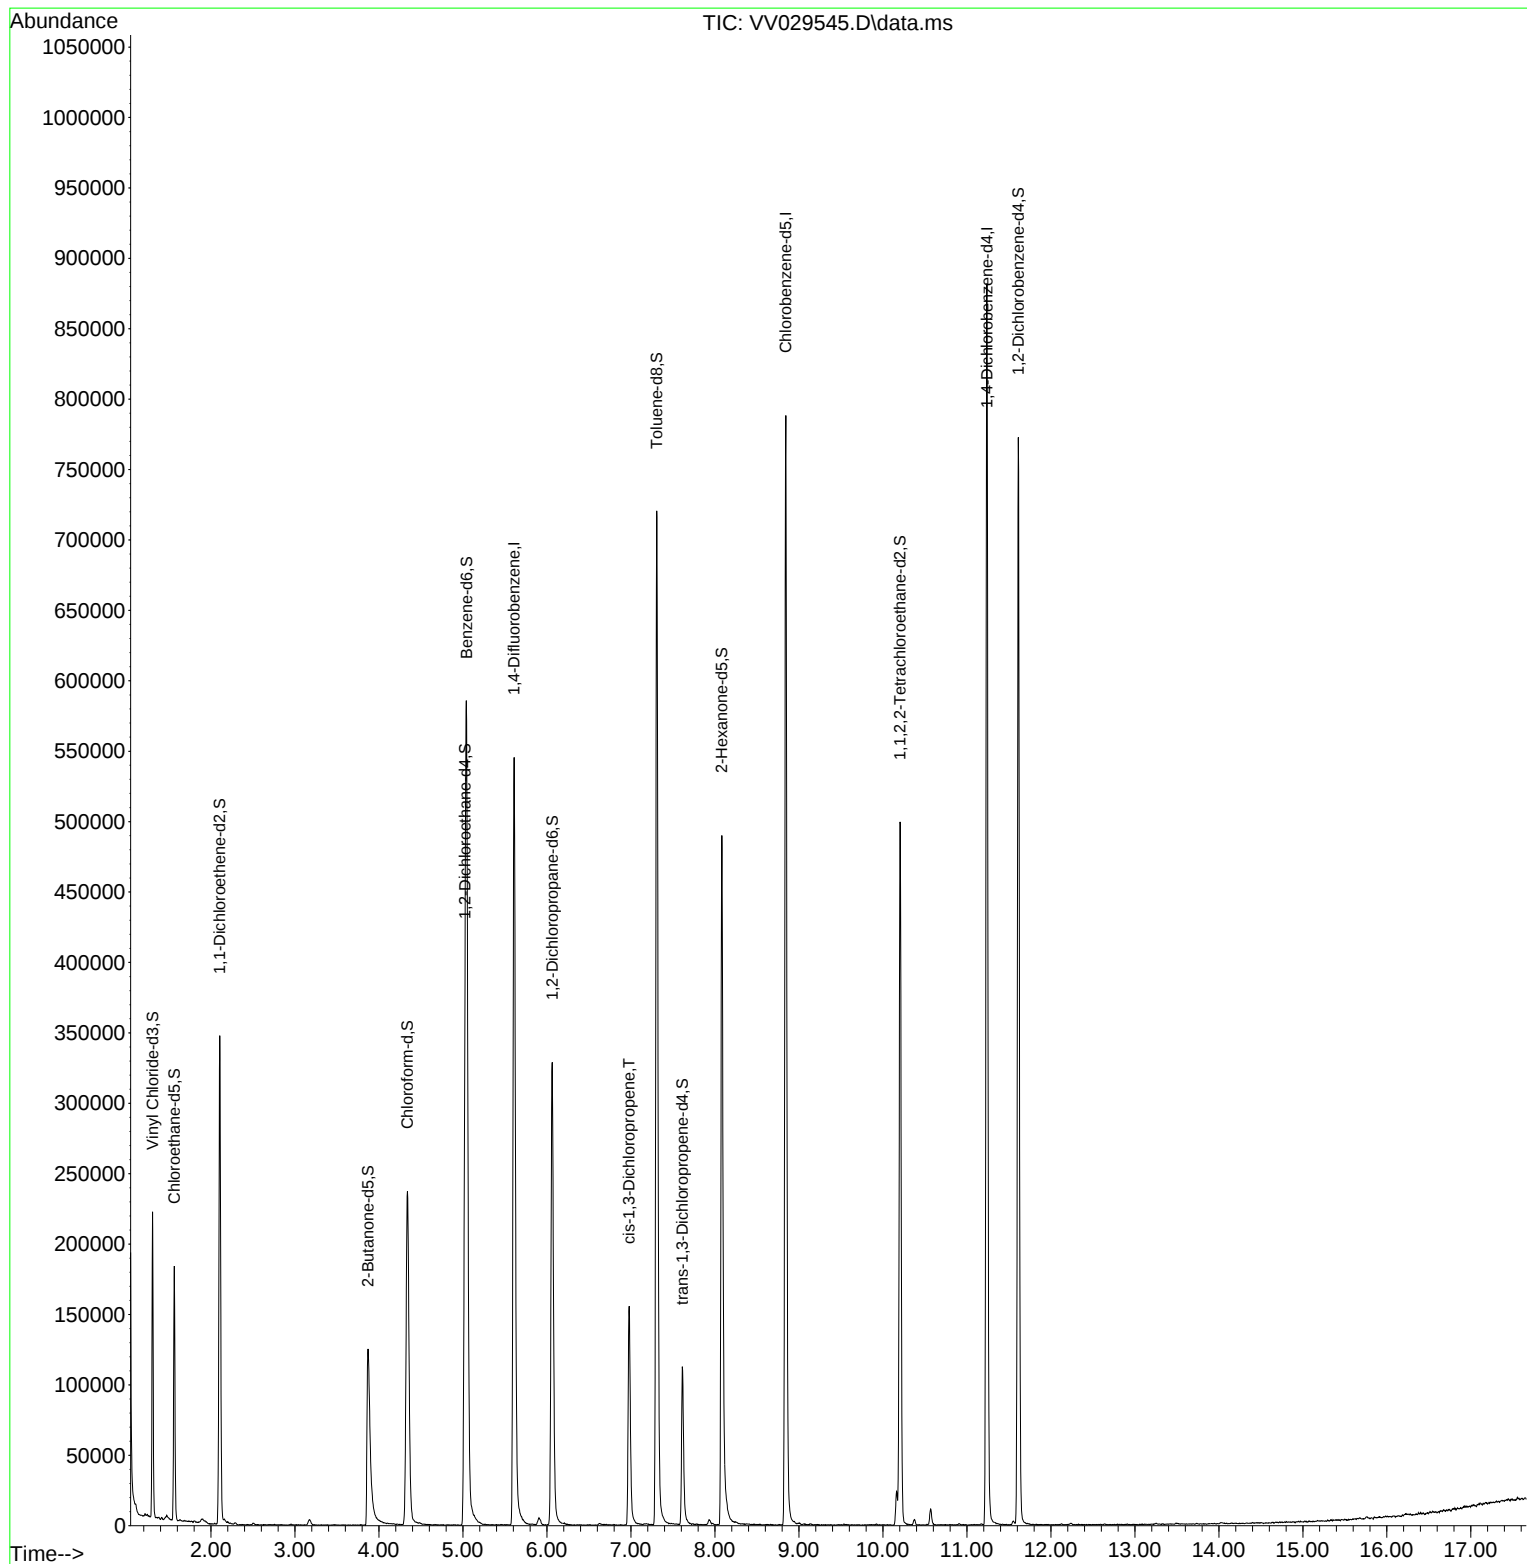

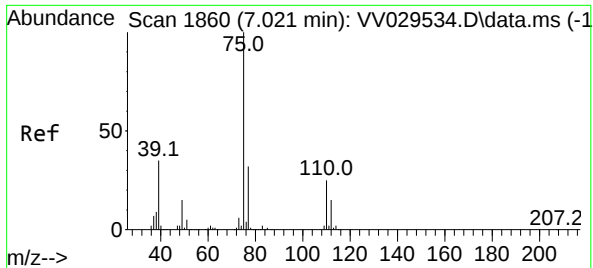

#39
 cis-1,3-Dichloropropene
 Concen: 0.756 ug/L
 RT: 6.979 min Scan# 11
 Delta R.T. -0.042 min
 Lab File: VV029545.D
 Acq: 10 Dec 2022 00:45

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N05

Tgt Ion: 75 Resp: 3881
 Ion Ratio Lower Upper
 75 100
 77 54.9 21.9 40.7#

