

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029548.D
 Acq On : 10 Dec 2022 01:56
 Operator : SY/MD
 Sample : N5915-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N15

Quant Time: Dec 10 02:49:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 10 00:41:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	514847	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	473566	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	244866	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	134146	42.549	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	85.100%		
7) Chloroethane-d5	1.564	69	114991	47.833	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	95.660%		
11) 1,1-Dichloroethene-d2	2.105	63	178140	36.227	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	72.460%		
21) 2-Butanone-d5	3.873	46	189767	98.671	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.670%		
24) Chloroform-d	4.339	84	255968	43.145	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.280%		
26) 1,2-Dichloroethane-d4	5.024	65	156615	46.221	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.440%		
32) Benzene-d6	5.043	84	562609	44.961	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.920%		
36) 1,2-Dichloropropane-d6	6.063	67	171683	44.917	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	89.840%		
41) Toluene-d8	7.307	98	504529	42.792	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.580%		
43) trans-1,3-Dichloroprop...	7.612	79	68010	35.237	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	70.480%		
47) 2-Hexanone-d5	8.082	63	160584	98.387	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.390%		
56) 1,1,2,2-Tetrachloroeth...	10.207	84	241963	44.300	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.600%		
66) 1,2-Dichlorobenzene-d4	11.612	152	204319	43.833	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.660%		
Target Compounds					Qvalue	
13) Acetone	2.163	43	2844	2.270	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029548.D
Acq On : 10 Dec 2022 01:56
Operator : SY/MD
Sample : N5915-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N15

Quant Time: Dec 10 02:49:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 10 00:41:04 2022
Response via : Initial Calibration

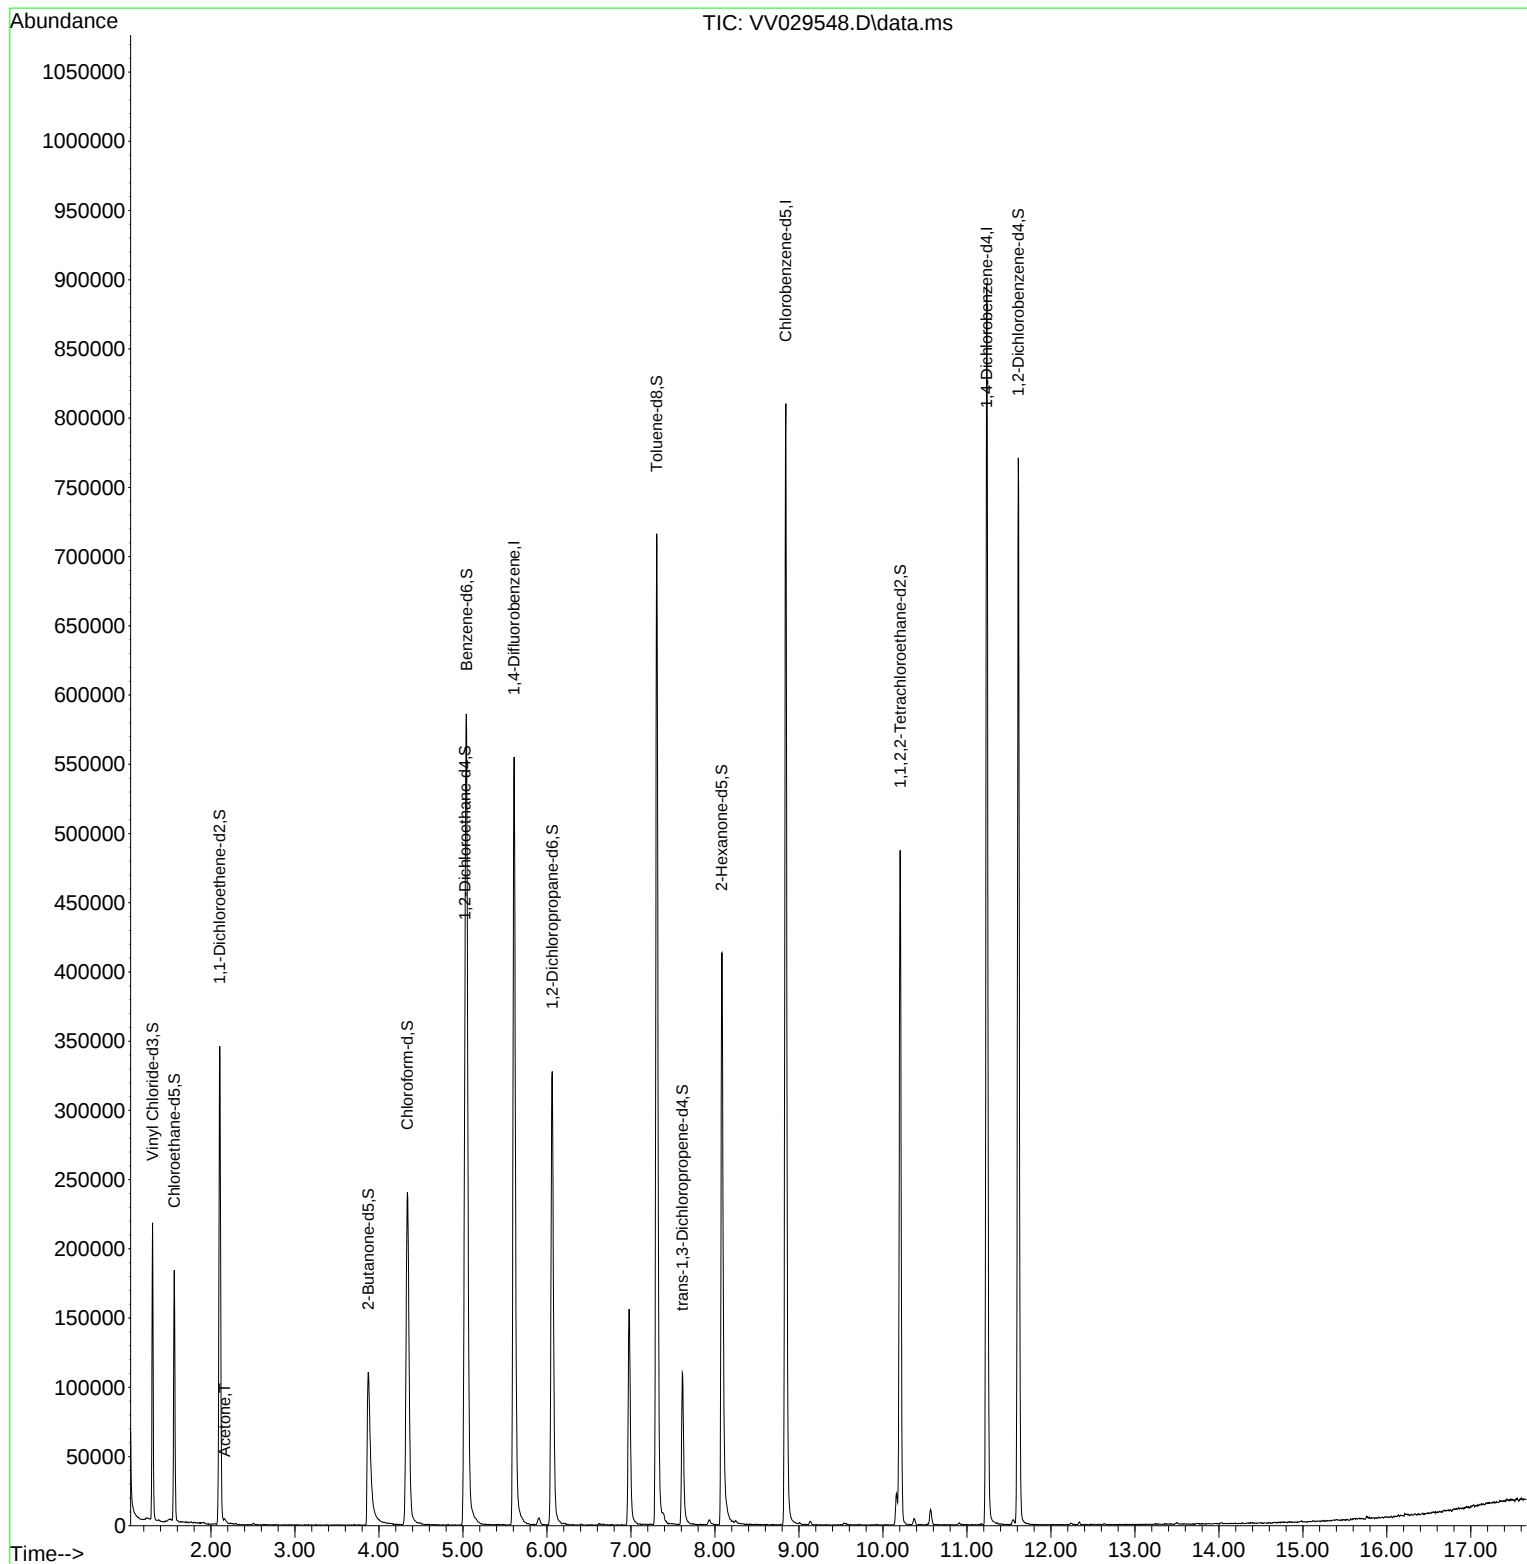

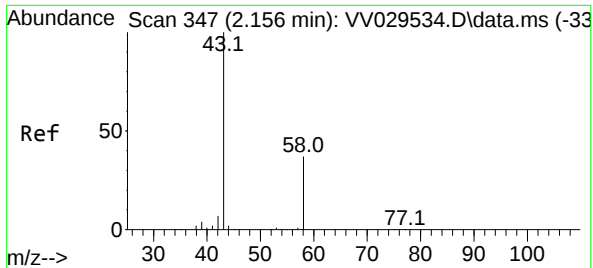

#13
 Acetone
 Concen: 2.270 ug/L
 RT: 2.163 min Scan# 34
 Delta R.T. 0.007 min
 Lab File: VV029548.D
 Acq: 10 Dec 2022 01:56

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N15

Tgt Ion:	43	Resp:	2844
Ion Ratio	Lower	Upper	
43	100		
58	34.3	0.0	74.8

