




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029540.D
 Acq On : 09 Dec 2022 22:49
 Operator : SY/MD
 Sample : N5959-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EM1

Manual IntegrationsAPPROVED

Quant Time: Dec 10 01:10:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 10 00:41:04 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/12/2022
 Supervised By :Mahesh Dadoda 12/12/2022

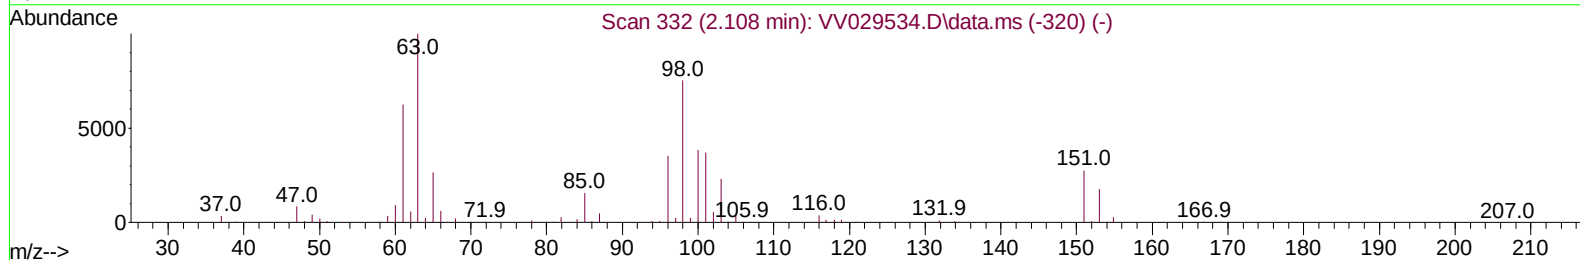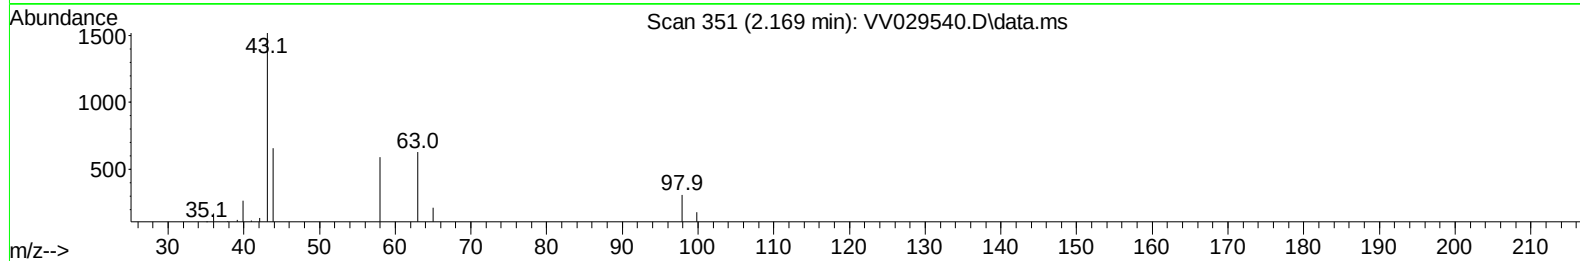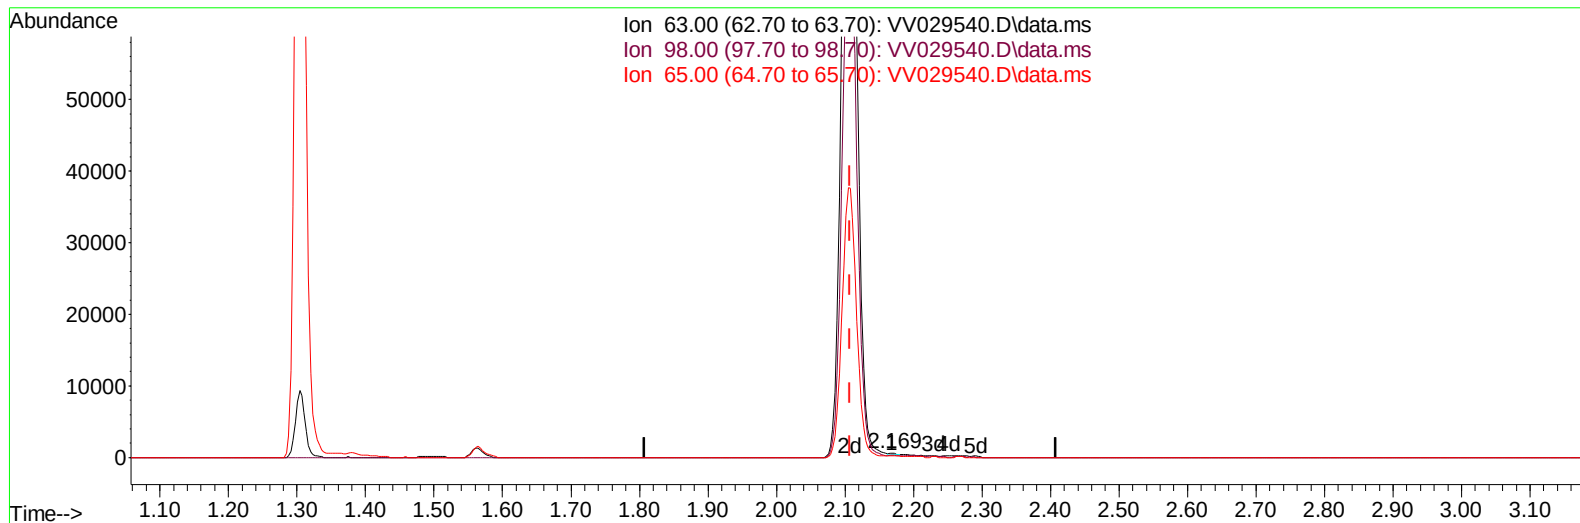

TIC: VV029540.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.169min (+ 0.061) 0.03 ug/L

response 134

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	84.90	60.45
65.00	23.50	17.91
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029540.D
Acq On : 09 Dec 2022 22:49
Operator : SY/MD
Sample : N5959-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EM1

Manual IntegrationsAPPROVED

Quant Time: Dec 10 01:10:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 10 00:41:04 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 12/12/2022
Supervised By :Mahesh Dadoda 12/12/2022

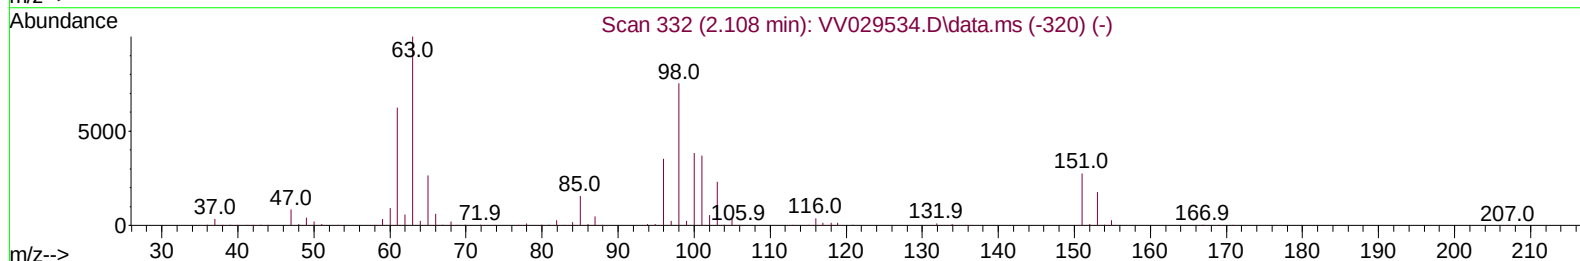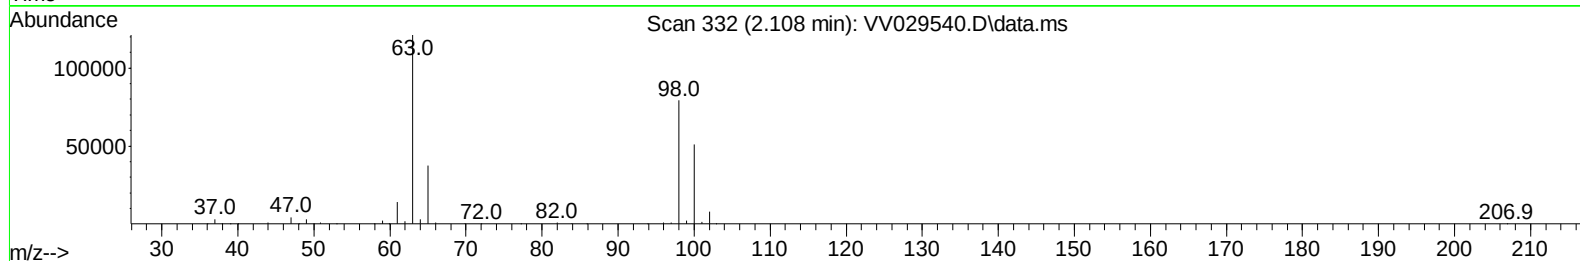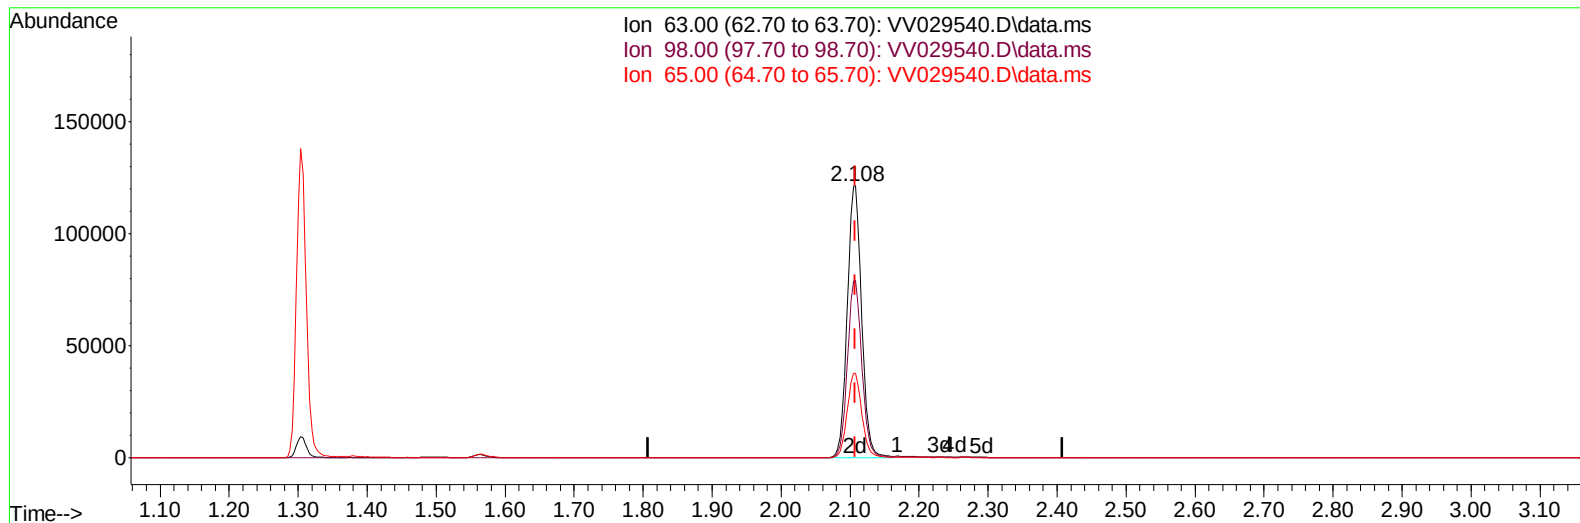

TIC: VV029540.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.108min (+ 0.000) 39.40 ug/L m

response 176169

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	84.90	0.05#
65.00	23.50	0.01#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029540.D
 Acq On : 09 Dec 2022 22:49
 Operator : SY/MD
 Sample : N5959-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EM1

Manual IntegrationsAPPROVED

Quant Time: Dec 10 01:10:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 10 00:41:04 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 12/12/2022
 Supervised By :Mahesh Dadoda 12/12/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	468092	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	430620	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	227553	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	135513	47.276	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	94.560%	
7) Chloroethane-d5	1.564	69	114705	52.479	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	104.960%	
11) 1,1-Dichloroethene-d2	2.108	63	176169m	39.404	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	78.800%	
21) 2-Butanone-d5	3.876	46	175306	100.256	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	100.260%	
24) Chloroform-d	4.342	84	254616	47.203	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	94.400%	
26) 1,2-Dichloroethane-d4	5.027	65	152550	49.518	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	99.040%	
32) Benzene-d6	5.047	84	556562	48.914	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	97.820%	
36) 1,2-Dichloropropane-d6	6.066	67	171038	49.211	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	98.420%	
41) Toluene-d8	7.310	98	503577	46.971	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	93.940%	
43) trans-1,3-Dichloroprop...	7.616	79	69001	39.316	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	78.640%	
47) 2-Hexanone-d5	8.085	63	148509	100.063	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	100.060%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	236930	47.705	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	95.400%	
66) 1,2-Dichlorobenzene-d4	11.615	152	204876	47.297	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	94.600%	
Target Compounds						
13) Acetone	2.166	43	2961	2.599	ug/L	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029540.D
Acq On : 09 Dec 2022 22:49
Operator : SY/MD
Sample : N5959-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
C0EM1

Manual IntegrationsAPPROVED

Quant Time: Dec 10 01:10:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 10 00:41:04 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 12/12/2022
Supervised By :Mahesh Dadoda 12/12/2022

