

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029517.D
 Acq On : 09 Dec 2022 13:36
 Operator : SY/MD
 Sample : N5920-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN1

Quant Time: Dec 09 23:50:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 09 23:48:53 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.609	114	467407	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.844	117	423349	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.236	152	223163	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.301	65	143804	50.242	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	100.480%	
7) Chloroethane-d5		1.561	69	112394	51.497	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.000%	
11) 1,1-Dichloroethene-d2		2.101	63	175677	39.352	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.700%	
21) 2-Butanone-d5		3.870	46	174676	100.042	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.040%	
24) Chloroform-d		4.339	84	250295	46.470	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.940%	
26) 1,2-Dichloroethane-d4		5.021	65	147631	47.991	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.980%	
32) Benzene-d6		5.040	84	553995	49.524	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.040%	
36) 1,2-Dichloropropane-d6		6.063	67	166882	48.840	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.680%	
41) Toluene-d8		7.307	98	493438	46.816	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.640%	
43) trans-1,3-Dichloroprop...		7.612	79	68538	39.723	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.440%	
47) 2-Hexanone-d5		8.082	63	152398	104.447	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	104.450%	
56) 1,1,2,2-Tetrachloroeth...		10.204	84	230416	47.190	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.380%	
66) 1,2-Dichlorobenzene-d4		11.612	152	197192	46.418	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.840%	
Target Compounds							
13) Acetone		2.162	43	2854	2.509	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029517.D
Acq On : 09 Dec 2022 13:36
Operator : SY/MD
Sample : N5920-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN1

Quant Time: Dec 09 23:50:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 09 23:48:53 2022
Response via : Initial Calibration

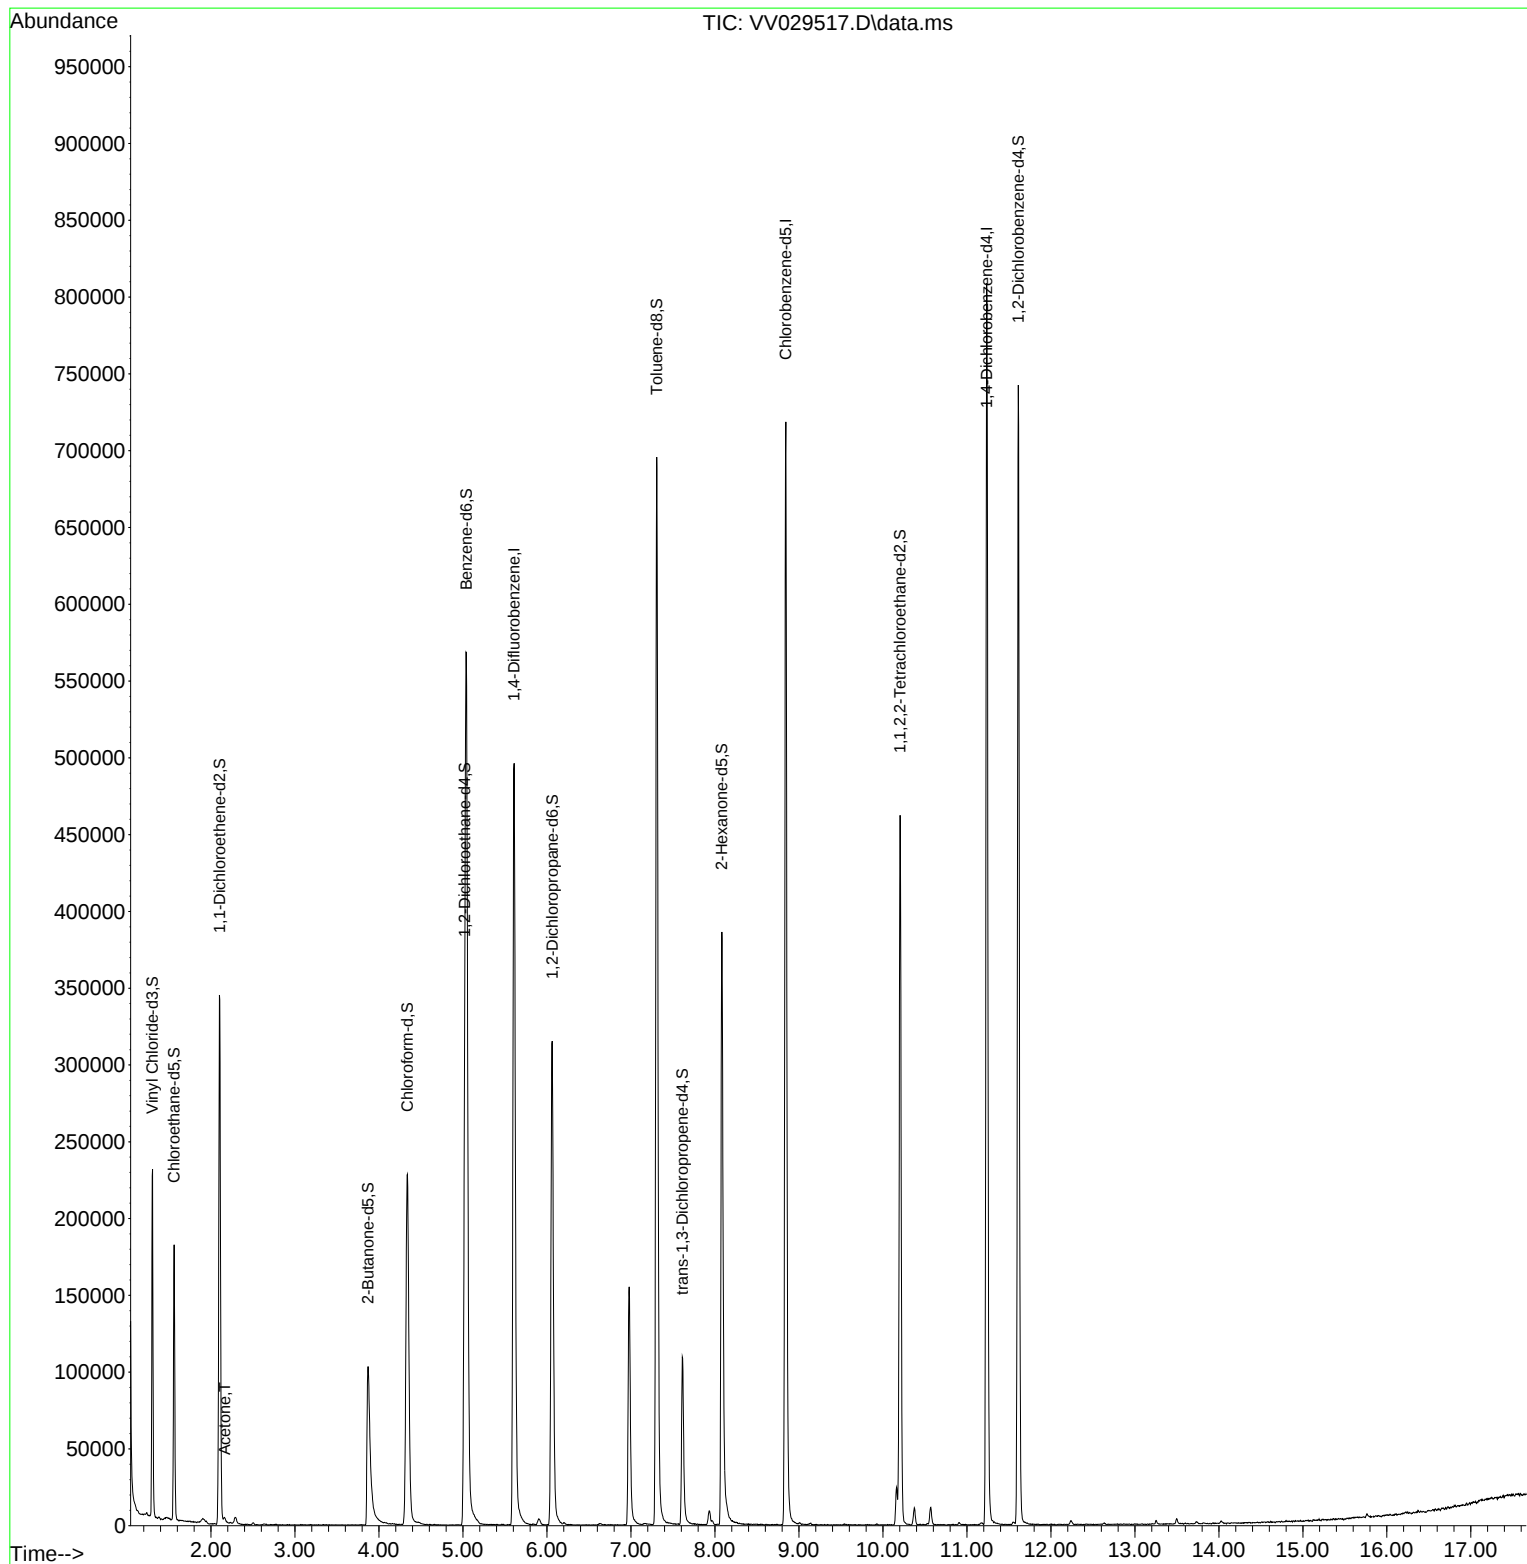

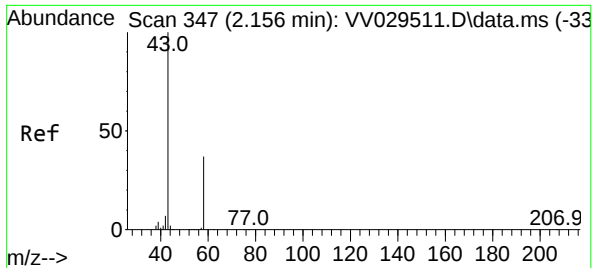

#13
 Acetone
 Concen: 2.509 ug/L
 RT: 2.162 min Scan# 34
 Delta R.T. 0.006 min
 Lab File: VV029517.D
 Acq: 09 Dec 2022 13:36

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN1

Tgt Ion: 43 Resp: 2854
 Ion Ratio Lower Upper
 43 100
 58 43.8 0.0 74.8

