

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029518.D
 Acq On : 09 Dec 2022 14:00
 Operator : SY/MD
 Sample : N5920-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN3

Quant Time: Dec 09 23:51:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 09 23:48:53 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	414675	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	383569	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	197983	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	156315	61.558	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	123.120%	
7) Chloroethane-d5	1.564	69	129800	67.035	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	134.080%#	
11) 1,1-Dichloroethene-d2	2.105	63	200487	50.620	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	101.240%	
21) 2-Butanone-d5	3.870	46	204060	131.733	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	131.730%#	
24) Chloroform-d	4.339	84	290506	60.795	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	121.580%	
26) 1,2-Dichloroethane-d4	5.024	65	174744	64.029	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	128.060%#	
32) Benzene-d6	5.043	84	642425	63.386	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	126.780%#	
36) 1,2-Dichloropropane-d6	6.063	67	191171	61.751	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	123.500%#	
41) Toluene-d8	7.307	98	574022	60.109	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	120.220%#	
43) trans-1,3-Dichloroprop...	7.612	79	79952	51.144	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	102.280%	
47) 2-Hexanone-d5	8.082	63	175299	132.602	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	132.600%#	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	269662	60.955	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	121.920%#	
66) 1,2-Dichlorobenzene-d4	11.612	152	232169	61.602	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	123.200%#	
Target Compounds						
13) Acetone	2.159	43	3315	3.285	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029518.D
Acq On : 09 Dec 2022 14:00
Operator : SY/MD
Sample : N5920-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN3

Quant Time: Dec 09 23:51:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 09 23:48:53 2022
Response via : Initial Calibration

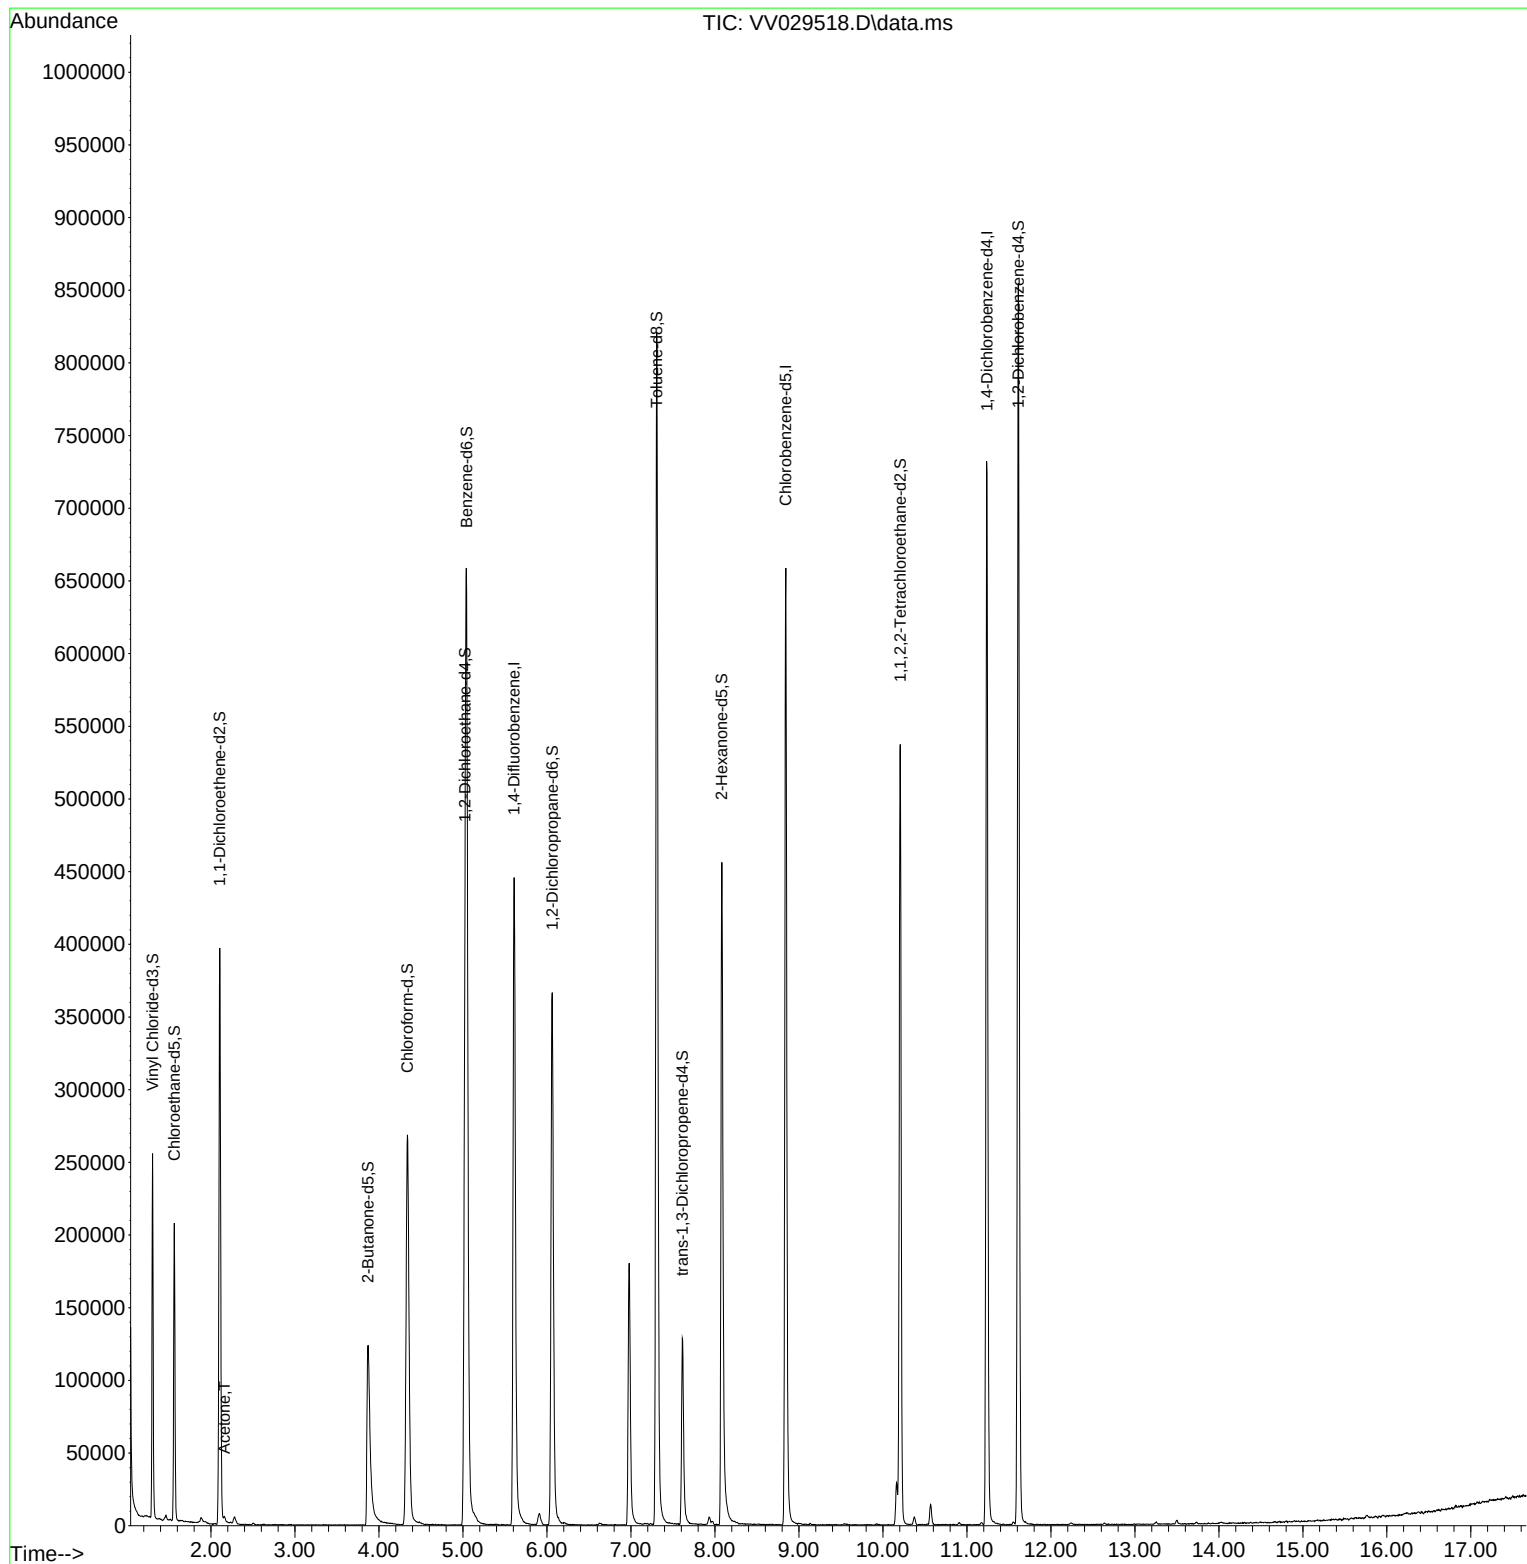

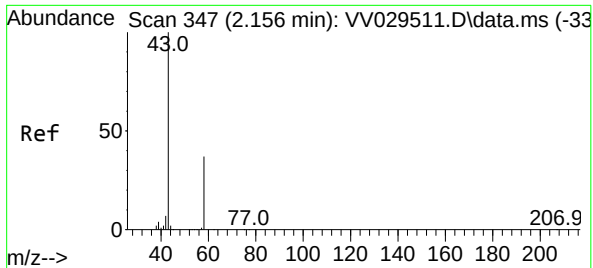

#13
 Acetone
 Concen: 3.285 ug/L
 RT: 2.159 min Scan# 34
 Delta R.T. 0.003 min
 Lab File: VV029518.D
 Acq: 09 Dec 2022 14:00

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN3

Tgt Ion:	43	Resp:	3315
Ion	Ratio	Lower	Upper
43	100		
58	39.0	0.0	74.8

