

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029521.D
 Acq On : 09 Dec 2022 15:10
 Operator : SY/MD
 Sample : N5920-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN7

Quant Time: Dec 09 23:51:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 09 23:48:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	404181	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	369559	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.236	152	191626	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	130768	52.835	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	105.660%	
7) Chloroethane-d5	1.564	69	107512	56.966	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	113.940%	
11) 1,1-Dichloroethene-d2	2.105	63	166077	43.021	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	86.040%	
21) 2-Butanone-d5	3.870	46	163600	108.356	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	108.360%	
24) Chloroform-d	4.339	84	239628	51.449	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.900%	
26) 1,2-Dichloroethane-d4	5.024	65	145967	54.873	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	109.740%	
32) Benzene-d6	5.043	84	525970	53.863	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	107.720%	
36) 1,2-Dichloropropane-d6	6.063	67	157789	52.900	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	105.800%	
41) Toluene-d8	7.307	98	477569	51.905	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	103.820%	
43) trans-1,3-Dichloroprop...	7.616	79	63953	42.460	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	84.920%	
47) 2-Hexanone-d5	8.082	63	142083	111.551	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	111.550%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	223796	52.505	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	105.020%	
66) 1,2-Dichlorobenzene-d4	11.612	152	189789	52.028	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	104.060%	
Target Compounds					Qvalue	
13) Acetone	2.159	43	2943	2.992	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029521.D
Acq On : 09 Dec 2022 15:10
Operator : SY/MD
Sample : N5920-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN7

Quant Time: Dec 09 23:51:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 09 23:48:53 2022
Response via : Initial Calibration

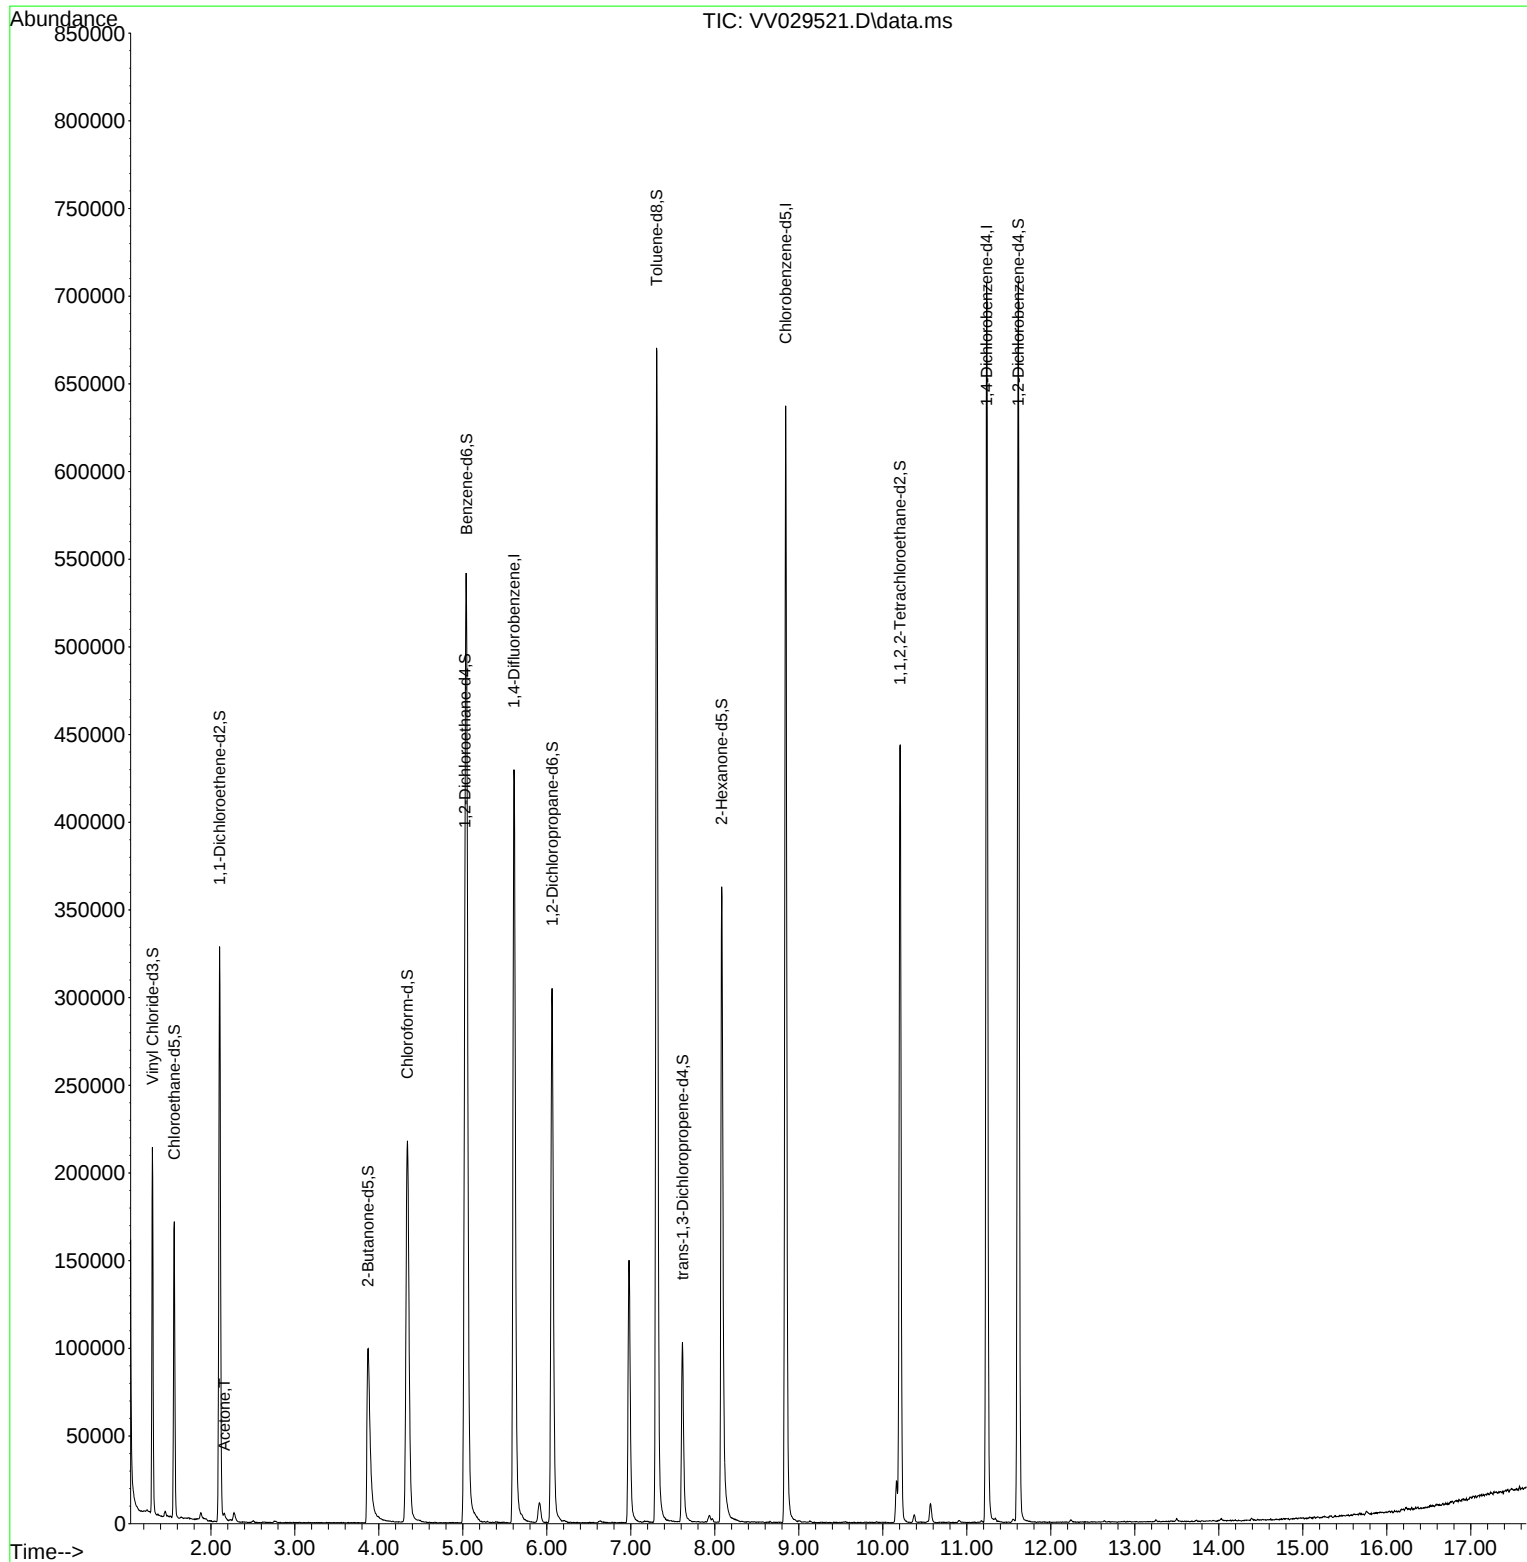

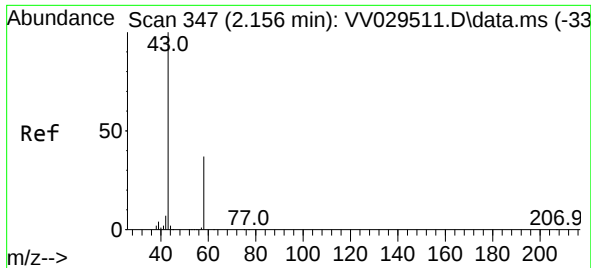

#13
 Acetone
 Concen: 2.992 ug/L
 RT: 2.159 min Scan# 34
 Delta R.T. 0.003 min
 Lab File: VV029521.D
 Acq: 09 Dec 2022 15:10

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN7

Tgt Ion: 43 Resp: 2943
 Ion Ratio Lower Upper
 43 100
 58 36.4 0.0 74.8

