

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029522.D
 Acq On : 09 Dec 2022 15:34
 Operator : SY/MD
 Sample : N5920-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN9

Quant Time: Dec 09 23:51:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 09 23:48:53 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.609	114	435746	50.000	ug/L	0.00
28) Chlorobenzene-d5		8.844	117	403031	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.239	152	209045	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.304	65	135108	50.634	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	101.260%	
7) Chloroethane-d5		1.565	69	105490	51.846	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.700%	
11) 1,1-Dichloroethene-d2		2.105	63	164132	39.437	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.880%	
21) 2-Butanone-d5		3.870	46	169283	103.998	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.000%	
24) Chloroform-d		4.339	84	235146	46.830	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.660%	
26) 1,2-Dichloroethane-d4		5.024	65	143801	50.143	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.280%	
32) Benzene-d6		5.043	84	511163	47.999	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.000%	
36) 1,2-Dichloropropane-d6		6.063	67	155198	47.710	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.420%	
41) Toluene-d8		7.307	98	462527	46.095	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.200%	
43) trans-1,3-Dichloroprop...		7.612	79	64886	39.502	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.000%	
47) 2-Hexanone-d5		8.082	63	142700	102.731	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	102.730%	
56) 1,1,2,2-Tetrachloroeth...		10.204	84	216070	46.483	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	92.960%	
66) 1,2-Dichlorobenzene-d4		11.612	152	187292	47.065	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.140%	
Target Compounds							
13) Acetone		2.159	43	2839	2.677	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029522.D
Acq On : 09 Dec 2022 15:34
Operator : SY/MD
Sample : N5920-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN9


Quant Time: Dec 09 23:51:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 09 23:48:53 2022
Response via : Initial Calibration

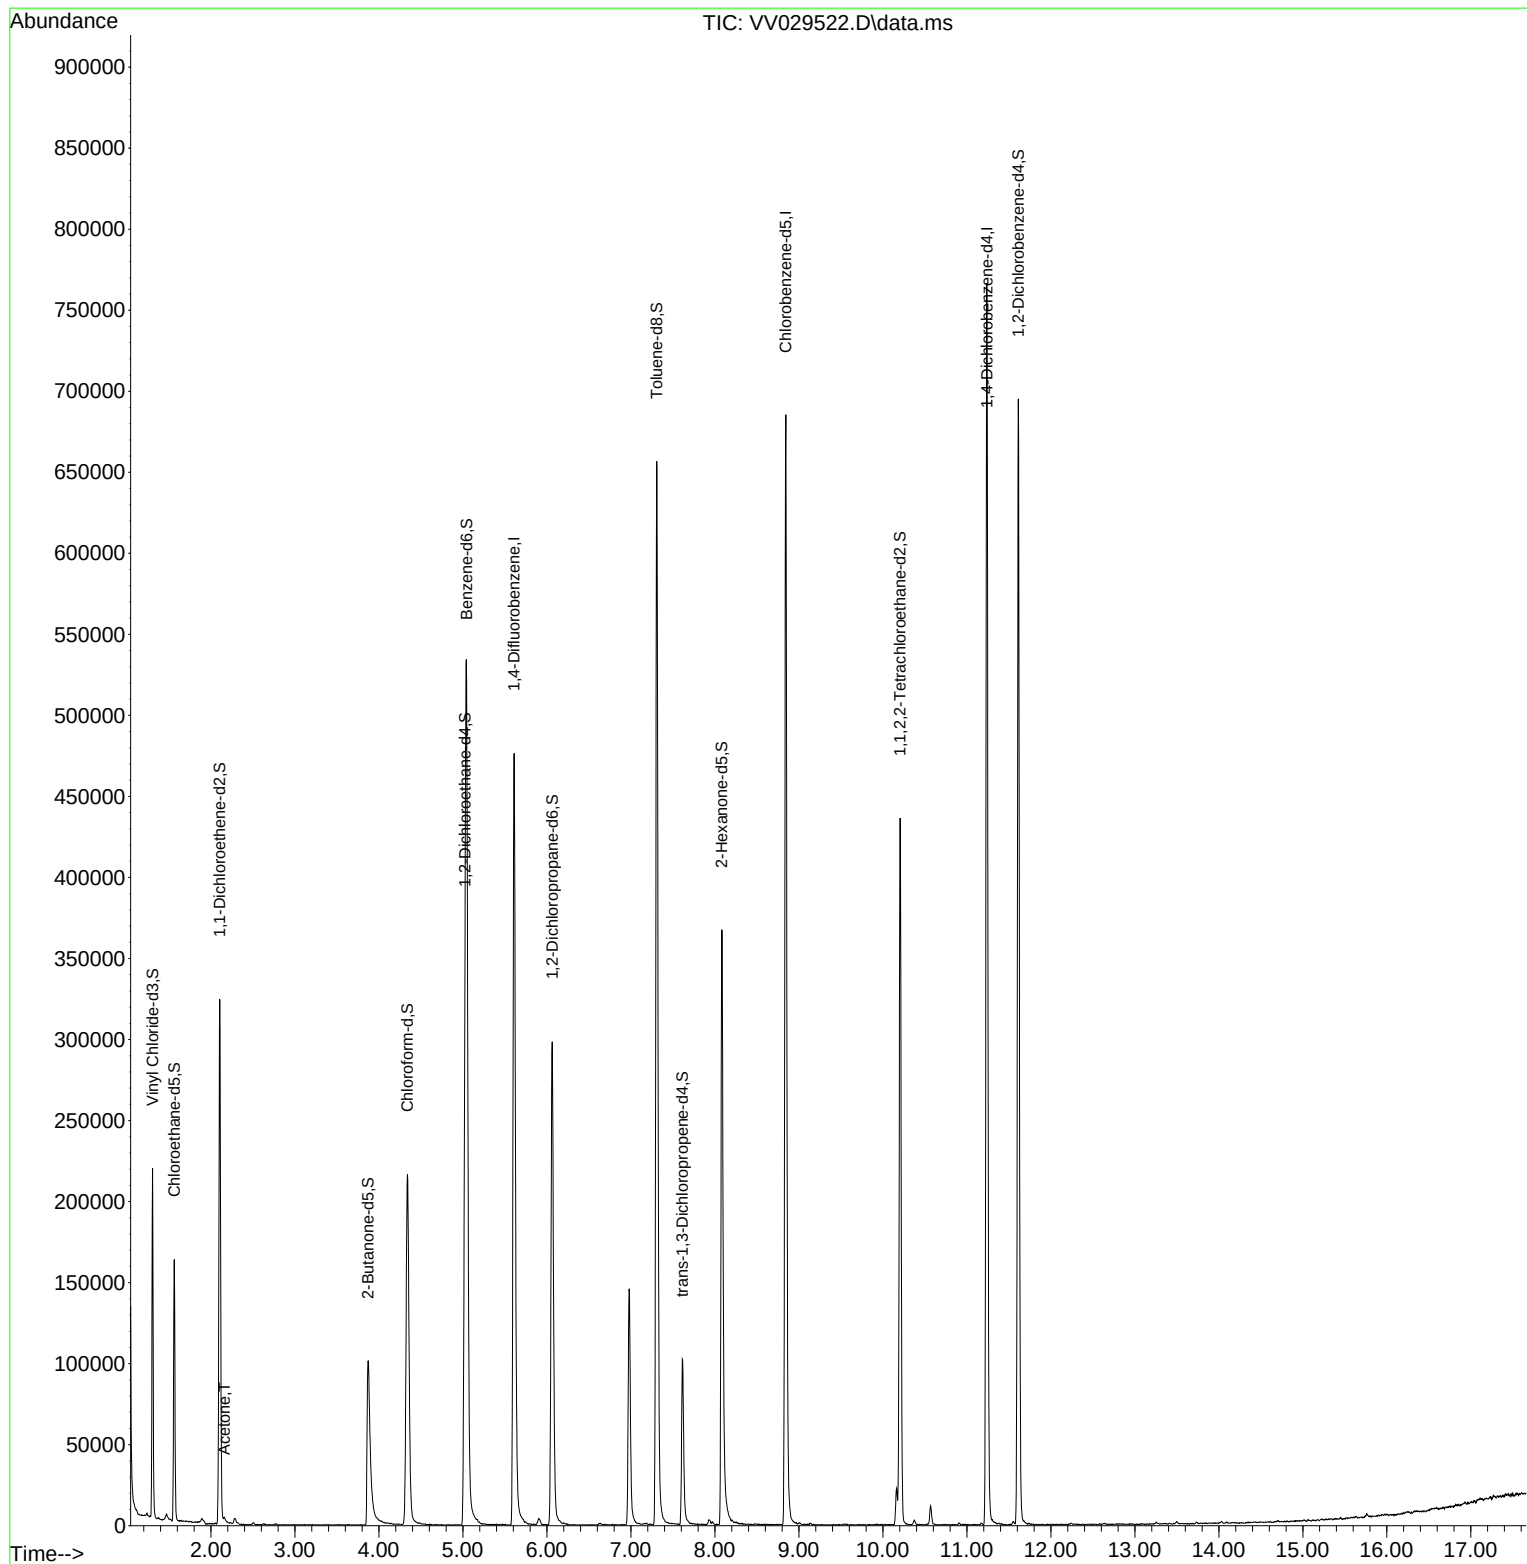

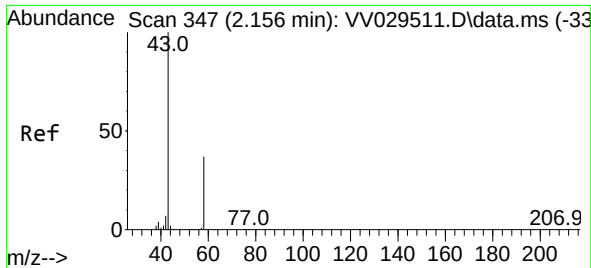

#13
 Acetone
 Concen: 2.677 ug/L
 RT: 2.159 min Scan# 34
 Delta R.T. 0.003 min
 Lab File: VV029522.D
 Acq: 09 Dec 2022 15:34

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN9

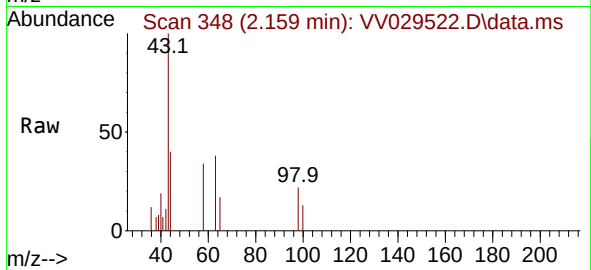

Tgt Ion: 43 Resp: 2839
 Ion Ratio Lower Upper
 43 100
 58 31.9 0.0 74.8

