

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029524.D
 Acq On : 09 Dec 2022 16:20
 Operator : SY/MD
 Sample : N5959-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ9

Quant Time: Dec 09 23:52:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Dec 09 23:48:53 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	411310	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	379595	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	197206	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	141165	56.047	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	112.100%	
7) Chloroethane-d5	1.565	69	109996	57.272	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	114.540%	
11) 1,1-Dichloroethene-d2	2.105	63	170390	43.373	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	86.740%	
21) 2-Butanone-d5	3.870	46	175262	114.068	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	114.070%	
24) Chloroform-d	4.339	84	247160	52.147	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	104.300%	
26) 1,2-Dichloroethane-d4	5.024	65	147398	54.451	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	108.900%	
32) Benzene-d6	5.044	84	534936	53.333	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	106.660%	
36) 1,2-Dichloropropane-d6	6.063	67	162590	53.069	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	106.140%	
41) Toluene-d8	7.307	98	482897	51.097	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	102.200%	
43) trans-1,3-Dichloroprop...	7.613	79	66334	42.877	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	85.760%	
47) 2-Hexanone-d5	8.082	63	144653	110.566	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	110.570%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	227058	51.862	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	103.720%	
66) 1,2-Dichlorobenzene-d4	11.612	152	195115	51.975	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	103.940%	
Target Compounds						
13) Acetone	2.156	43	4142	4.138	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029524.D
Acq On : 09 Dec 2022 16:20
Operator : SY/MD
Sample : N5959-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ9

Quant Time: Dec 09 23:52:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Dec 09 23:48:53 2022
Response via : Initial Calibration

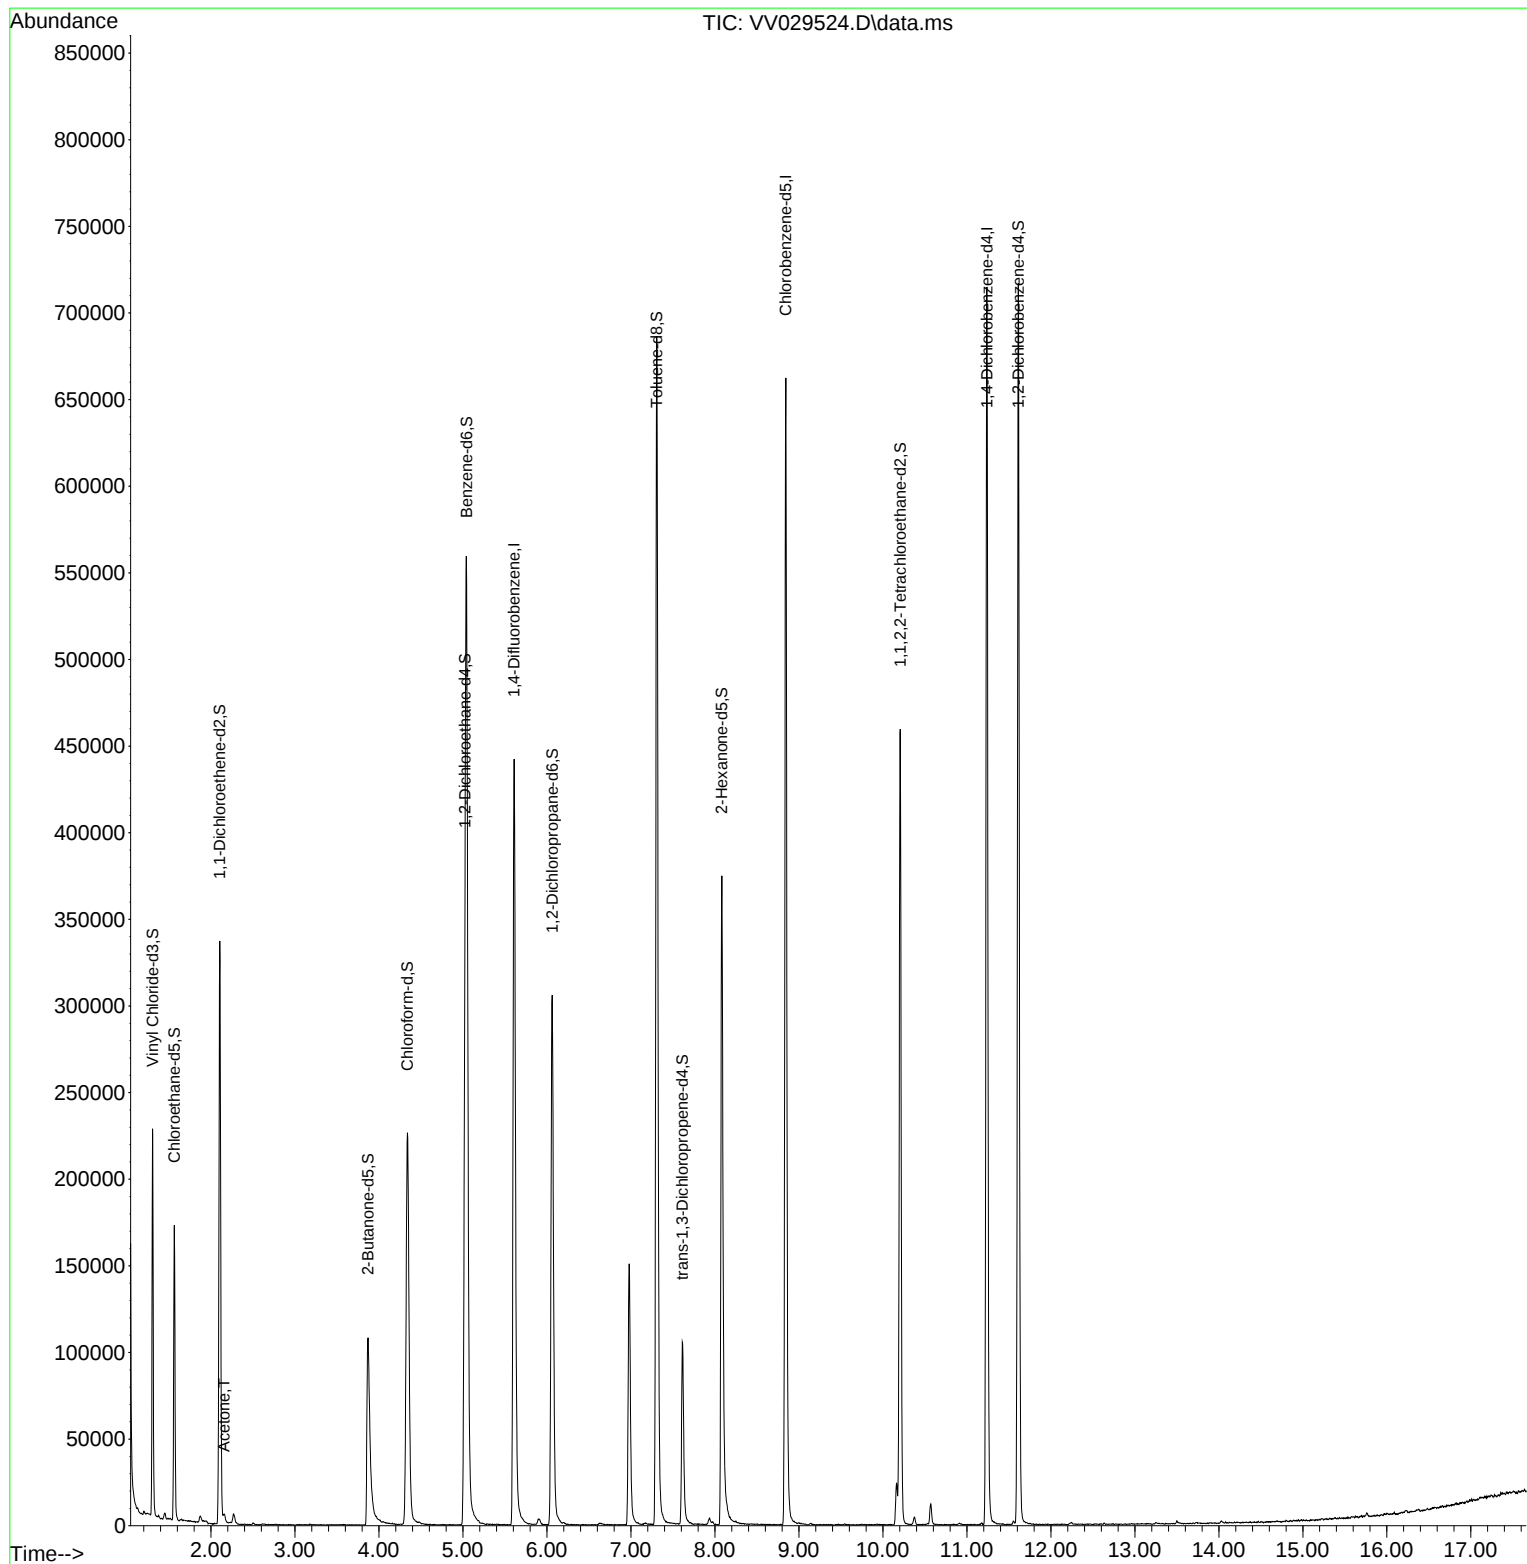

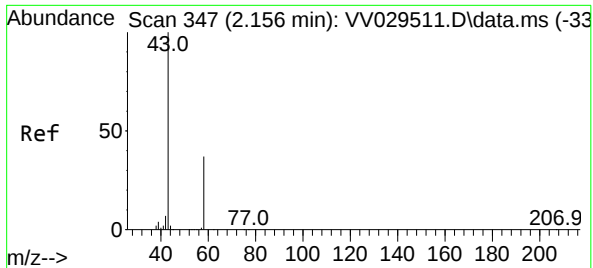

#13
Acetone
Concen: 4.138 ug/L
RT: 2.156 min Scan# 34
Delta R.T. 0.000 min
Lab File: VV029524.D
Acq: 09 Dec 2022 16:20

Instrument :
MSVOA_V
ClientSampleId :
C0EJ9

Tgt Ion: 43 Resp: 4142
Ion Ratio Lower Upper
43 100
58 32.2 0.0 74.8

