

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029542.D
 Acq On : 09 Dec 2022 23:35
 Operator : SY/MD
 Sample : N5959-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EM9

Quant Time: Dec 10 01:11:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 10 00:41:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	455580	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	419134	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	221771	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	136732	49.012	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	98.020%	
7) Chloroethane-d5	1.565	69	112154	52.722	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	105.440%	
11) 1,1-Dichloroethene-d2	2.105	63	171900	39.505	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	79.020%	
21) 2-Butanone-d5	3.873	46	178088	104.644	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	104.640%	
24) Chloroform-d	4.339	84	245624	46.787	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.580%	
26) 1,2-Dichloroethane-d4	5.024	65	146507	48.862	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.720%	
32) Benzene-d6	5.044	84	534719	48.282	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.560%	
36) 1,2-Dichloropropane-d6	6.063	67	162999	48.183	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	96.360%	
41) Toluene-d8	7.307	98	481922	46.183	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.360%	
43) trans-1,3-Dichloroprop...	7.616	79	64666	37.856	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	75.720%	
47) 2-Hexanone-d5	8.082	63	150650	104.287	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	104.290%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	227784	47.120	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	94.240%	
66) 1,2-Dichlorobenzene-d4	11.612	152	194451	46.060	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	92.120%	
Target Compounds						
13) Acetone	2.166	43	5264	4.748	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029542.D
Acq On : 09 Dec 2022 23:35
Operator : SY/MD
Sample : N5959-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EM9

Quant Time: Dec 10 01:11:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 10 00:41:04 2022
Response via : Initial Calibration

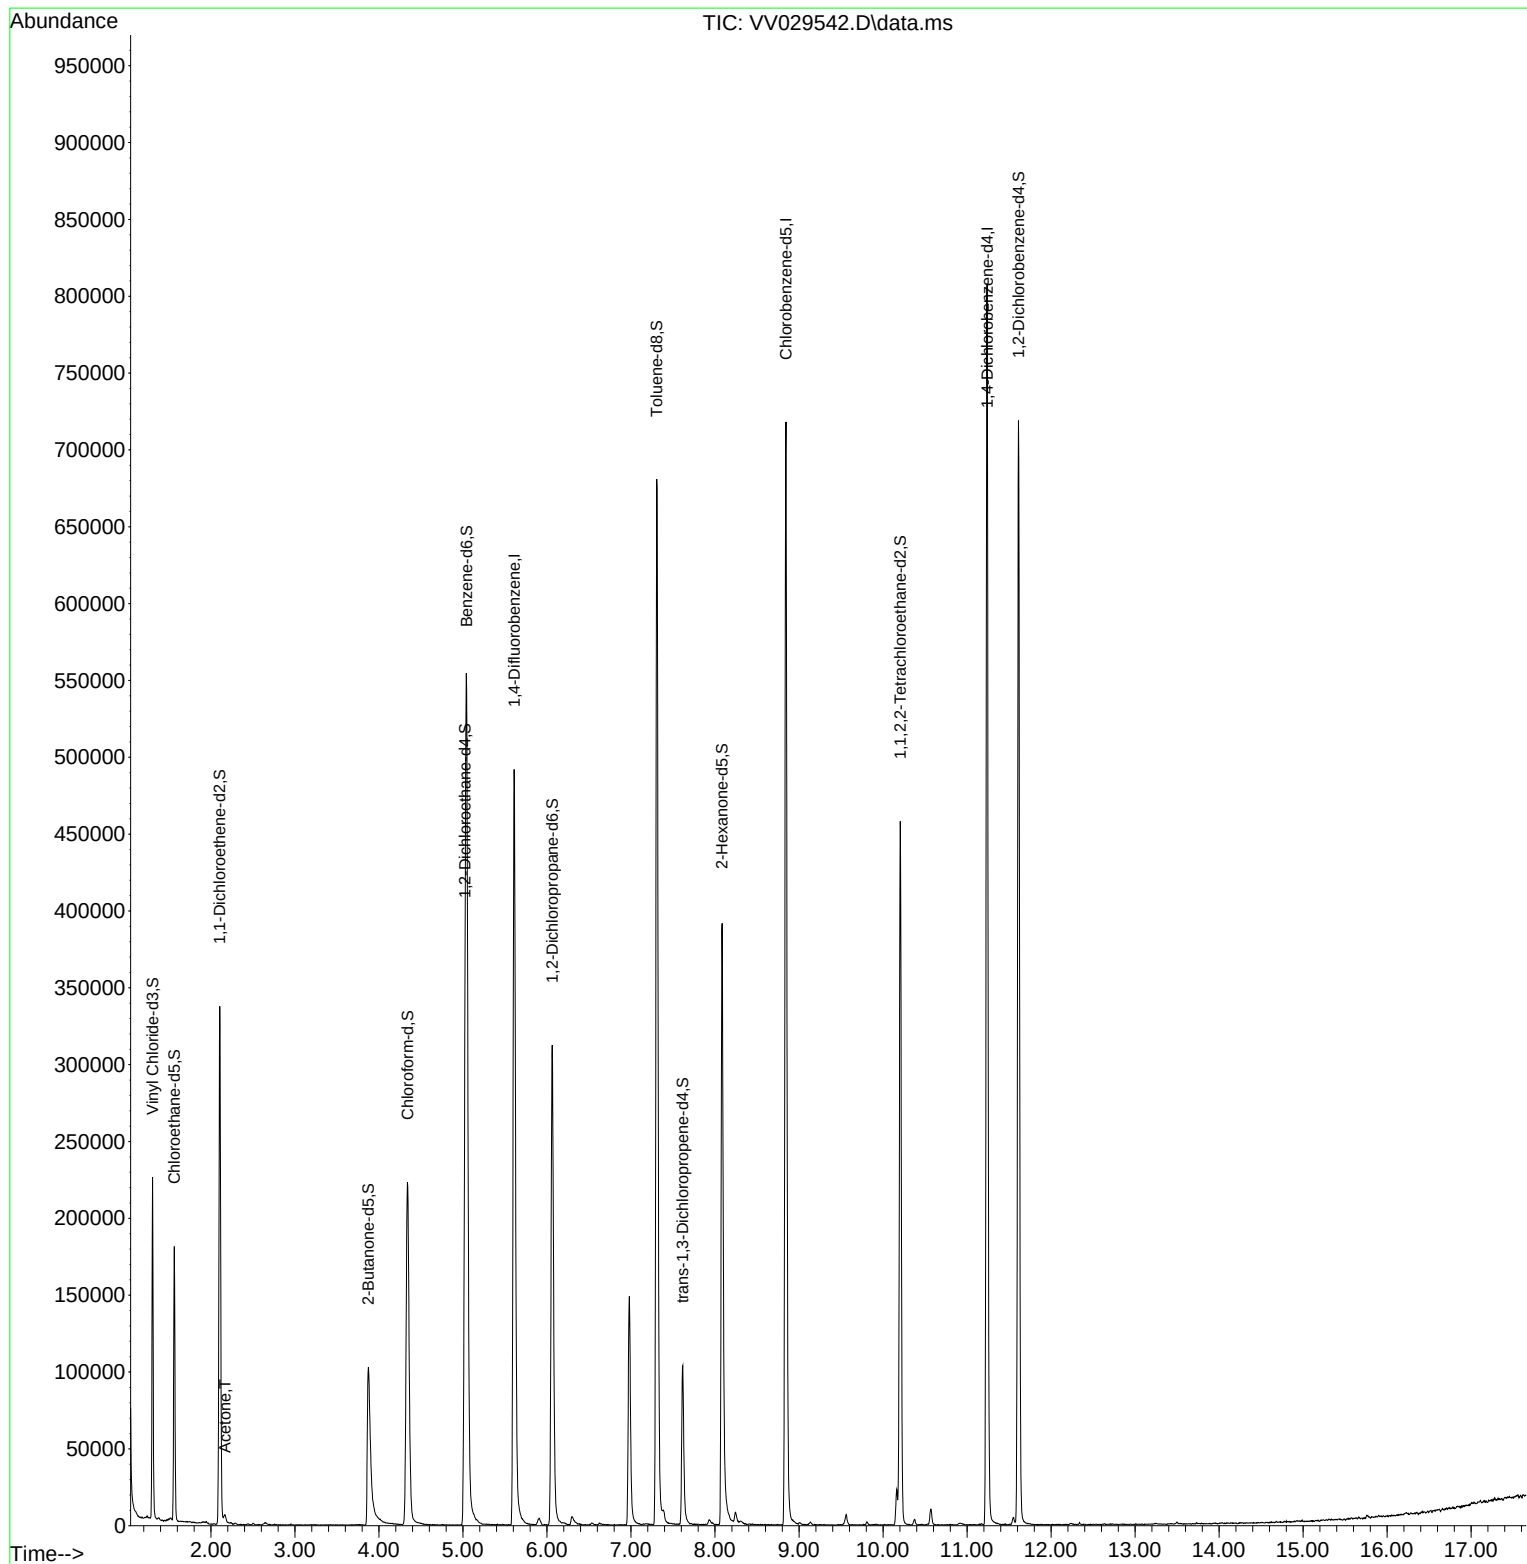

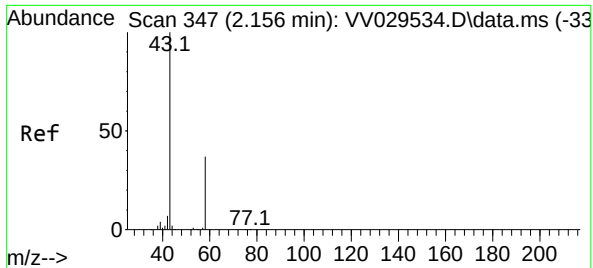

#13
 Acetone
 Concen: 4.748 ug/L
 RT: 2.166 min Scan# 31
 Delta R.T. 0.010 min
 Lab File: VV029542.D
 Acq: 09 Dec 2022 23:35

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EM9

Tgt Ion: 43 Resp: 5264
 Ion Ratio Lower Upper
 43 100
 58 38.6 0.0 74.8

