

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VW120922\  
 Data File : VW029554.D  
 Acq On : 10 Dec 2022 04:17  
 Operator : SY/MD  
 Sample : N5915-15  
 Misc : 5.0mL/MSVOA\_V/WATER  
 ALS Vial : 47 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 F5N13

Quant Time: Dec 10 04:44:29 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM120722WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Sat Dec 10 00:41:04 2022  
 Response via : Initial Calibration


| Compound                      | R.T.    | QIon           | Response | Conc   | Units   | Dev(Min)  |
|-------------------------------|---------|----------------|----------|--------|---------|-----------|
| -----                         |         |                |          |        |         |           |
| Internal Standards            |         |                |          |        |         |           |
| 1) 1,4-Difluorobenzene        | 5.609   | 114            | 477763   | 50.000 | ug/L    | 0.00      |
| 28) Chlorobenzene-d5          | 8.844   | 117            | 448212   | 50.000 | ug/L    | 0.00      |
| 58) 1,4-Dichlorobenzene-d4    | 11.239  | 152            | 231895   | 50.000 | ug/L    | 0.00      |
| System Monitoring Compounds   |         |                |          |        |         |           |
| 4) Vinyl Chloride-d3          | 1.304   | 65             | 130865   | 44.731 | ug/L    | 0.00      |
| Spiked Amount                 | 50.000  | Range 60 - 135 | Recovery | =      | 89.460% |           |
| 7) Chloroethane-d5            | 1.565   | 69             | 108907   | 48.818 | ug/L    | 0.00      |
| Spiked Amount                 | 50.000  | Range 70 - 130 | Recovery | =      | 97.640% |           |
| 11) 1,1-Dichloroethene-d2     | 2.105   | 63             | 166428   | 36.472 | ug/L    | 0.00      |
| Spiked Amount                 | 50.000  | Range 60 - 125 | Recovery | =      | 72.940% |           |
| 21) 2-Butanone-d5             | 3.873   | 46             | 177648   | 99.539 | ug/L    | 0.00      |
| Spiked Amount                 | 100.000 | Range 40 - 130 | Recovery | =      | 99.540% |           |
| 24) Chloroform-d              | 4.339   | 84             | 243480   | 44.225 | ug/L    | 0.00      |
| Spiked Amount                 | 50.000  | Range 70 - 125 | Recovery | =      | 88.460% |           |
| 26) 1,2-Dichloroethane-d4     | 5.024   | 65             | 147580   | 46.935 | ug/L    | 0.00      |
| Spiked Amount                 | 50.000  | Range 70 - 125 | Recovery | =      | 93.860% |           |
| 32) Benzene-d6                | 5.044   | 84             | 526834   | 44.484 | ug/L    | 0.00      |
| Spiked Amount                 | 50.000  | Range 70 - 125 | Recovery | =      | 88.960% |           |
| 36) 1,2-Dichloropropane-d6    | 6.063   | 67             | 161907   | 44.756 | ug/L    | 0.00      |
| Spiked Amount                 | 50.000  | Range 70 - 120 | Recovery | =      | 89.520% |           |
| 41) Toluene-d8                | 7.307   | 98             | 472590   | 42.351 | ug/L    | 0.00      |
| Spiked Amount                 | 50.000  | Range 80 - 120 | Recovery | =      | 84.700% |           |
| 43) trans-1,3-Dichloroprop... | 7.613   | 79             | 63318    | 34.662 | ug/L    | 0.00      |
| Spiked Amount                 | 50.000  | Range 60 - 125 | Recovery | =      | 69.320% |           |
| 47) 2-Hexanone-d5             | 8.082   | 63             | 149927   | 97.053 | ug/L    | 0.00      |
| Spiked Amount                 | 100.000 | Range 45 - 130 | Recovery | =      | 97.050% |           |
| 56) 1,1,2,2-Tetrachloroeth... | 10.204  | 84             | 226271   | 43.770 | ug/L    | 0.00      |
| Spiked Amount                 | 50.000  | Range 65 - 120 | Recovery | =      | 87.540% |           |
| 66) 1,2-Dichlorobenzene-d4    | 11.612  | 152            | 191455   | 43.371 | ug/L    | 0.00      |
| Spiked Amount                 | 50.000  | Range 80 - 120 | Recovery | =      | 86.740% |           |
| Target Compounds              |         |                |          |        |         |           |
| 13) Acetone                   | 2.166   | 43             | 8076     | 6.946  | ug/L    | Qvalue 98 |
| -----                         |         |                |          |        |         |           |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV120922\  
Data File : VV029554.D  
Acq On : 10 Dec 2022 04:17  
Operator : SY/MD  
Sample : N5915-15  
Misc : 5.0mL/MSVOA\_V/WATER  
ALS Vial : 47 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
F5N13

Quant Time: Dec 10 04:44:29 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM120722WMA.M  
Quant Title : VOC Analysis  
QLast Update : Sat Dec 10 00:41:04 2022  
Response via : Initial Calibration

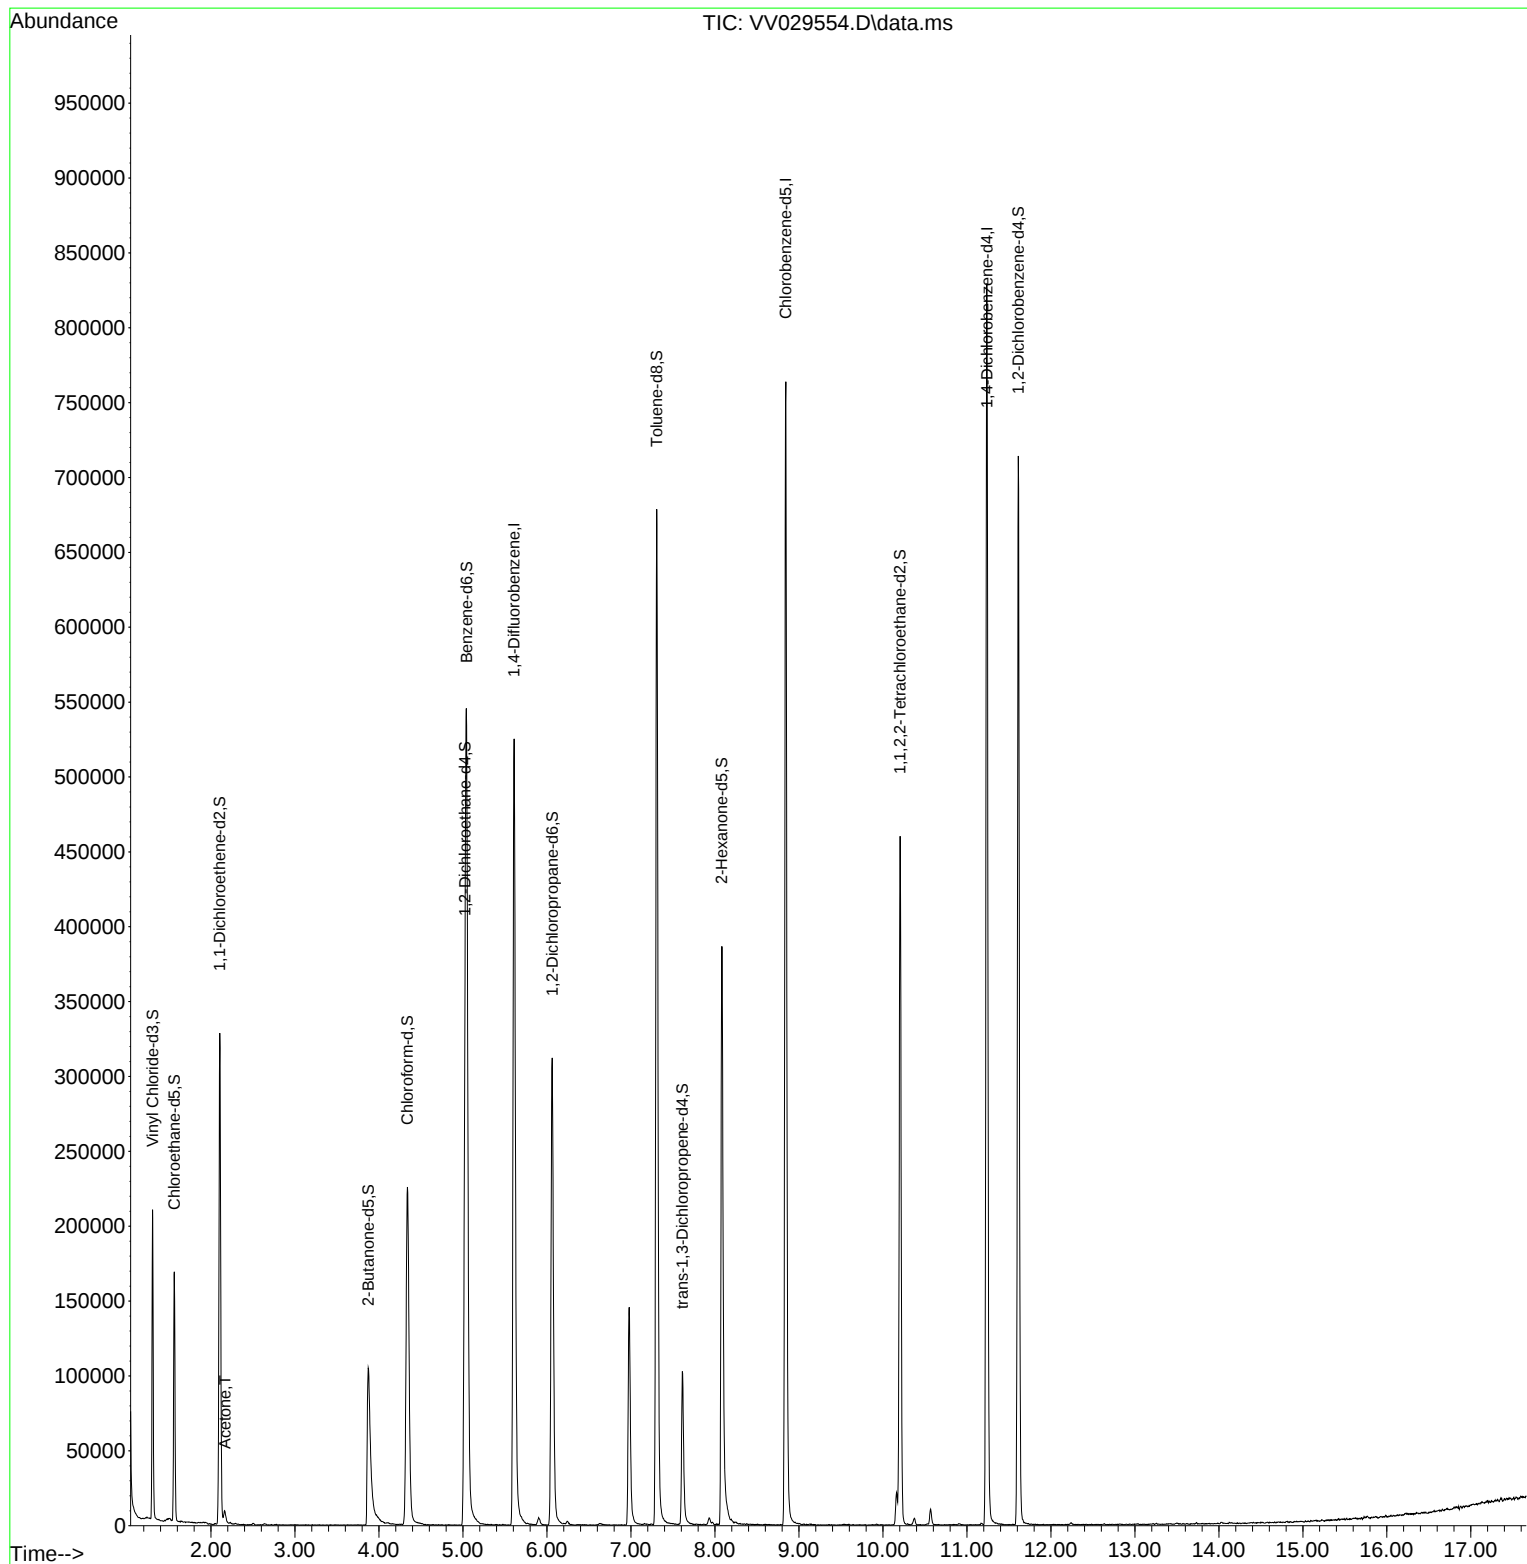

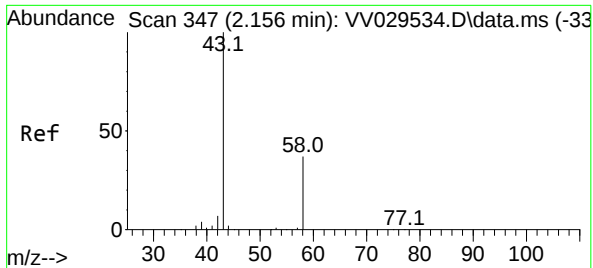

#13  
 Acetone  
 Concen: 6.946 ug/L  
 RT: 2.166 min Scan# 31  
 Delta R.T. 0.010 min  
 Lab File: VV029554.D  
 Acq: 10 Dec 2022 04:17

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 F5N13

Tgt Ion: 43 Resp: 8076  
 Ion Ratio Lower Upper  
 43 100  
 58 36.1 0.0 74.8

