

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029580.D
 Acq On : 10 Dec 2022 14:51
 Operator : SY/MD
 Sample : N5928-15 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ76

Quant Time: Dec 12 00:06:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 10 07:45:47 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	525095	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	484583	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	248136	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	122202	38.004	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.000%
7) Chloroethane-d5	1.564	69	109413	44.624	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.240%
11) 1,1-Dichloroethene-d2	2.105	63	167510	33.400	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.800%
21) 2-Butanone-d5	3.873	46	190645	97.193	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.190%
24) Chloroform-d	4.339	84	248747	41.109	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.220%
26) 1,2-Dichloroethane-d4	5.024	65	151224	43.759	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.520%
32) Benzene-d6	5.043	84	539922	42.167	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	84.340%
36) 1,2-Dichloropropane-d6	6.063	67	168718	43.138	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	86.280%
41) Toluene-d8	7.307	98	479274	39.726	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.460%#
43) trans-1,3-Dichloroprop...	7.616	79	64932	32.877	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.760%
47) 2-Hexanone-d5	8.082	63	157750	94.453	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.450%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	236379	42.294	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.580%
66) 1,2-Dichlorobenzene-d4	11.612	152	187631	39.722	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	79.440%#
Target Compounds						
					Qvalue	
30) 1,1,1-Trichloroethane	4.603	97	9187	1.740	ug/L	# 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029580.D
Acq On : 10 Dec 2022 14:51
Operator : SY/MD
Sample : N5928-15 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 74 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ76

Quant Time: Dec 12 00:06:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 10 07:45:47 2022
Response via : Initial Calibration

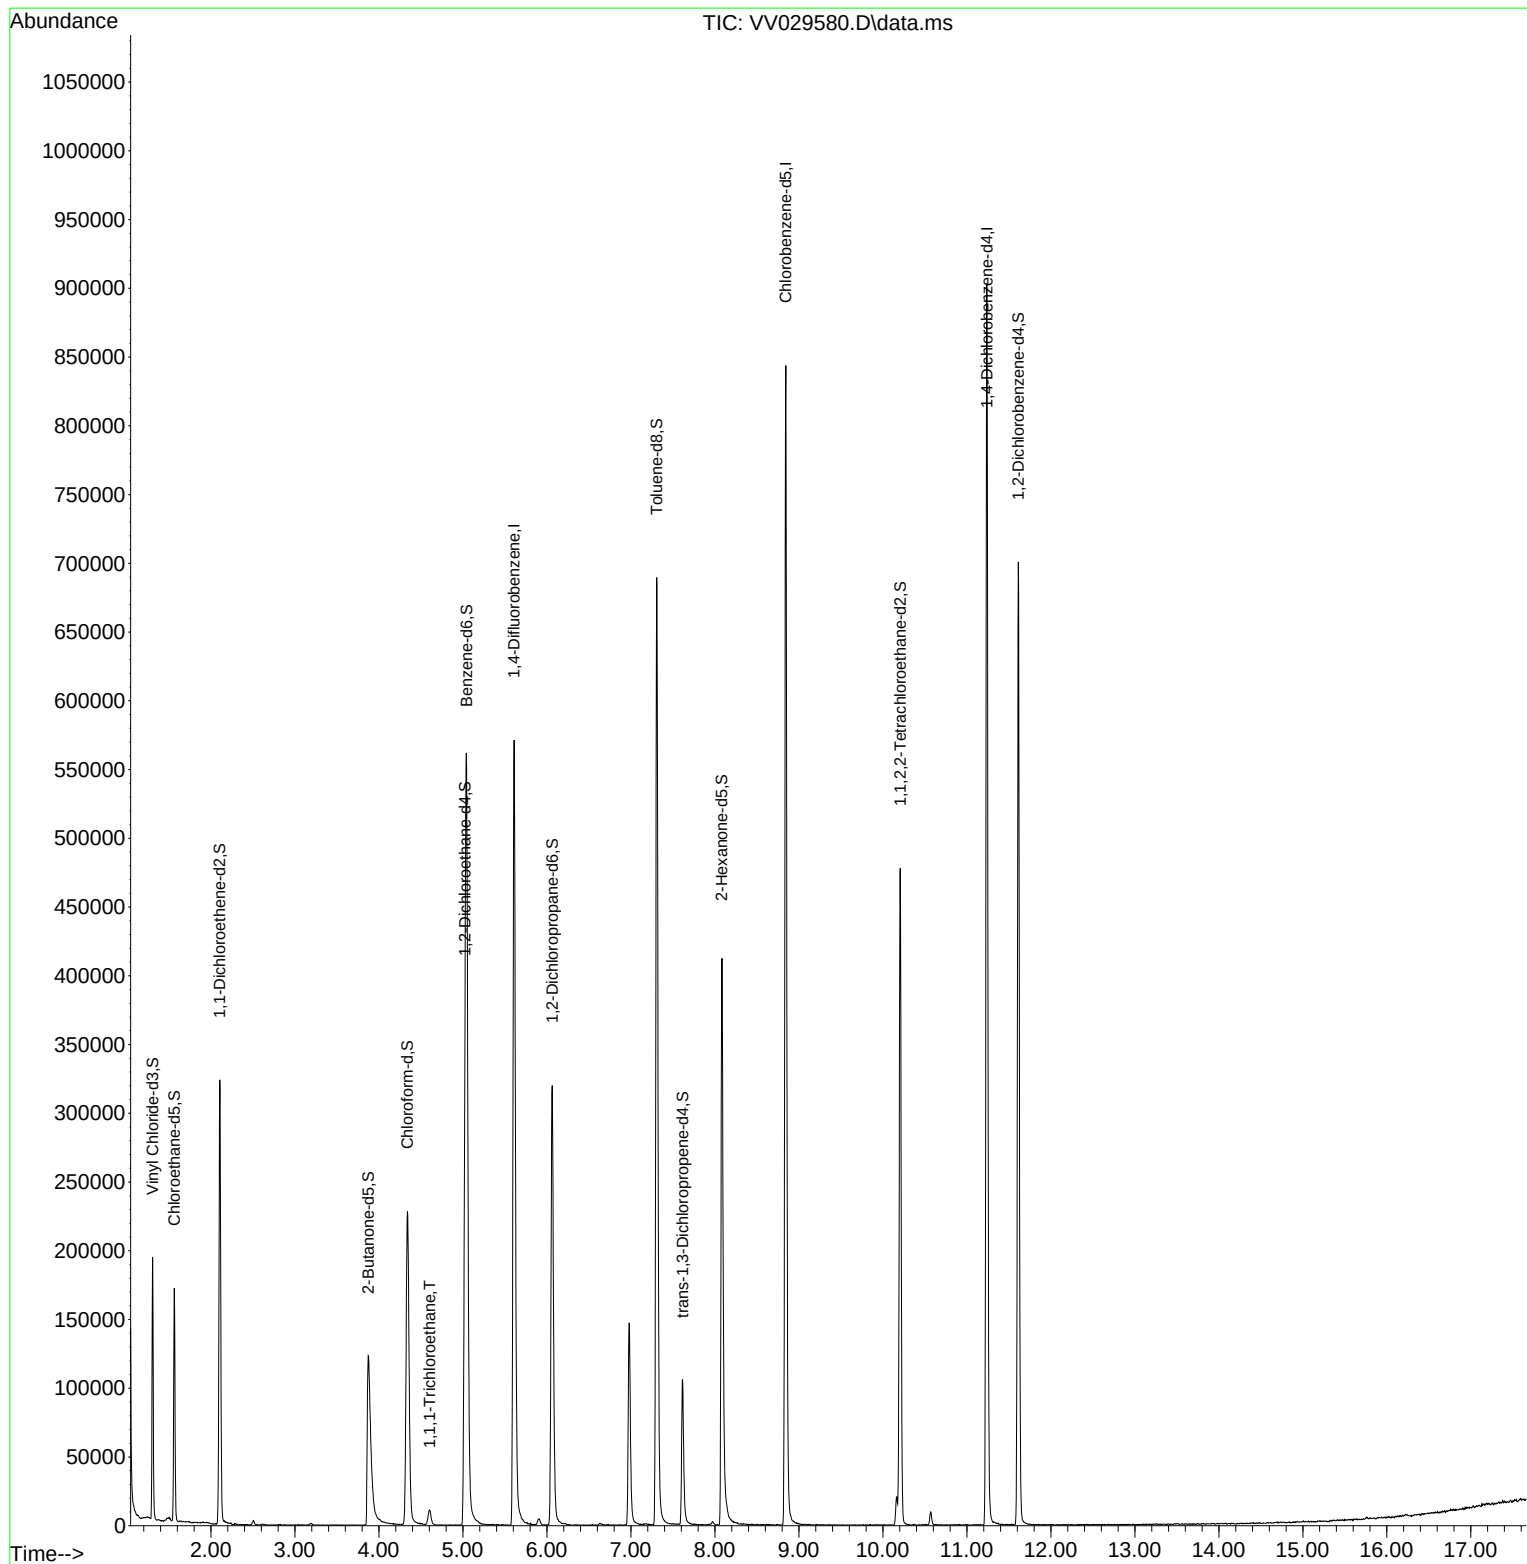

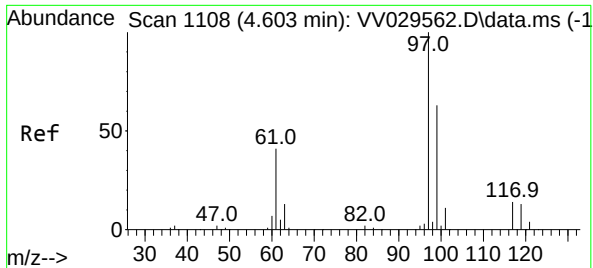

#30
 1,1,1-Trichloroethane
 Concen: 1.740 ug/L
 RT: 4.603 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VV029580.D
 Acq: 10 Dec 2022 14:51

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ76

Tgt Ion:	97	Resp:	9187
Ion	Ratio	Lower	Upper
97	100		
99	33.7	52.1	78.1#
61	44.2	31.8	47.8

