

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029512.D
 Acq On : 09 Dec 2022 11:39
 Operator : SY/MD
 Sample : VV1209WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK303

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	266463	265592	14.76%	1.877%
2	1.564	155	163	180	rVB	211622	240668	13.38%	1.701%
3	2.050	311	314	316	rBV3	497	291	0.02%	0.002%
4	2.105	320	331	349	rBV	414112	594959	33.07%	4.204%
5	2.503	447	455	467	rVB2	4880	7834	0.44%	0.055%
6	2.622	485	492	495	rVB3	410	437	0.02%	0.003%
7	2.764	529	536	545	rVB5	1513	2307	0.13%	0.016%
8	2.815	546	552	556	rBV	309	346	0.02%	0.002%
9	2.899	576	578	583	rVB2	344	267	0.01%	0.002%
10	2.947	589	593	598	rBV3	308	329	0.02%	0.002%
11	3.182	662	666	669	rBV3	510	461	0.03%	0.003%
12	3.201	669	672	679	rVB4	371	350	0.02%	0.002%
13	3.272	689	694	697	rBV	216	245	0.01%	0.002%
14	3.339	710	715	721	rVB3	339	395	0.02%	0.003%
15	3.735	833	838	841	rBV3	308	352	0.02%	0.002%
16	3.764	844	847	856	rVB3	299	294	0.02%	0.002%
17	3.870	868	880	932	rBV	131899	393785	21.88%	2.782%
18	4.339	1008	1026	1062	rBV	270114	678452	37.71%	4.794%
19	4.664	1121	1127	1132	rBV4	578	860	0.05%	0.006%
20	4.751	1151	1154	1159	rVB2	265	258	0.01%	0.002%
21	5.040	1223	1244	1292	rBV2	682971	1799340	100.00%	12.714%
22	5.404	1348	1357	1361	rVB4	309	523	0.03%	0.004%
23	5.477	1374	1380	1384	rBV3	437	402	0.02%	0.003%
24	5.542	1393	1400	1404	rVB4	435	514	0.03%	0.004%
25	5.609	1404	1421	1447	rBV	570390	1149780	63.90%	8.124%
26	5.905	1500	1513	1526	rBV7	6072	13625	0.76%	0.096%
27	6.063	1545	1562	1595	rBV	374944	784195	43.58%	5.541%
28	6.194	1600	1603	1609	rVB4	861	986	0.05%	0.007%
29	6.291	1629	1633	1638	rVV3	298	273	0.02%	0.002%
30	6.394	1662	1665	1668	rBV2	463	328	0.02%	0.002%
31	6.416	1668	1672	1676	rVB3	349	256	0.01%	0.002%
32	6.497	1695	1697	1699	rBV2	400	236	0.01%	0.002%
33	6.625	1732	1737	1746	rVV5	805	1461	0.08%	0.010%
34	6.699	1758	1760	1765	rBV3	363	241	0.01%	0.002%
35	6.751	1770	1776	1778	rBV3	291	329	0.02%	0.002%
36	6.773	1780	1783	1787	rVV3	298	318	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029512.D
 Acq On : 09 Dec 2022 11:39
 Operator : SY/MD
 Sample : VV1209WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK303

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.796	1788	1790	1797	rVB2	447	292	0.02%	0.002%
38	6.915	1820	1827	1831	rBV2	258	315	0.02%	0.002%
39	6.979	1834	1847	1871	rBV	188977	348086	19.35%	2.460%
40	7.233	1921	1926	1934	rVB7	1151	1679	0.09%	0.012%
41	7.307	1937	1949	1985	rBV	848545	1506130	83.70%	10.642%
42	7.535	2018	2020	2025	rVB2	625	414	0.02%	0.003%
43	7.564	2025	2029	2033	rBV4	300	343	0.02%	0.002%
44	7.612	2033	2044	2075	rVV	130922	234730	13.05%	1.659%
45	7.754	2085	2088	2093	rBV4	560	548	0.03%	0.004%
46	7.838	2109	2114	2118	rBV3	793	631	0.04%	0.004%
47	7.915	2135	2138	2140	rBV2	432	326	0.02%	0.002%
48	7.928	2140	2142	2144	rBV2	577	337	0.02%	0.002%
49	7.973	2149	2156	2168	rVB5	3521	6112	0.34%	0.043%
50	8.082	2180	2190	2222	rBV	482674	858422	47.71%	6.066%
51	8.317	2260	2263	2266	rBV2	378	277	0.02%	0.002%
52	8.416	2285	2294	2306	rVB5	3249	6203	0.34%	0.044%
53	8.487	2313	2316	2319	rBV2	481	395	0.02%	0.003%
54	8.519	2324	2326	2331	rBV6	363	286	0.02%	0.002%
55	8.574	2338	2343	2345	rBV2	232	229	0.01%	0.002%
56	8.667	2366	2372	2375	rBV4	391	417	0.02%	0.003%
57	8.844	2414	2427	2448	rBV	823452	1354654	75.29%	9.572%
58	9.008	2472	2478	2486	rVB4	2383	3502	0.19%	0.025%
59	9.063	2491	2495	2499	rVB3	496	386	0.02%	0.003%
60	9.085	2500	2502	2509	rVB4	471	316	0.02%	0.002%
61	9.136	2509	2518	2527	rBV4	2620	4293	0.24%	0.030%
62	9.194	2531	2536	2542	rBV4	272	293	0.02%	0.002%
63	9.307	2564	2571	2573	rBV2	334	276	0.02%	0.002%
64	9.358	2582	2587	2589	rBV3	390	265	0.01%	0.002%
65	9.551	2634	2647	2648	rBV5	2223	3425	0.19%	0.024%
66	9.632	2668	2672	2675	rBV2	427	358	0.02%	0.003%
67	9.828	2726	2733	2738	rVB3	447	532	0.03%	0.004%
68	9.924	2756	2763	2770	rVV3	2204	2948	0.16%	0.021%
69	10.072	2805	2809	2814	rVB4	542	439	0.02%	0.003%
70	10.162	2827	2837	2841	rBV2	28518	41568	2.31%	0.294%
71	10.207	2841	2851	2875	rVB	545832	870400	48.37%	6.150%
72	10.442	2918	2924	2925	rBV3	393	402	0.02%	0.003%
73	10.464	2925	2931	2935	rVV3	607	722	0.04%	0.005%
74	10.532	2941	2952	2955	rBV4	2375	2835	0.16%	0.020%
75	10.567	2955	2963	2978	rVB2	13953	22558	1.25%	0.159%
76	10.702	2999	3005	3007	rBV3	361	298	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029512.D
 Acq On : 09 Dec 2022 11:39
 Operator : SY/MD
 Sample : VV1209WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK303

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.847	3046	3050	3053	rBV3	557	510	0.03%	0.004%
78	10.908	3057	3069	3079	rBV3	3837	6280	0.35%	0.044%
79	11.014	3099	3102	3108	rVB2	472	388	0.02%	0.003%
80	11.175	3142	3152	3159	rBV4	4494	6987	0.39%	0.049%
81	11.239	3159	3172	3192	rBV	898891	1423147	79.09%	10.056%
82	11.400	3219	3222	3229	rVB3	582	660	0.04%	0.005%
83	11.442	3230	3235	3238	rBV3	468	469	0.03%	0.003%
84	11.612	3275	3288	3312	rBV	875759	1398173	77.70%	9.879%
85	11.815	3347	3351	3356	rBV3	337	304	0.02%	0.002%
86	11.908	3376	3380	3387	rBV3	624	712	0.04%	0.005%
87	12.188	3462	3467	3470	rBV3	321	323	0.02%	0.002%
88	12.323	3507	3509	3512	rVB2	475	247	0.01%	0.002%
89	12.419	3533	3539	3544	rVB5	911	1129	0.06%	0.008%
90	12.558	3579	3582	3585	rBV2	495	362	0.02%	0.003%
91	12.635	3599	3606	3615	rVV4	4781	7376	0.41%	0.052%
92	12.760	3642	3645	3650	rBV4	274	265	0.01%	0.002%
93	12.837	3664	3669	3670	rBV3	364	314	0.02%	0.002%
94	12.979	3710	3713	3717	rBV2	383	360	0.02%	0.003%
95	13.159	3764	3769	3772	rBV3	413	417	0.02%	0.003%
96	13.252	3788	3798	3815	rVB3	9469	14748	0.82%	0.104%
97	13.493	3855	3873	3887	rBV	29847	54964	3.05%	0.388%
98	13.648	3919	3921	3923	rBV2	529	242	0.01%	0.002%
99	13.731	3938	3947	3963	rVB3	10115	15764	0.88%	0.111%
100	13.808	3969	3971	3974	rBV3	454	264	0.01%	0.002%




Sum of corrected areas: 14152336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029512.D
Acq On : 09 Dec 2022 11:39
Operator : SY/MD
Sample : VV1209WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK303

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

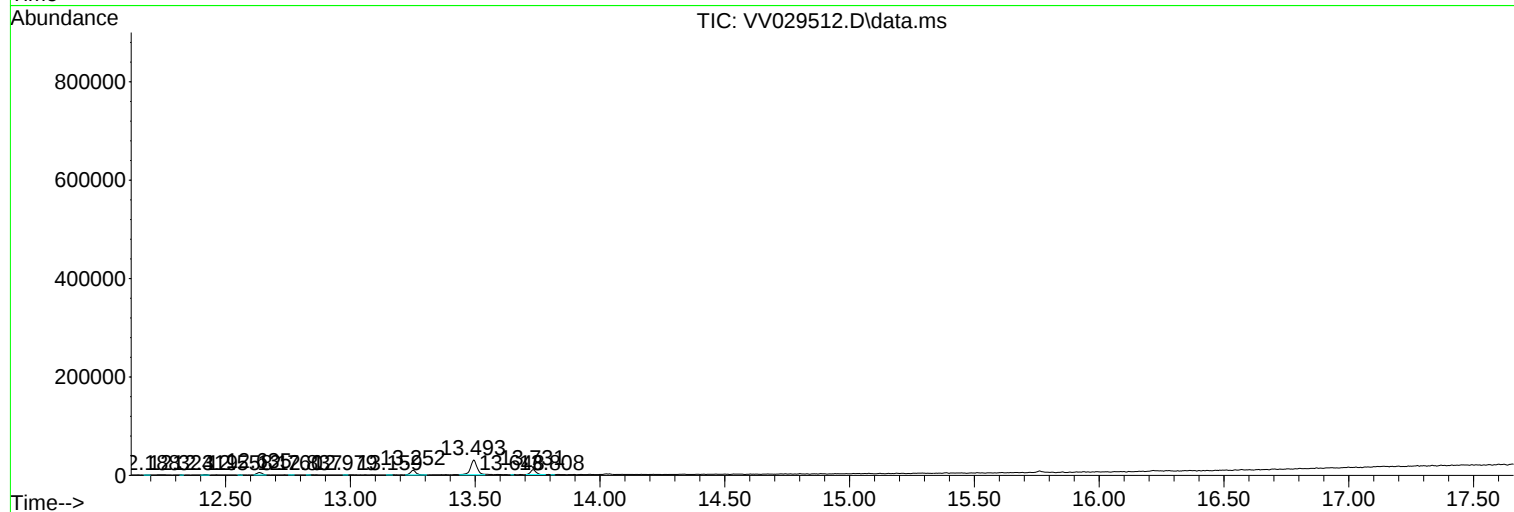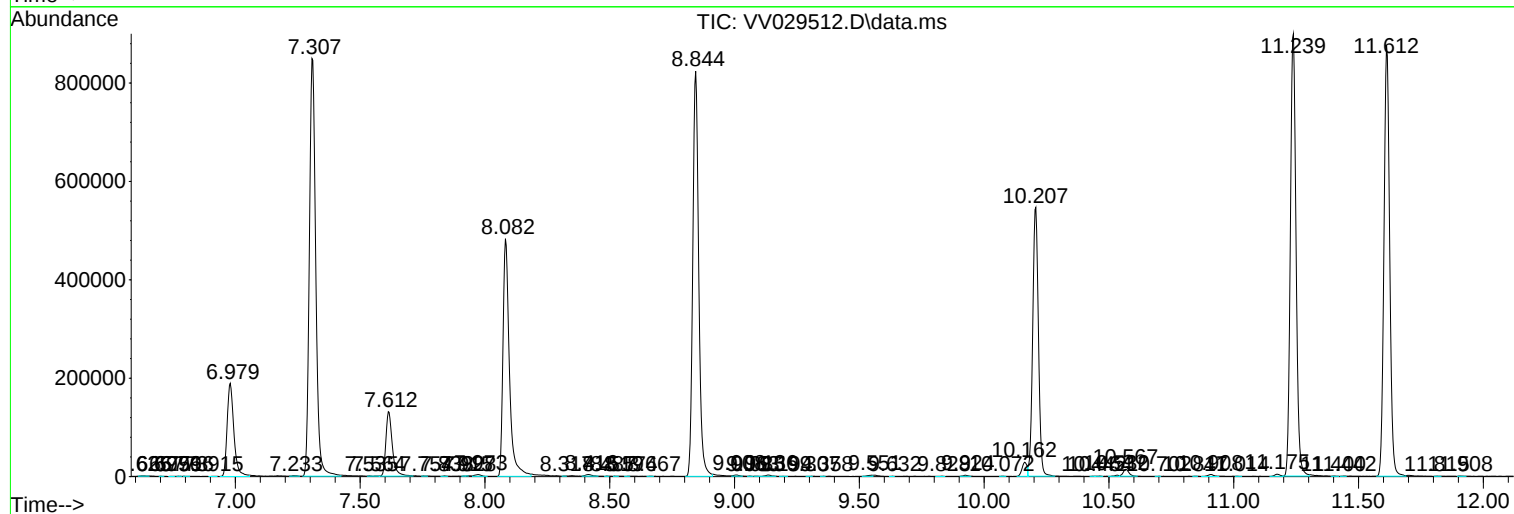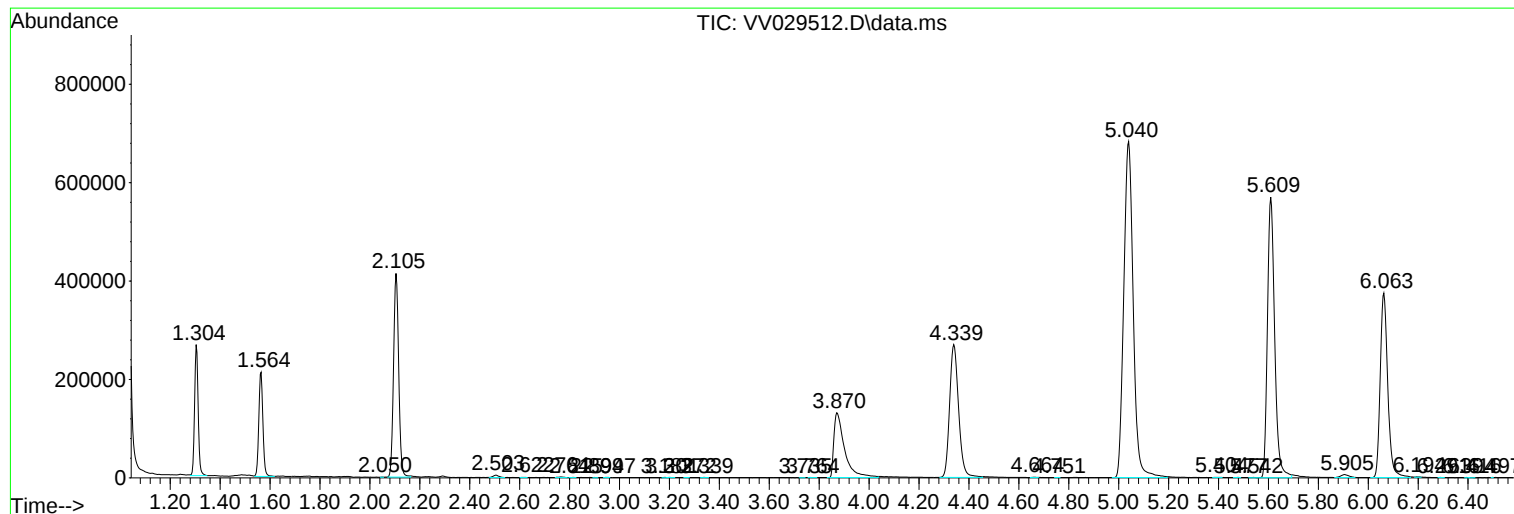

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029512.D
Acq On : 09 Dec 2022 11:39
Operator : SY/MD
Sample : VV1209WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK303

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029512.D
Acq On : 09 Dec 2022 11:39
Operator : SY/MD
Sample : VV1209WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK303

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------