

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029513.D
 Acq On : 09 Dec 2022 12:02
 Operator : SY/MD
 Sample : N5919-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VW029513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	256244	253202	14.48%	1.747%
2	1.564	155	163	179	rVB	205840	233611	13.36%	1.612%
3	2.105	320	331	364	rBV2	411666	611347	34.95%	4.219%
4	2.445	434	437	439	rBV	342	221	0.01%	0.002%
5	2.503	446	455	472	rVB2	6907	11725	0.67%	0.081%
6	2.603	484	486	487	rBV	387	185	0.01%	0.001%
7	2.709	516	519	522	rBV2	353	266	0.02%	0.002%
8	2.764	528	536	543	rVB4	1017	1579	0.09%	0.011%
9	2.850	558	563	566	rBV2	306	275	0.02%	0.002%
10	3.076	631	633	639	rVB3	196	152	0.01%	0.001%
11	3.127	646	649	653	rVB2	355	238	0.01%	0.002%
12	3.150	653	656	658	rBV3	301	199	0.01%	0.001%
13	3.159	658	659	661	rBV	224	97	0.01%	0.001%
14	3.178	661	665	666	rBV2	502	308	0.02%	0.002%
15	3.291	697	700	705	rVB2	257	173	0.01%	0.001%
16	3.368	721	724	726	rBV2	172	126	0.01%	0.001%
17	3.420	737	740	743	rBV	162	107	0.01%	0.001%
18	3.439	743	746	749	rVV	240	133	0.01%	0.001%
19	3.455	749	751	754	rVB	233	104	0.01%	0.001%
20	3.513	767	769	773	rBV2	234	135	0.01%	0.001%
21	3.613	798	800	804	rVB	302	164	0.01%	0.001%
22	3.703	823	828	831	rBV3	202	215	0.01%	0.001%
23	3.767	845	848	852	rVB2	213	157	0.01%	0.001%
24	3.802	856	859	863	rBV2	128	103	0.01%	0.001%
25	3.873	868	881	915	rBV	134021	430902	24.64%	2.973%
26	4.339	1009	1026	1054	rBV	267542	660324	37.76%	4.556%
27	4.603	1096	1108	1120	rVB3	11510	26410	1.51%	0.182%
28	4.719	1142	1144	1147	rBV2	239	151	0.01%	0.001%
29	4.773	1157	1161	1163	rVB2	315	215	0.01%	0.001%
30	4.886	1191	1196	1199	rBV2	302	216	0.01%	0.001%
31	4.912	1199	1204	1207	rBV2	380	283	0.02%	0.002%
32	4.931	1207	1210	1214	rVB2	218	147	0.01%	0.001%
33	4.979	1222	1225	1226	rBV	158	106	0.01%	0.001%
34	5.040	1226	1244	1287	rBV2	666905	1748965	100.00%	12.069%
35	5.397	1350	1355	1358	rBV2	434	445	0.03%	0.003%
36	5.461	1371	1375	1377	rBV2	335	255	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029513.D
 Acq On : 09 Dec 2022 12:02
 Operator : SY/MD
 Sample : N5919-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.609	1408	1421	1453	rBV	555169	1132070	64.73%	7.812%
38	5.908	1501	1514	1547	rBV	346173	701827	40.13%	4.843%
39	6.063	1550	1562	1594	rVB	370786	758921	43.39%	5.237%
40	6.304	1635	1637	1641	rVB	343	229	0.01%	0.002%
41	6.439	1675	1679	1682	rBV2	281	238	0.01%	0.002%
42	6.484	1689	1693	1696	rBV2	240	139	0.01%	0.001%
43	6.500	1696	1698	1703	rVB2	267	153	0.01%	0.001%
44	6.583	1722	1724	1728	rBV	180	104	0.01%	0.001%
45	6.625	1728	1737	1747	rBV6	1498	2717	0.16%	0.019%
46	6.731	1766	1770	1773	rVB2	362	284	0.02%	0.002%
47	6.773	1779	1783	1786	rBV2	416	330	0.02%	0.002%
48	6.979	1835	1847	1872	rBV	184253	336765	19.26%	2.324%
49	7.307	1937	1949	1988	rBV	824497	1469304	84.01%	10.139%
50	7.612	2034	2044	2070	rBV	126098	225243	12.88%	1.554%
51	7.834	2110	2113	2119	rVB5	1087	950	0.05%	0.007%
52	8.082	2180	2190	2226	rBV	462727	822968	47.05%	5.679%
53	8.593	2347	2349	2353	rVB2	442	263	0.02%	0.002%
54	8.622	2353	2358	2363	rVB4	492	499	0.03%	0.003%
55	8.644	2363	2365	2369	rVB3	306	253	0.01%	0.002%
56	8.673	2369	2374	2377	rBV2	396	369	0.02%	0.003%
57	8.712	2383	2386	2390	rVB2	475	348	0.02%	0.002%
58	8.741	2390	2395	2398	rBV4	534	514	0.03%	0.004%
59	8.773	2402	2405	2407	rBV2	293	201	0.01%	0.001%
60	8.844	2414	2427	2456	rBV	810374	1329079	75.99%	9.171%
61	9.082	2499	2501	2504	rVB	348	185	0.01%	0.001%
62	9.098	2504	2506	2508	rBV3	331	208	0.01%	0.001%
63	9.197	2534	2537	2542	rBV3	440	408	0.02%	0.003%
64	9.262	2555	2557	2559	rBV2	307	168	0.01%	0.001%
65	9.275	2559	2561	2563	rVB	505	239	0.01%	0.002%
66	9.291	2563	2566	2568	rBV	203	112	0.01%	0.001%
67	9.387	2594	2596	2601	rVB2	356	213	0.01%	0.001%
68	9.423	2601	2607	2608	rBV	239	208	0.01%	0.001%
69	9.452	2613	2616	2620	rBV2	195	151	0.01%	0.001%
70	9.474	2620	2623	2628	rBV2	166	119	0.01%	0.001%
71	9.503	2628	2632	2634	rBV	342	255	0.01%	0.002%
72	9.542	2637	2644	2645	rBV2	1336	1282	0.07%	0.009%
73	9.635	2670	2673	2676	rVB	272	128	0.01%	0.001%
74	9.664	2678	2682	2684	rBV2	307	267	0.02%	0.002%
75	9.751	2706	2709	2712	rBV2	252	125	0.01%	0.001%
76	9.770	2712	2715	2720	rBV2	358	321	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029513.D
 Acq On : 09 Dec 2022 12:02
 Operator : SY/MD
 Sample : N5919-02DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EF0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.927	2759	2764	2770	rVB4	1189	1488	0.09%	0.010%
78	9.988	2781	2783	2785	rBV2	178	99	0.01%	0.001%
79	10.078	2809	2811	2814	rVB3	347	180	0.01%	0.001%
80	10.162	2826	2837	2841	rBV	30114	43695	2.50%	0.302%
81	10.207	2842	2851	2877	rVB	540463	855580	48.92%	5.904%
82	10.451	2918	2927	2930	rBV4	546	816	0.05%	0.006%
83	10.500	2938	2942	2943	rBV2	190	118	0.01%	0.001%
84	10.529	2945	2951	2955	rVV3	1598	2069	0.12%	0.014%
85	10.567	2955	2963	2977	rVB2	14747	23833	1.36%	0.164%
86	10.644	2984	2987	2989	rBV	318	187	0.01%	0.001%
87	10.841	3046	3048	3049	rBV	524	206	0.01%	0.001%
88	10.908	3062	3069	3080	rVB3	2617	3678	0.21%	0.025%
89	11.091	3124	3126	3128	rBV	259	112	0.01%	0.001%
90	11.168	3146	3150	3152	rBV4	2409	2000	0.11%	0.014%
91	11.239	3160	3172	3193	rBV	901109	1390083	79.48%	9.592%
92	11.509	3254	3256	3258	rBV2	396	160	0.01%	0.001%
93	11.612	3274	3288	3307	rBV	858618	1351747	77.29%	9.328%
94	12.027	3407	3417	3418	rBV2	359	514	0.03%	0.004%
95	12.149	3452	3455	3456	rBV	361	232	0.01%	0.002%
96	12.419	3534	3539	3542	rBV3	681	750	0.04%	0.005%
97	12.635	3601	3606	3618	rVB6	2868	4455	0.25%	0.031%
98	13.252	3791	3798	3811	rVB4	5192	7478	0.43%	0.052%
99	13.496	3866	3874	3888	rVB	13725	23360	1.34%	0.161%
100	13.734	3940	3948	3956	rBV5	5067	7681	0.44%	0.053%




Sum of corrected areas: 14491919

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029513.D
Acq On : 09 Dec 2022 12:02
Operator : SY/MD
Sample : N5919-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

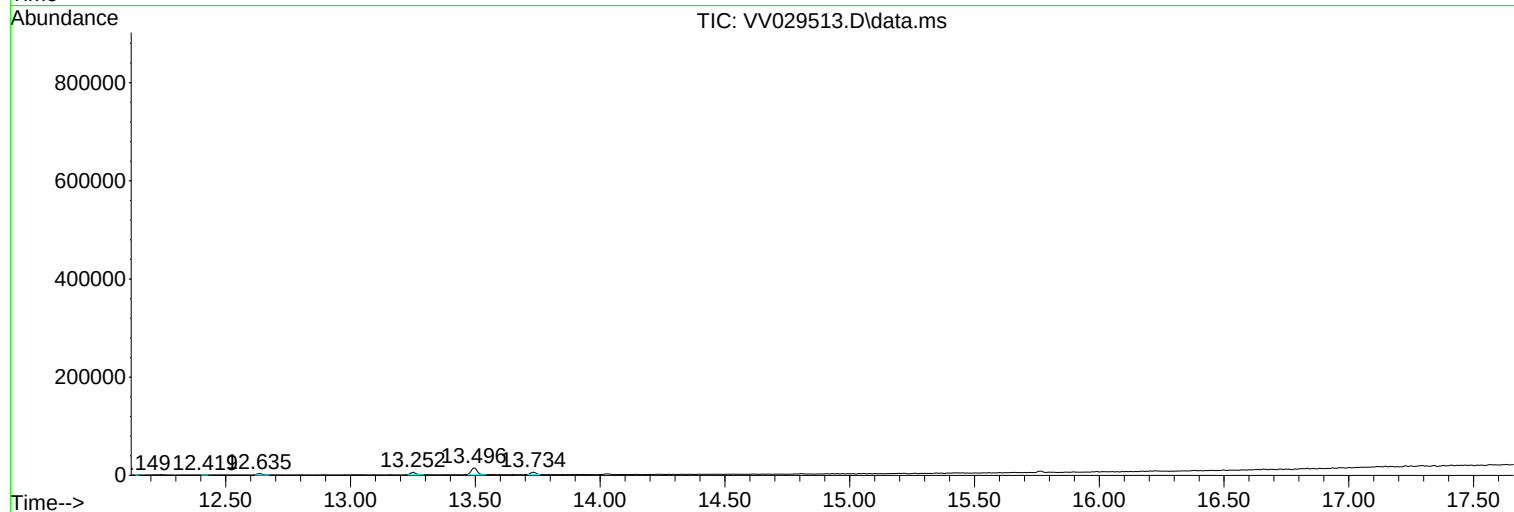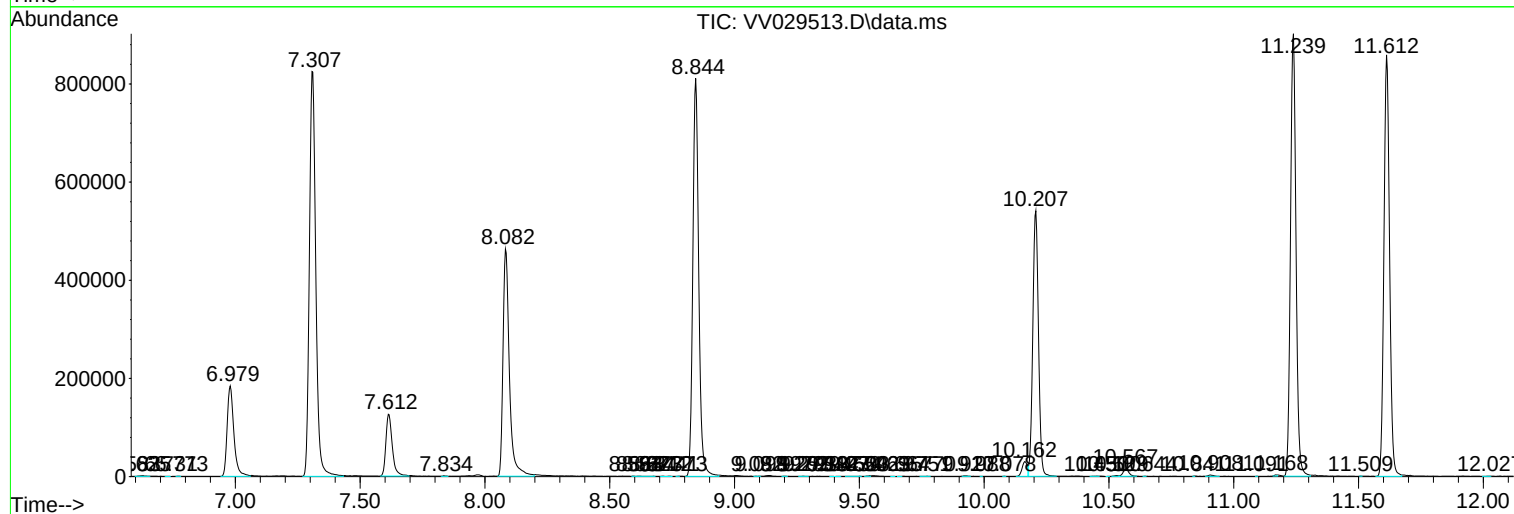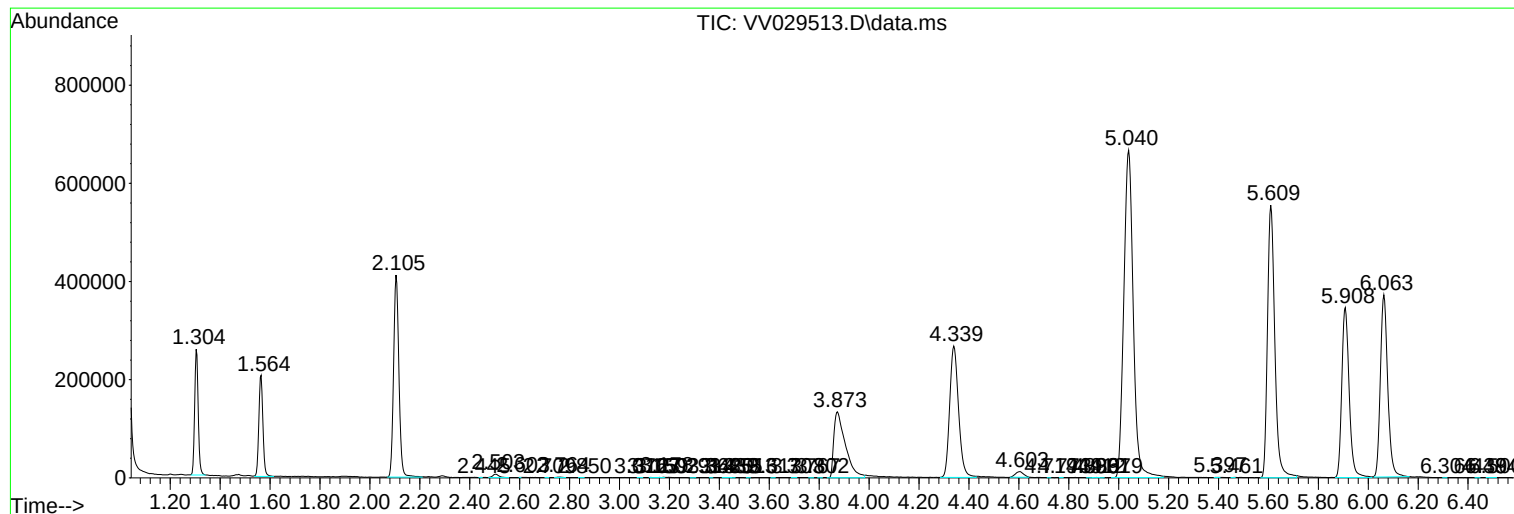

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029513.D
Acq On : 09 Dec 2022 12:02
Operator : SY/MD
Sample : N5919-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029513.D
Acq On : 09 Dec 2022 12:02
Operator : SY/MD
Sample : N5919-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EF0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------