

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029514.D
 Acq On : 09 Dec 2022 12:26
 Operator : SY/MD
 Sample : N5919-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029514.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rVB	272859	268338	14.48%	1.969%
2	1.564	155	163	180	rVB	219224	246105	13.28%	1.806%
3	2.056	313	316	318	rBV2	424	288	0.02%	0.002%
4	2.104	320	331	344	rBV	428046	613806	33.12%	4.503%
5	2.278	378	385	399	rVB3	5678	11913	0.64%	0.087%
6	2.500	448	454	467	rVB5	1506	2668	0.14%	0.020%
7	2.555	467	471	476	rVB2	330	315	0.02%	0.002%
8	2.616	486	490	497	rBV4	564	699	0.04%	0.005%
9	2.706	513	518	523	rVB2	265	291	0.02%	0.002%
10	2.757	530	534	538	rBV2	642	724	0.04%	0.005%
11	2.924	576	586	589	rBV2	377	499	0.03%	0.004%
12	2.976	599	602	604	rBV	302	228	0.01%	0.002%
13	3.320	705	709	714	rVB2	276	252	0.01%	0.002%
14	3.870	863	880	916	rBV	127043	350429	18.91%	2.571%
15	4.339	1008	1026	1064	rBV	283117	706487	38.12%	5.183%
16	4.632	1110	1117	1119	rBV2	568	559	0.03%	0.004%
17	4.940	1209	1213	1216	rBV3	305	226	0.01%	0.002%
18	5.040	1224	1244	1283	rBV2	705418	1853451	100.00%	13.599%
19	5.326	1331	1333	1336	rVB2	461	276	0.01%	0.002%
20	5.349	1336	1340	1342	rBV2	365	271	0.01%	0.002%
21	5.471	1374	1378	1381	rBV2	533	470	0.03%	0.003%
22	5.609	1408	1421	1469	rBV	478701	978606	52.80%	7.180%
23	5.789	1475	1477	1484	rVV4	448	431	0.02%	0.003%
24	5.905	1502	1513	1528	rVB7	5672	13318	0.72%	0.098%
25	5.969	1528	1533	1538	rBV2	378	388	0.02%	0.003%
26	6.063	1547	1562	1597	rBV	391741	812614	43.84%	5.962%
27	6.979	1835	1847	1877	rBV	192753	359931	19.42%	2.641%
28	7.140	1894	1897	1899	rBV2	496	303	0.02%	0.002%
29	7.307	1937	1949	1989	rBV	886857	1561800	84.26%	11.459%
30	7.612	2034	2044	2077	rBV	136449	244543	13.19%	1.794%
31	7.847	2112	2117	2120	rBV2	533	518	0.03%	0.004%
32	7.934	2133	2144	2163	rBV2	13230	27848	1.50%	0.204%
33	8.082	2180	2190	2234	rBV	462949	826530	44.59%	6.064%
34	8.506	2316	2322	2323	rBV2	227	222	0.01%	0.002%
35	8.538	2330	2332	2337	rVV3	319	230	0.01%	0.002%
36	8.606	2350	2353	2357	rVB2	508	351	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029514.D
 Acq On : 09 Dec 2022 12:26
 Operator : SY/MD
 Sample : N5919-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	8.635	2360	2362	2366	rVB3	421	264	0.01%	0.002%
38	8.661	2366	2370	2373	rVB3	415	371	0.02%	0.003%
39	8.686	2373	2378	2381	rBV3	428	512	0.03%	0.004%
40	8.709	2381	2385	2389	rVB2	322	307	0.02%	0.002%
41	8.786	2406	2409	2412	rBV	461	367	0.02%	0.003%
42	8.844	2415	2427	2459	rBV	698048	1152473	62.18%	8.456%
43	9.062	2490	2495	2497	rBV3	435	410	0.02%	0.003%
44	9.098	2502	2506	2507	rBV	303	237	0.01%	0.002%
45	9.133	2511	2517	2526	rBV5	1370	2155	0.12%	0.016%
46	9.201	2533	2538	2542	rBV2	339	347	0.02%	0.003%
47	9.236	2547	2549	2555	rVB3	325	263	0.01%	0.002%
48	9.275	2555	2561	2567	rVB2	384	416	0.02%	0.003%
49	9.323	2567	2576	2579	rBV3	406	458	0.02%	0.003%
50	9.477	2618	2624	2631	rBV2	298	410	0.02%	0.003%
51	9.538	2637	2643	2646	rBV	977	1039	0.06%	0.008%
52	9.689	2687	2690	2695	rVB2	352	333	0.02%	0.002%
53	9.731	2701	2703	2707	rVB2	363	249	0.01%	0.002%
54	9.824	2727	2732	2738	rBV3	277	451	0.02%	0.003%
55	9.924	2756	2763	2769	rVV4	1030	1401	0.08%	0.010%
56	9.995	2781	2785	2788	rBV2	284	229	0.01%	0.002%
57	10.075	2806	2810	2815	rBV4	499	569	0.03%	0.004%
58	10.162	2826	2837	2841	rBV	30635	44759	2.41%	0.328%
59	10.207	2841	2851	2873	rVB	562154	892296	48.14%	6.547%
60	10.374	2892	2903	2915	rVB	13056	21674	1.17%	0.159%
61	10.439	2920	2923	2925	rBV2	483	267	0.01%	0.002%
62	10.487	2937	2938	2943	rVB2	344	227	0.01%	0.002%
63	10.532	2945	2952	2954	rBV	1021	1015	0.05%	0.007%
64	10.567	2954	2963	2975	rVB	15411	23801	1.28%	0.175%
65	10.641	2982	2986	2988	rBV2	358	296	0.02%	0.002%
66	10.850	3045	3051	3061	rVB4	618	957	0.05%	0.007%
67	10.905	3061	3068	3081	rBV4	2456	3886	0.21%	0.029%
68	11.017	3099	3103	3106	rBV3	354	356	0.02%	0.003%
69	11.172	3145	3151	3160	rVB3	2274	3216	0.17%	0.024%
70	11.239	3160	3172	3194	rBV	745124	1168281	63.03%	8.572%
71	11.381	3213	3216	3219	rBV3	356	238	0.01%	0.002%
72	11.451	3235	3238	3242	rVB2	395	278	0.01%	0.002%
73	11.541	3262	3266	3267	rBV2	424	270	0.01%	0.002%
74	11.557	3268	3271	3274	rVB2	500	277	0.01%	0.002%
75	11.612	3276	3288	3314	rBV	871799	1379670	74.44%	10.123%
76	11.821	3351	3353	3359	rVB3	460	363	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029514.D
 Acq On : 09 Dec 2022 12:26
 Operator : SY/MD
 Sample : N5919-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.853	3359	3363	3367	rBV3	419	321	0.02%	0.002%
78	11.876	3368	3370	3375	rBV2	297	237	0.01%	0.002%
79	11.914	3379	3382	3385	rBV4	485	315	0.02%	0.002%
80	12.139	3449	3452	3454	rBV2	292	219	0.01%	0.002%
81	12.184	3463	3466	3470	rBV3	289	243	0.01%	0.002%
82	12.242	3476	3484	3491	rBV3	2649	3990	0.22%	0.029%
83	12.303	3500	3503	3508	rVB3	254	225	0.01%	0.002%
84	12.336	3511	3513	3518	rVB2	518	275	0.01%	0.002%
85	12.371	3518	3524	3526	rBV2	395	325	0.02%	0.002%
86	12.413	3534	3537	3542	rBV3	372	284	0.02%	0.002%
87	12.490	3558	3561	3565	rVV3	494	414	0.02%	0.003%
88	12.635	3599	3606	3614	rBV7	2691	3848	0.21%	0.028%
89	12.834	3664	3668	3673	rBV5	480	479	0.03%	0.004%
90	12.950	3700	3704	3706	rBV2	339	226	0.01%	0.002%
91	13.091	3744	3748	3750	rBV2	374	274	0.01%	0.002%
92	13.255	3789	3799	3807	rBV6	3510	5952	0.32%	0.044%
93	13.326	3817	3821	3823	rBV	388	357	0.02%	0.003%
94	13.496	3863	3874	3889	rVB2	7350	13502	0.73%	0.099%
95	13.551	3889	3891	3895	rBV2	476	387	0.02%	0.003%
96	13.635	3915	3917	3921	rBV3	338	252	0.01%	0.002%
97	13.728	3941	3946	3956	rVB5	3122	4803	0.26%	0.035%
98	13.853	3982	3985	3986	rBV	477	275	0.01%	0.002%
99	13.898	3996	3999	4004	rBV4	808	697	0.04%	0.005%
100	15.123	4378	4380	4381	rBV2	949	362	0.02%	0.003%




Sum of corrected areas: 13629578

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029514.D
Acq On : 09 Dec 2022 12:26
Operator : SY/MD
Sample : N5919-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

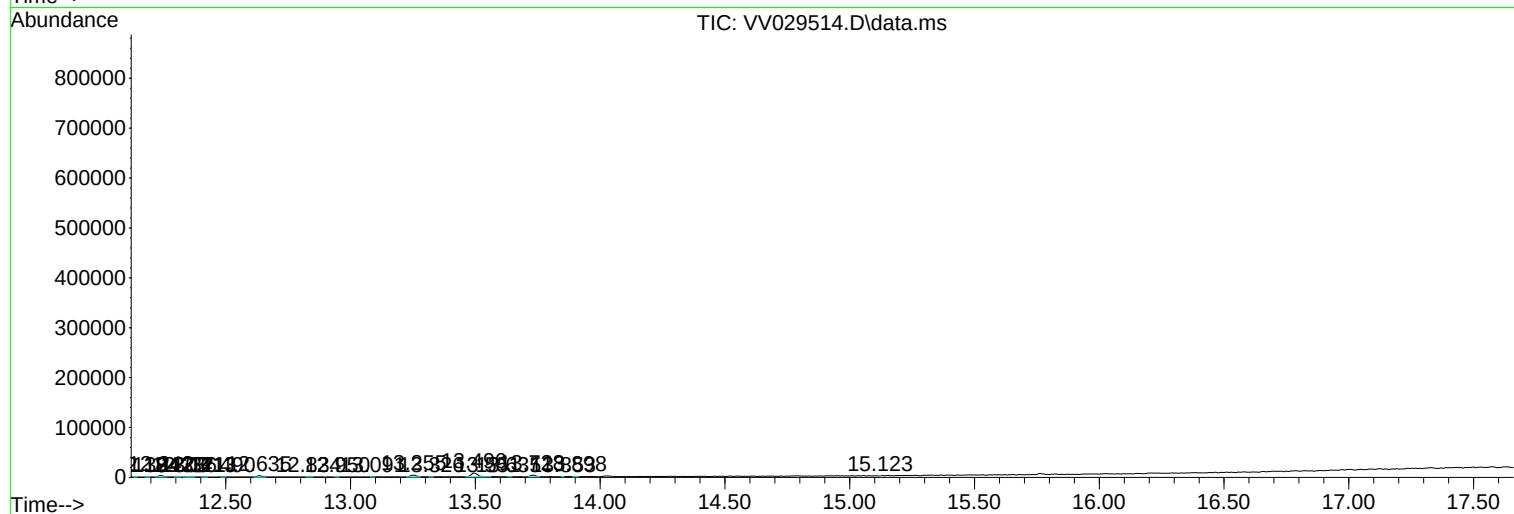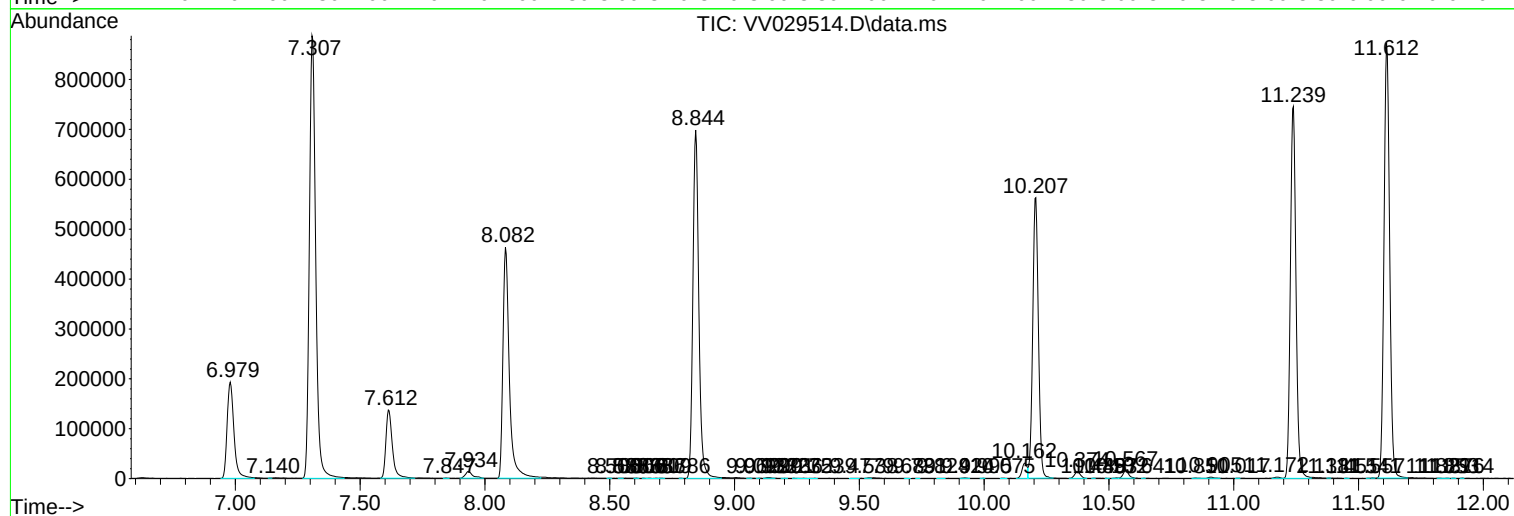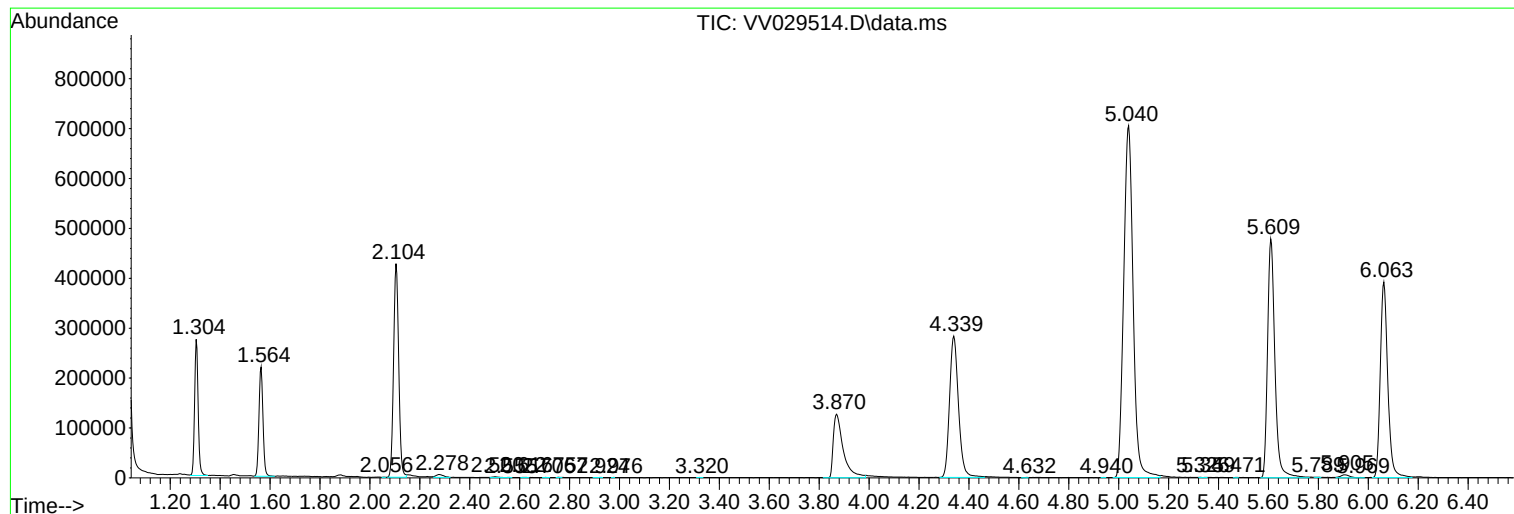

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029514.D
Acq On : 09 Dec 2022 12:26
Operator : SY/MD
Sample : N5919-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029514.D
Acq On : 09 Dec 2022 12:26
Operator : SY/MD
Sample : N5919-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc