

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029515.D
 Acq On : 09 Dec 2022 12:49
 Operator : SY/MD
 Sample : N5919-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029515.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	246637	240767	14.96%	1.921%
2	1.564	155	163	177	rVB	184355	206925	12.86%	1.651%
3	2.105	320	331	345	rBV	364673	522852	32.49%	4.172%
4	2.503	447	455	464	rBV3	3941	6382	0.40%	0.051%
5	2.564	471	474	476	rBV2	185	124	0.01%	0.001%
6	2.671	503	507	510	rBV3	226	195	0.01%	0.002%
7	2.767	531	537	544	rVB6	765	1156	0.07%	0.009%
8	2.912	578	582	585	rBV2	369	354	0.02%	0.003%
9	3.040	618	622	624	rBV	202	128	0.01%	0.001%
10	3.085	634	636	640	rBV2	193	147	0.01%	0.001%
11	3.185	663	667	668	rBV	245	157	0.01%	0.001%
12	3.285	695	698	702	rVB	225	138	0.01%	0.001%
13	3.468	752	755	760	rVB2	229	138	0.01%	0.001%
14	3.571	784	787	790	rBV	184	140	0.01%	0.001%
15	3.725	832	835	839	rVB	178	138	0.01%	0.001%
16	3.761	839	846	851	rBV2	238	379	0.02%	0.003%
17	3.873	870	881	938	rBV	121462	367568	22.84%	2.933%
18	4.339	1009	1026	1064	rBV	244406	612120	38.03%	4.884%
19	4.789	1163	1166	1171	rVB2	255	160	0.01%	0.001%
20	4.822	1174	1176	1179	rVV	327	174	0.01%	0.001%
21	4.873	1189	1192	1196	rBV2	368	239	0.01%	0.002%
22	4.928	1207	1209	1211	rVB	273	110	0.01%	0.001%
23	4.941	1211	1213	1215	rBV	262	125	0.01%	0.001%
24	5.040	1225	1244	1293	rBV2	605704	1609377	100.00%	12.841%
25	5.387	1350	1352	1353	rBV	262	117	0.01%	0.001%
26	5.458	1370	1374	1376	rBV2	442	291	0.02%	0.002%
27	5.535	1396	1398	1403	rVB	464	320	0.02%	0.003%
28	5.558	1403	1405	1408	rBV	137	99	0.01%	0.001%
29	5.609	1408	1421	1452	rBV	501950	1014480	63.04%	8.094%
30	5.902	1503	1512	1527	rVV6	5072	11778	0.73%	0.094%
31	6.063	1548	1562	1598	rBV	344039	708660	44.03%	5.654%
32	6.243	1617	1618	1621	rVV2	272	128	0.01%	0.001%
33	6.288	1628	1632	1634	rVB2	223	128	0.01%	0.001%
34	6.323	1641	1643	1645	rBV	207	103	0.01%	0.001%
35	6.394	1663	1665	1669	rVB2	345	130	0.01%	0.001%
36	6.423	1670	1674	1676	rBV	273	213	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029515.D
 Acq On : 09 Dec 2022 12:49
 Operator : SY/MD
 Sample : N5919-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.497	1696	1697	1706	rVB2	435	423	0.03%	0.003%
38	6.542	1706	1711	1714	rBV2	123	129	0.01%	0.001%
39	6.574	1719	1721	1723	rBV	158	89	0.01%	0.001%
40	6.593	1724	1727	1728	rBV	215	102	0.01%	0.001%
41	6.622	1731	1736	1737	rBV3	887	725	0.05%	0.006%
42	6.735	1767	1771	1773	rBV2	303	268	0.02%	0.002%
43	6.777	1782	1784	1785	rBV	215	85	0.01%	0.001%
44	6.831	1797	1801	1806	rVB3	281	269	0.02%	0.002%
45	6.915	1825	1827	1831	rVB	320	147	0.01%	0.001%
46	6.937	1831	1834	1835	rBV	137	84	0.01%	0.001%
47	6.979	1835	1847	1875	rBV	167228	311729	19.37%	2.487%
48	7.162	1897	1904	1905	rBV3	1004	1025	0.06%	0.008%
49	7.233	1922	1926	1927	rBV2	687	485	0.03%	0.004%
50	7.307	1937	1949	1988	rBV	754258	1334142	82.90%	10.645%
51	7.616	2034	2045	2064	rBV	118637	210490	13.08%	1.679%
52	7.863	2117	2122	2125	rBV3	490	458	0.03%	0.004%
53	7.934	2135	2144	2149	rBV4	1582	2855	0.18%	0.023%
54	8.082	2180	2190	2231	rBV	435034	782557	48.62%	6.244%
55	8.558	2335	2338	2340	rBV2	308	221	0.01%	0.002%
56	8.625	2356	2359	2360	rBV2	202	117	0.01%	0.001%
57	8.728	2385	2391	2392	rBV2	325	281	0.02%	0.002%
58	8.789	2403	2410	2411	rBV	178	192	0.01%	0.002%
59	8.844	2413	2427	2458	rBV	732532	1212230	75.32%	9.672%
60	9.140	2510	2519	2527	rBV5	1303	2294	0.14%	0.018%
61	9.194	2534	2536	2539	rBV2	313	153	0.01%	0.001%
62	9.236	2547	2549	2551	rBV	246	109	0.01%	0.001%
63	9.304	2566	2570	2576	rBV3	277	272	0.02%	0.002%
64	9.333	2576	2579	2582	rBV	307	210	0.01%	0.002%
65	9.349	2582	2584	2586	rBV2	188	85	0.01%	0.001%
66	9.362	2586	2588	2593	rVV2	188	128	0.01%	0.001%
67	9.510	2631	2634	2638	rBV2	262	173	0.01%	0.001%
68	9.538	2638	2643	2644	rBV3	871	822	0.05%	0.007%
69	9.606	2662	2664	2666	rBV	166	82	0.01%	0.001%
70	9.773	2712	2716	2718	rBV2	472	298	0.02%	0.002%
71	9.821	2728	2731	2732	rBV2	212	112	0.01%	0.001%
72	9.873	2745	2747	2751	rBV2	232	145	0.01%	0.001%
73	9.931	2755	2765	2774	rVV5	914	1642	0.10%	0.013%
74	9.979	2778	2780	2783	rBV2	251	140	0.01%	0.001%
75	10.043	2796	2800	2804	rBV	172	142	0.01%	0.001%
76	10.066	2804	2807	2808	rBV	240	164	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029515.D
 Acq On : 09 Dec 2022 12:49
 Operator : SY/MD
 Sample : N5919-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.162	2827	2837	2841	rBV2	25907	38040	2.36%	0.304%
78	10.207	2842	2851	2875	rVB	502752	794227	49.35%	6.337%
79	10.368	2898	2901	2903	rBV3	693	510	0.03%	0.004%
80	10.445	2922	2925	2929	rVB3	395	370	0.02%	0.003%
81	10.471	2931	2933	2937	rVB3	348	245	0.02%	0.002%
82	10.497	2937	2941	2943	rBV2	296	179	0.01%	0.001%
83	10.509	2943	2945	2946	rBV	185	98	0.01%	0.001%
84	10.522	2946	2949	2950	rBV	660	455	0.03%	0.004%
85	10.567	2956	2963	2973	rVB2	12173	18533	1.15%	0.148%
86	10.722	3009	3011	3013	rBV	362	174	0.01%	0.001%
87	10.799	3033	3035	3036	rBV2	183	98	0.01%	0.001%
88	10.844	3046	3049	3051	rBV2	464	340	0.02%	0.003%
89	11.030	3103	3107	3110	rVB	341	258	0.02%	0.002%
90	11.091	3124	3126	3130	rVB	294	155	0.01%	0.001%
91	11.108	3130	3131	3135	rBV	174	110	0.01%	0.001%
92	11.175	3145	3152	3159	rVB4	2312	3038	0.19%	0.024%
93	11.236	3159	3171	3194	rBV	813809	1259550	78.26%	10.050%
94	11.439	3231	3234	3238	rBV2	619	466	0.03%	0.004%
95	11.526	3258	3261	3264	rBV2	258	207	0.01%	0.002%
96	11.612	3275	3288	3313	rBV	789291	1242322	77.19%	9.912%
97	11.943	3388	3391	3393	rBV2	119	83	0.01%	0.001%
98	11.966	3395	3398	3401	rVV2	416	271	0.02%	0.002%
99	12.403	3532	3534	3539	rVB2	449	257	0.02%	0.002%
100	12.587	3586	3591	3597	rBV3	514	554	0.03%	0.004%




Sum of corrected areas: 12533054

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029515.D
Acq On : 09 Dec 2022 12:49
Operator : SY/MD
Sample : N5919-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

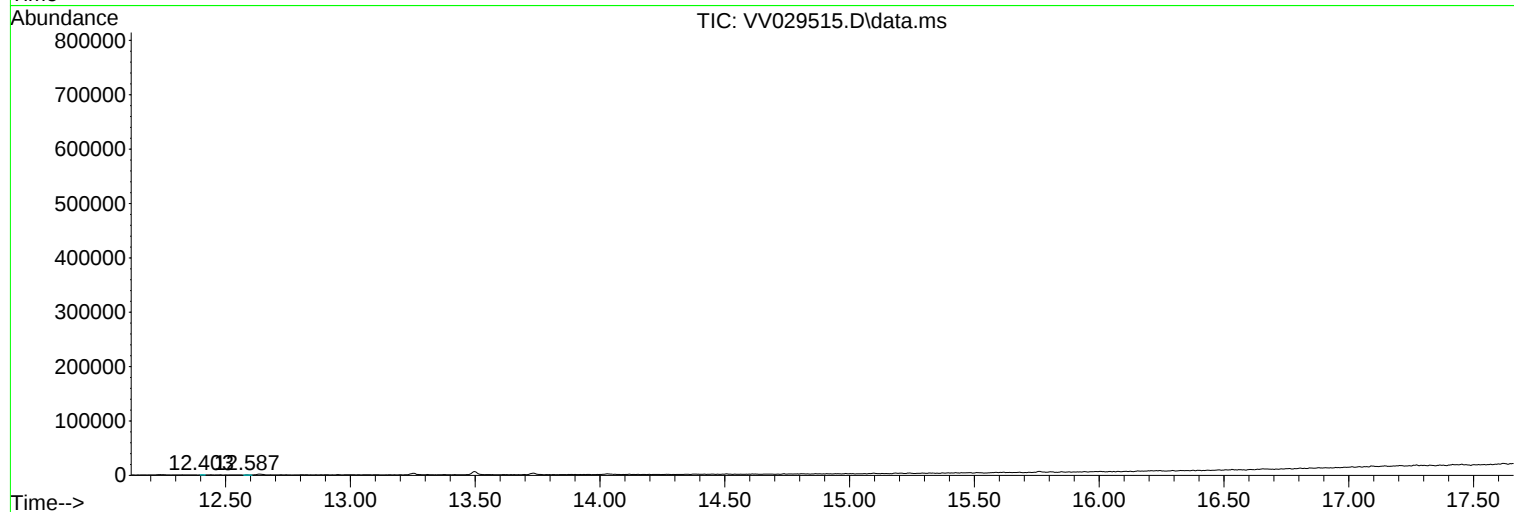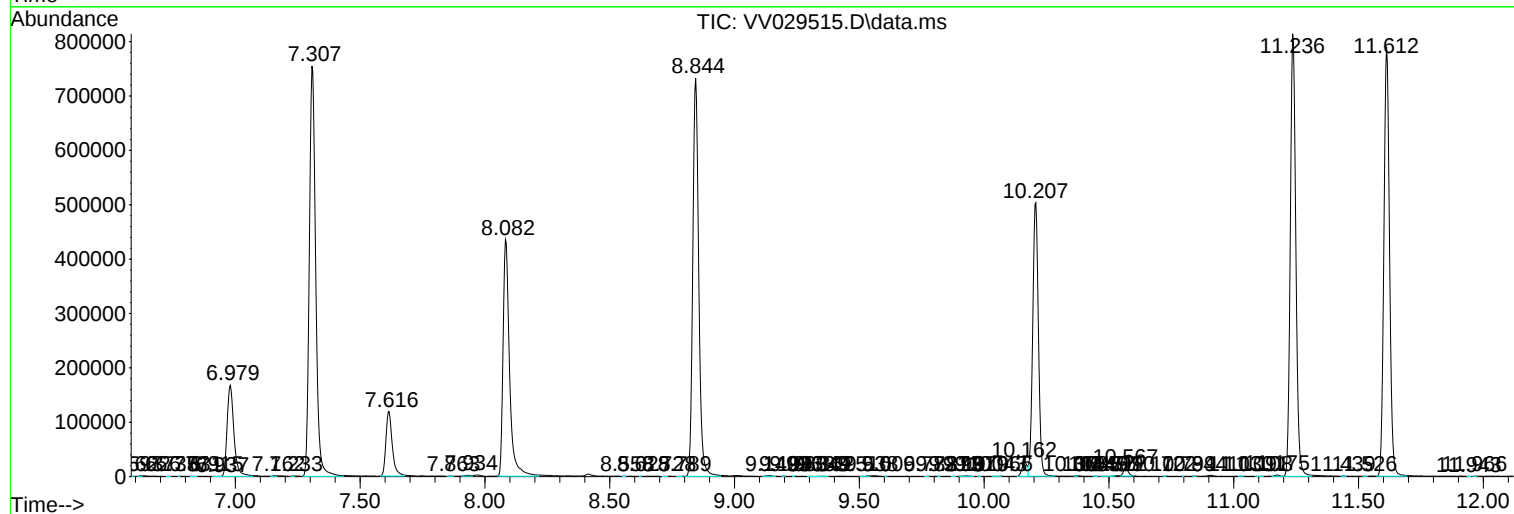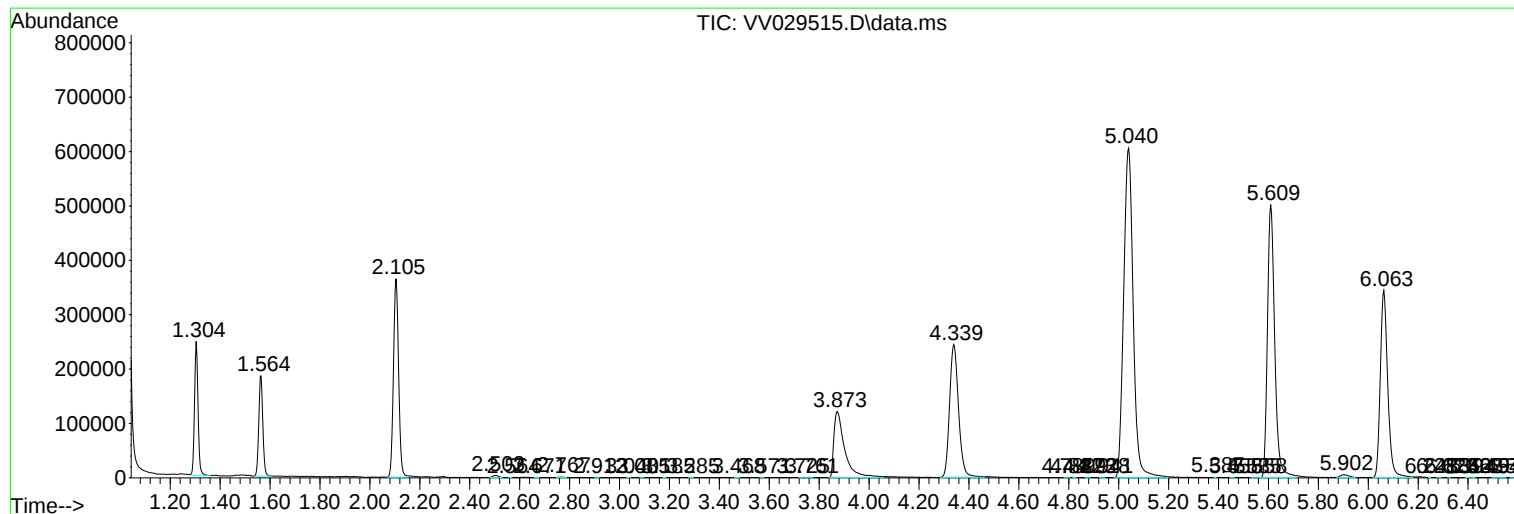

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029515.D
Acq On : 09 Dec 2022 12:49
Operator : SY/MD
Sample : N5919-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029515.D
Acq On : 09 Dec 2022 12:49
Operator : SY/MD
Sample : N5919-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc