

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029516.D
 Acq On : 09 Dec 2022 13:13
 Operator : SY/MD
 Sample : N5920-04DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VV029516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	254883	248122	14.68%	1.868%
2	1.561	155	162	183	rVB	201050	223456	13.22%	1.682%
3	2.105	320	331	344	rBV	388836	558340	33.04%	4.203%
4	2.503	446	455	467	rVB2	11827	19201	1.14%	0.145%
5	2.600	482	485	486	rBV	490	278	0.02%	0.002%
6	2.651	499	501	505	rBV	282	246	0.01%	0.002%
7	3.050	622	625	629	rVV	241	157	0.01%	0.001%
8	3.179	660	665	666	rBV	312	192	0.01%	0.001%
9	3.275	692	695	697	rVB	206	97	0.01%	0.001%
10	3.307	697	705	708	rBV2	226	250	0.01%	0.002%
11	3.327	708	711	715	rVB	204	144	0.01%	0.001%
12	3.510	765	768	772	rVV2	276	175	0.01%	0.001%
13	3.577	786	789	791	rBV	166	110	0.01%	0.001%
14	3.671	815	818	822	rBV2	169	148	0.01%	0.001%
15	3.754	836	844	846	rBV	153	136	0.01%	0.001%
16	3.825	863	866	868	rBV2	264	153	0.01%	0.001%
17	3.870	870	880	923	rBV2	133406	386317	22.86%	2.908%
18	4.339	1010	1026	1061	rBV	257259	641614	37.96%	4.830%
19	4.613	1104	1111	1118	rBV5	683	960	0.06%	0.007%
20	4.638	1118	1119	1123	rVB2	418	204	0.01%	0.002%
21	4.667	1123	1128	1130	rBV3	441	410	0.02%	0.003%
22	4.767	1156	1159	1160	rBV2	390	157	0.01%	0.001%
23	4.851	1182	1185	1187	rVV2	225	160	0.01%	0.001%
24	4.873	1191	1192	1195	rVB	189	83	0.00%	0.001%
25	4.915	1202	1205	1209	rBV2	331	220	0.01%	0.002%
26	4.950	1213	1216	1220	rBV2	311	276	0.02%	0.002%
27	5.040	1225	1244	1270	rBV2	644823	1690045	100.00%	12.723%
28	5.468	1372	1377	1379	rBV2	365	336	0.02%	0.003%
29	5.609	1408	1421	1453	rBV	549639	1119434	66.24%	8.427%
30	5.902	1504	1512	1532	rVB10	4180	8972	0.53%	0.068%
31	6.063	1547	1562	1597	rBV	359345	750952	44.43%	5.653%
32	6.278	1627	1629	1631	rBV	392	148	0.01%	0.001%
33	6.310	1637	1639	1641	rBV	158	97	0.01%	0.001%
34	6.336	1645	1647	1648	rBV	232	100	0.01%	0.001%
35	6.368	1655	1657	1659	rBV	213	109	0.01%	0.001%
36	6.458	1682	1685	1688	rBV2	131	98	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029516.D
 Acq On : 09 Dec 2022 13:13
 Operator : SY/MD
 Sample : N5920-04DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.490	1691	1695	1700	rVB2	280	244	0.01%	0.002%
38	6.519	1701	1704	1705	rBV2	439	179	0.01%	0.001%
39	6.590	1725	1726	1729	rVB2	336	119	0.01%	0.001%
40	6.622	1729	1736	1739	rBV4	1243	1593	0.09%	0.012%
41	6.812	1794	1795	1797	rVV	292	98	0.01%	0.001%
42	6.828	1797	1800	1803	rVB2	376	213	0.01%	0.002%
43	6.905	1822	1824	1826	rBV	147	106	0.01%	0.001%
44	6.921	1826	1829	1832	rVB3	386	253	0.01%	0.002%
45	6.941	1832	1835	1836	rBV2	273	154	0.01%	0.001%
46	6.979	1836	1847	1876	rBV2	177875	327016	19.35%	2.462%
47	7.307	1937	1949	1984	rBV	811144	1430407	84.64%	10.768%
48	7.613	2034	2044	2069	rBV	124461	221937	13.13%	1.671%
49	7.818	2106	2108	2110	rBV2	352	171	0.01%	0.001%
50	8.037	2174	2176	2178	rBV	259	99	0.01%	0.001%
51	8.082	2180	2190	2230	rVV	449641	799134	47.28%	6.016%
52	8.516	2322	2325	2326	rBV2	498	256	0.02%	0.002%
53	8.593	2344	2349	2351	rBV3	386	375	0.02%	0.003%
54	8.757	2397	2400	2404	rBV2	376	232	0.01%	0.002%
55	8.780	2404	2407	2410	rVB3	205	134	0.01%	0.001%
56	8.802	2410	2414	2415	rBV2	538	333	0.02%	0.003%
57	8.844	2415	2427	2455	rBV	795220	1318602	78.02%	9.927%
58	9.101	2505	2507	2510	rBV2	236	115	0.01%	0.001%
59	9.137	2510	2518	2525	rVV5	1161	2028	0.12%	0.015%
60	9.166	2525	2527	2535	rVV4	363	344	0.02%	0.003%
61	9.259	2553	2556	2559	rVB	426	304	0.02%	0.002%
62	9.349	2581	2584	2587	rBV	214	198	0.01%	0.001%
63	9.394	2594	2598	2599	rBV	381	175	0.01%	0.001%
64	9.442	2608	2613	2617	rVB2	199	187	0.01%	0.001%
65	9.468	2617	2621	2623	rBV	312	168	0.01%	0.001%
66	9.497	2627	2630	2634	rBV	277	263	0.02%	0.002%
67	9.535	2638	2642	2645	rBV4	640	597	0.04%	0.004%
68	9.674	2683	2685	2688	rVB	192	88	0.01%	0.001%
69	9.693	2688	2691	2694	rBV2	195	143	0.01%	0.001%
70	9.805	2723	2726	2727	rBV2	174	104	0.01%	0.001%
71	9.818	2727	2730	2735	rVB2	281	264	0.02%	0.002%
72	9.844	2735	2738	2741	rVB2	172	105	0.01%	0.001%
73	9.866	2741	2745	2747	rBV2	225	202	0.01%	0.002%
74	9.957	2771	2773	2776	rVB2	250	121	0.01%	0.001%
75	10.034	2794	2797	2800	rVB	288	177	0.01%	0.001%
76	10.050	2800	2802	2806	rBV3	208	144	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029516.D
 Acq On : 09 Dec 2022 13:13
 Operator : SY/MD
 Sample : N5920-04DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EJ3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.079	2806	2811	2815	rBV3	345	347	0.02%	0.003%
78	10.162	2825	2837	2841	rBV2	29794	43439	2.57%	0.327%
79	10.204	2842	2850	2874	rVB	527252	835726	49.45%	6.292%
80	10.374	2896	2903	2913	rVB3	2146	3592	0.21%	0.027%
81	10.567	2955	2963	2977	rVB	14448	22609	1.34%	0.170%
82	10.632	2980	2983	2986	rVB3	432	280	0.02%	0.002%
83	10.651	2987	2989	2993	rBV	207	119	0.01%	0.001%
84	10.719	3007	3010	3011	rBV	194	126	0.01%	0.001%
85	10.728	3011	3013	3014	rVB	224	102	0.01%	0.001%
86	10.838	3044	3047	3050	rBV2	498	367	0.02%	0.003%
87	10.908	3062	3069	3077	rVB2	1530	2174	0.13%	0.016%
88	10.982	3089	3092	3096	rVB2	301	233	0.01%	0.002%
89	11.005	3096	3099	3102	rBV	259	203	0.01%	0.002%
90	11.092	3123	3126	3129	rVB	273	199	0.01%	0.001%
91	11.108	3129	3131	3136	rBV	208	171	0.01%	0.001%
92	11.175	3146	3152	3159	rBV5	1376	1930	0.11%	0.015%
93	11.236	3159	3171	3197	rBV	853464	1330592	78.73%	10.017%
94	11.551	3267	3269	3272	rBV3	334	182	0.01%	0.001%
95	11.612	3272	3288	3314	rBV	817239	1275238	75.46%	9.600%
96	12.037	3417	3420	3423	rBV	378	340	0.02%	0.003%
97	12.217	3472	3476	3478	rBV2	359	322	0.02%	0.002%
98	12.606	3594	3597	3598	rBV	314	178	0.01%	0.001%
99	12.635	3601	3606	3611	rVV6	1353	1572	0.09%	0.012%
100	13.249	3791	3797	3806	rBV7	2682	3954	0.23%	0.030%




Sum of corrected areas: 13283274

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029516.D
Acq On : 09 Dec 2022 13:13
Operator : SY/MD
Sample : N5920-04DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

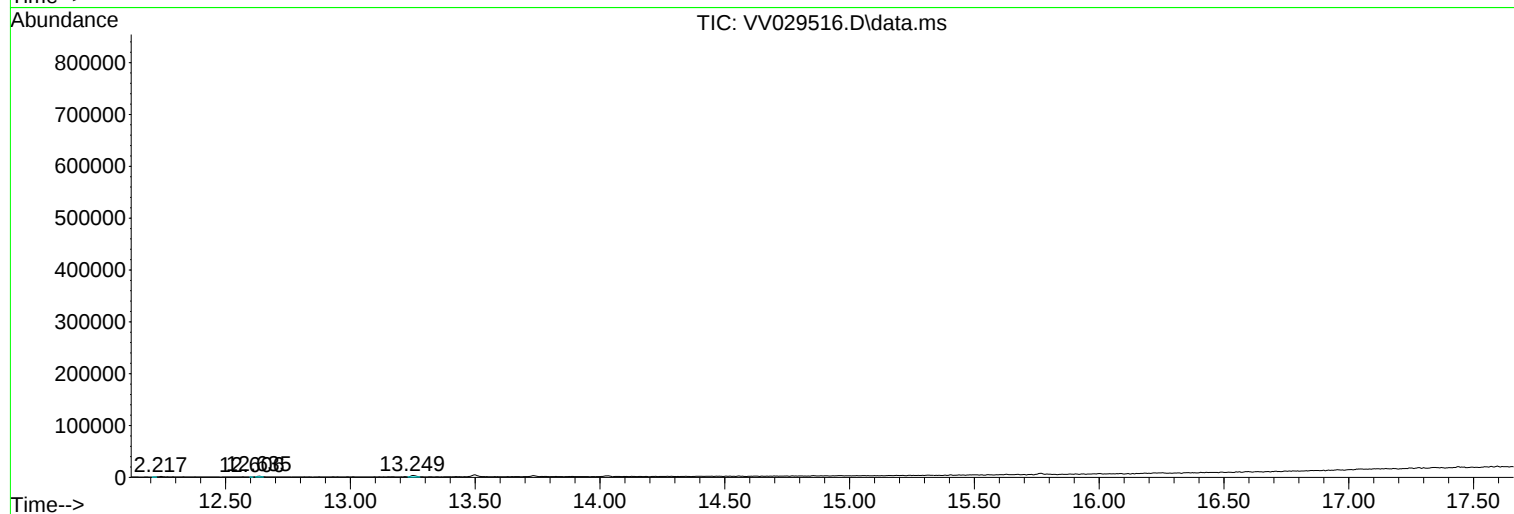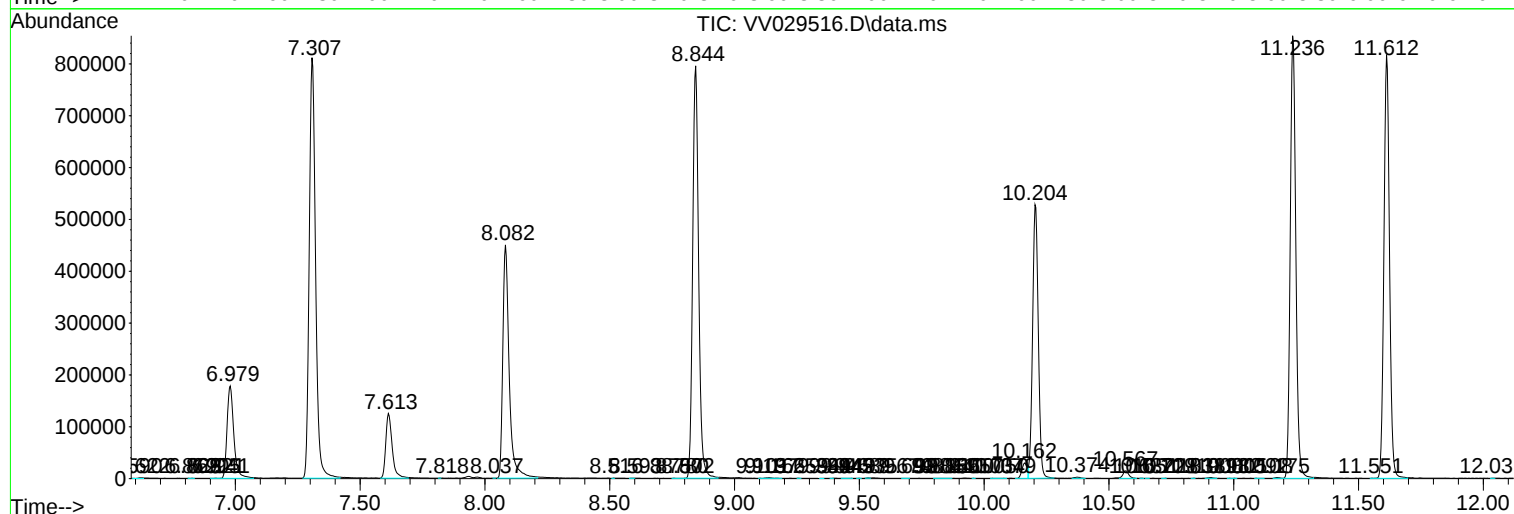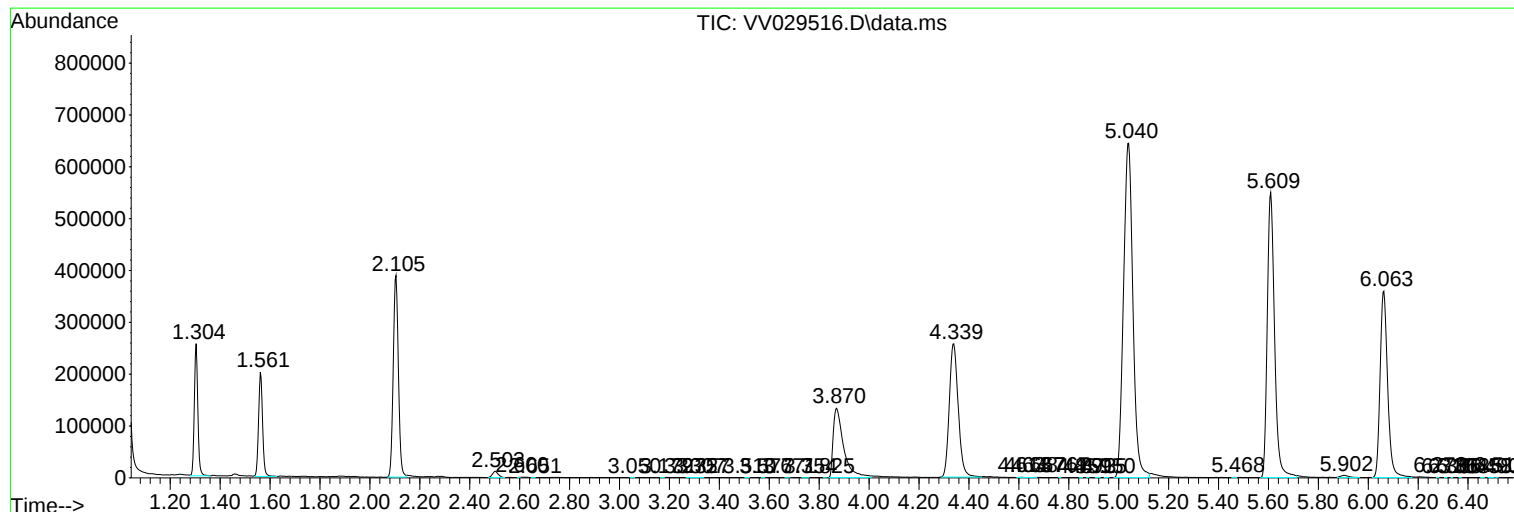

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029516.D
Acq On : 09 Dec 2022 13:13
Operator : SY/MD
Sample : N5920-04DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029516.D
Acq On : 09 Dec 2022 13:13
Operator : SY/MD
Sample : N5920-04DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EJ3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------