

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029518.D
 Acq On : 09 Dec 2022 14:00
 Operator : SY/MD
 Sample : N5920-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	251202	248231	14.31%	1.933%
2	1.564	155	163	176	rVB	204547	225671	13.01%	1.757%
3	2.105	320	331	344	rBV	396637	567781	32.74%	4.421%
4	2.368	412	413	415	rBV2	263	98	0.01%	0.001%
5	2.500	448	454	456	rBV2	1120	1139	0.07%	0.009%
6	2.738	524	528	531	rBV3	224	215	0.01%	0.002%
7	2.921	580	585	589	rBV3	307	326	0.02%	0.003%
8	2.941	589	591	594	rVV2	218	129	0.01%	0.001%
9	2.992	605	607	610	rBV2	218	111	0.01%	0.001%
10	3.034	618	620	623	rBV	196	97	0.01%	0.001%
11	3.095	637	639	643	rVB2	217	115	0.01%	0.001%
12	3.130	648	650	652	rBV2	210	122	0.01%	0.001%
13	3.207	671	674	676	rBV	196	103	0.01%	0.001%
14	3.365	721	723	726	rVB	232	98	0.01%	0.001%
15	3.458	749	752	753	rBV	195	88	0.01%	0.001%
16	3.548	777	780	782	rBV2	143	80	0.00%	0.001%
17	3.664	811	816	818	rBV2	113	94	0.01%	0.001%
18	3.693	822	825	828	rBV	129	90	0.01%	0.001%
19	3.709	828	830	834	rVB2	239	114	0.01%	0.001%
20	3.735	834	838	841	rBV2	316	255	0.01%	0.002%
21	3.773	846	850	855	rVV	242	197	0.01%	0.002%
22	3.870	870	880	918	rBV	123654	342823	19.77%	2.669%
23	4.339	1009	1026	1066	rBV	268143	672936	38.80%	5.240%
24	4.558	1092	1094	1097	rBV3	359	222	0.01%	0.002%
25	4.638	1116	1119	1126	rVB3	428	392	0.02%	0.003%
26	4.783	1160	1164	1166	rVB2	283	159	0.01%	0.001%
27	4.828	1175	1178	1180	rVB	160	82	0.00%	0.001%
28	4.899	1196	1200	1203	rVB	260	159	0.01%	0.001%
29	4.918	1203	1206	1211	rBV	106	103	0.01%	0.001%
30	5.040	1226	1244	1288	rBV2	658406	1734332	100.00%	13.505%
31	5.371	1345	1347	1350	rBV2	333	193	0.01%	0.002%
32	5.461	1373	1375	1378	rVB3	298	110	0.01%	0.001%
33	5.516	1389	1392	1393	rBV2	235	134	0.01%	0.001%
34	5.609	1408	1421	1466	rBV	445427	919938	53.04%	7.163%
35	5.912	1503	1515	1533	rVB9	7719	18146	1.05%	0.141%
36	6.063	1548	1562	1583	rBV	366175	753316	43.44%	5.866%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029518.D
 Acq On : 09 Dec 2022 14:00
 Operator : SY/MD
 Sample : N5920-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.288	1630	1632	1634	rBV	248	157	0.01%	0.001%
38	6.301	1634	1636	1637	rVV	294	111	0.01%	0.001%
39	6.310	1637	1639	1642	rVV	195	141	0.01%	0.001%
40	6.358	1650	1654	1658	rBV3	336	330	0.02%	0.003%
41	6.477	1684	1691	1692	rBV	147	127	0.01%	0.001%
42	6.497	1695	1697	1699	rVB	237	119	0.01%	0.001%
43	6.529	1704	1707	1714	rVB2	236	260	0.01%	0.002%
44	6.590	1721	1726	1729	rBV2	289	217	0.01%	0.002%
45	6.629	1729	1738	1746	rBV5	1193	2440	0.14%	0.019%
46	6.703	1759	1761	1764	rBV2	207	141	0.01%	0.001%
47	6.809	1789	1794	1795	rBV2	385	241	0.01%	0.002%
48	6.886	1815	1818	1820	rBV	209	175	0.01%	0.001%
49	6.979	1836	1847	1877	rBV	180100	333051	19.20%	2.593%
50	7.236	1922	1927	1932	rVB4	669	681	0.04%	0.005%
51	7.307	1937	1949	1987	rBV	820095	1444057	83.26%	11.245%
52	7.612	2034	2044	2070	rBV	128214	227203	13.10%	1.769%
53	8.021	2168	2171	2176	rVB4	343	192	0.01%	0.001%
54	8.082	2180	2190	2228	rBV	455587	817892	47.16%	6.369%
55	8.561	2337	2339	2343	rVB2	276	155	0.01%	0.001%
56	8.728	2386	2391	2393	rBV2	409	353	0.02%	0.003%
57	8.844	2414	2427	2452	rBV	658219	1083753	62.49%	8.439%
58	8.998	2471	2475	2478	rBV3	817	844	0.05%	0.007%
59	9.120	2510	2513	2514	rBV2	446	214	0.01%	0.002%
60	9.201	2536	2538	2540	rVB2	252	101	0.01%	0.001%
61	9.226	2544	2546	2548	rBV2	156	112	0.01%	0.001%
62	9.281	2560	2563	2566	rVB2	319	206	0.01%	0.002%
63	9.345	2581	2583	2585	rVB	257	90	0.01%	0.001%
64	9.358	2585	2587	2589	rBV	304	157	0.01%	0.001%
65	9.506	2630	2633	2636	rVB	179	116	0.01%	0.001%
66	9.542	2636	2644	2645	rBV5	715	828	0.05%	0.006%
67	9.641	2672	2675	2679	rBV	295	228	0.01%	0.002%
68	9.661	2679	2681	2684	rBV	269	192	0.01%	0.001%
69	9.805	2723	2726	2728	rBV	185	89	0.01%	0.001%
70	9.837	2734	2736	2741	rVV	259	229	0.01%	0.002%
71	9.876	2745	2748	2750	rBV	150	89	0.01%	0.001%
72	9.918	2758	2761	2763	rBV	613	417	0.02%	0.003%
73	9.960	2773	2774	2779	rBV2	278	172	0.01%	0.001%
74	10.066	2804	2807	2812	rBV3	296	234	0.01%	0.002%
75	10.101	2815	2818	2820	rBV	178	134	0.01%	0.001%
76	10.127	2822	2826	2827	rBV	233	172	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029518.D
 Acq On : 09 Dec 2022 14:00
 Operator : SY/MD
 Sample : N5920-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.162	2828	2837	2841	rVV2	28847	41526	2.39%	0.323%
78	10.207	2842	2851	2874	rVB	536459	851424	49.09%	6.630%
79	10.374	2895	2903	2916	rVB2	5485	9189	0.53%	0.072%
80	10.435	2916	2922	2925	rBV4	367	437	0.03%	0.003%
81	10.525	2946	2950	2952	rBV3	708	532	0.03%	0.004%
82	10.567	2955	2963	2978	rVB	13948	22846	1.32%	0.178%
83	10.648	2983	2988	2989	rBV	255	208	0.01%	0.002%
84	10.702	3002	3005	3006	rBV	322	176	0.01%	0.001%
85	10.744	3016	3018	3023	rVB2	324	219	0.01%	0.002%
86	10.834	3044	3046	3049	rBV	422	317	0.02%	0.002%
87	10.879	3057	3060	3062	rBV2	175	130	0.01%	0.001%
88	10.911	3062	3070	3074	rBV3	1416	2076	0.12%	0.016%
89	11.005	3096	3099	3102	rBV2	242	162	0.01%	0.001%
90	11.175	3147	3152	3159	rVB3	1433	2073	0.12%	0.016%
91	11.236	3159	3171	3197	rBV	731651	1137858	65.61%	8.860%
92	11.426	3227	3230	3232	rBV2	375	274	0.02%	0.002%
93	11.474	3243	3245	3249	rBV3	303	154	0.01%	0.001%
94	11.509	3254	3256	3259	rBV2	259	147	0.01%	0.001%
95	11.554	3265	3270	3276	rBV4	1557	2083	0.12%	0.016%
96	11.612	3276	3288	3324	rVV	853531	1360617	78.45%	10.595%
97	12.297	3499	3501	3504	rBV3	328	197	0.01%	0.002%
98	12.635	3600	3606	3614	rVB6	1066	1535	0.09%	0.012%
99	12.670	3614	3617	3618	rBV	293	136	0.01%	0.001%
100	13.255	3786	3799	3807	rBV8	1767	3373	0.19%	0.026%




Sum of corrected areas: 12842308

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029518.D
Acq On : 09 Dec 2022 14:00
Operator : SY/MD
Sample : N5920-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

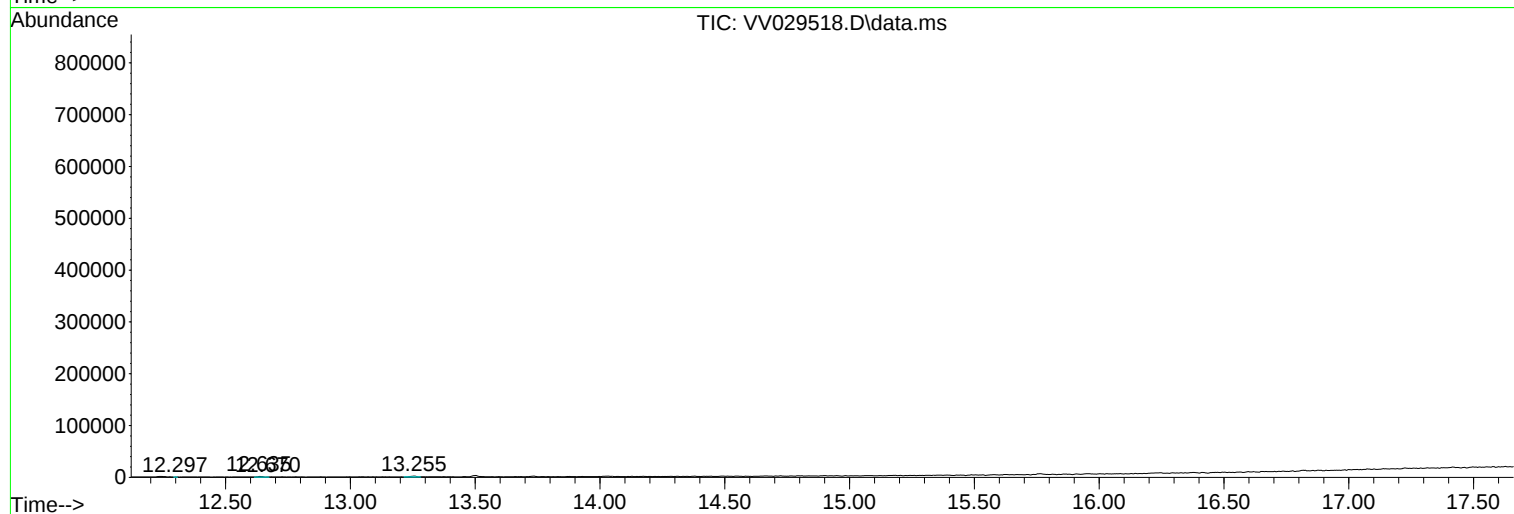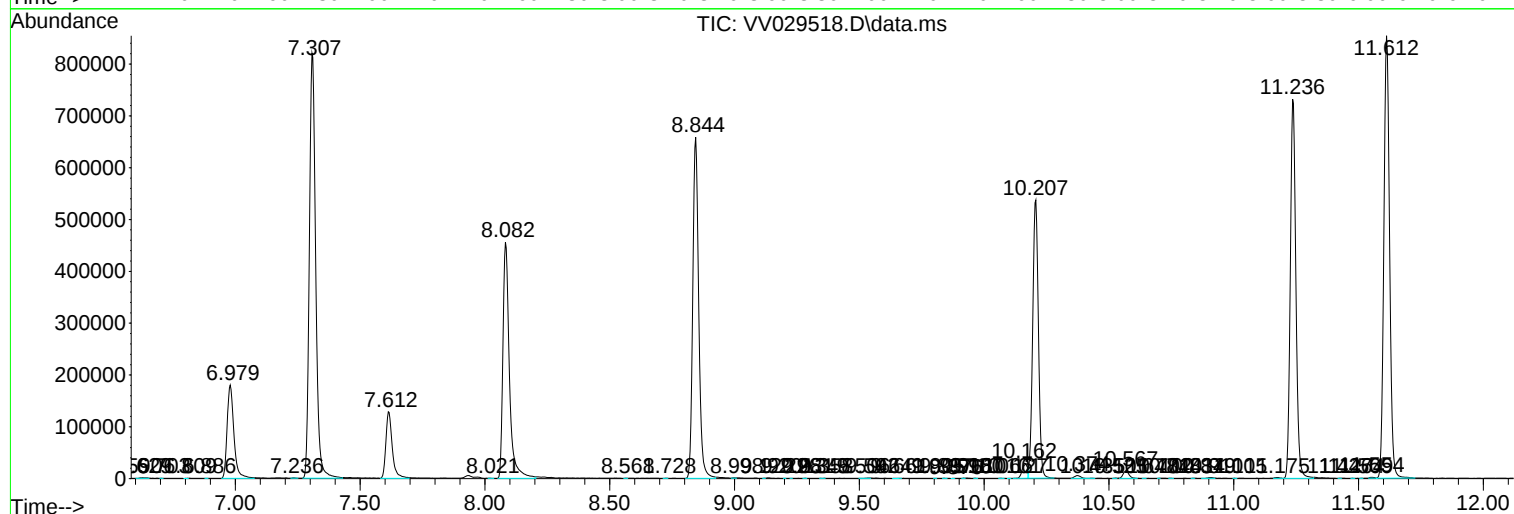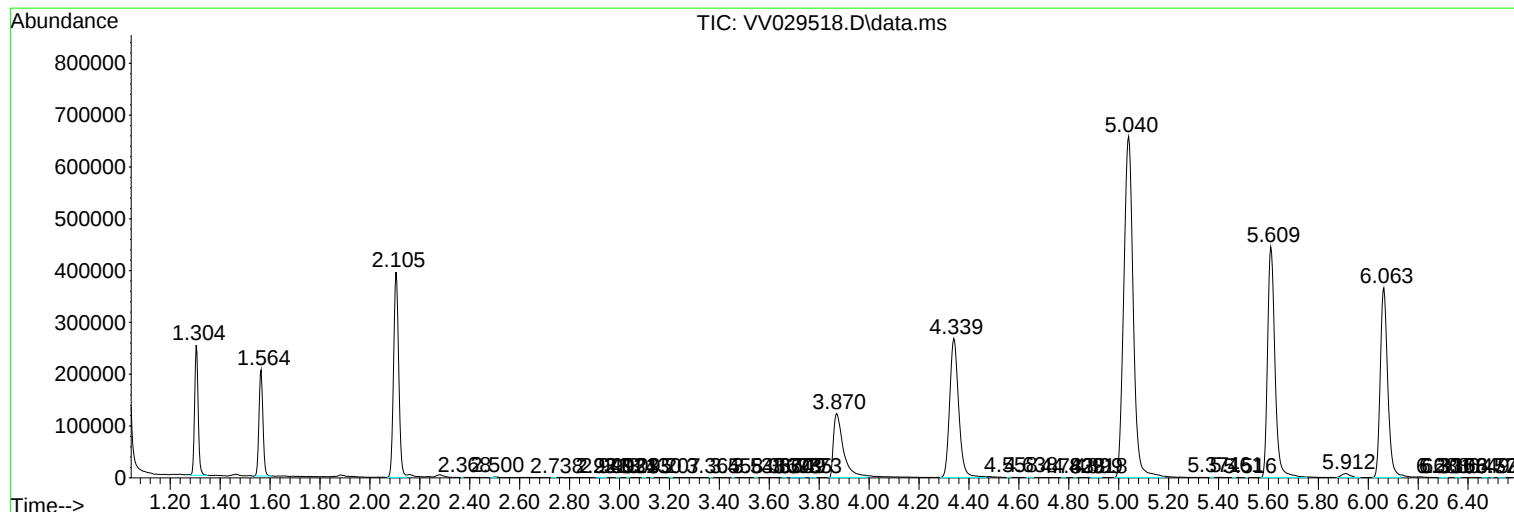

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029518.D
Acq On : 09 Dec 2022 14:00
Operator : SY/MD
Sample : N5920-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029518.D
Acq On : 09 Dec 2022 14:00
Operator : SY/MD
Sample : N5920-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc