

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029519.D
 Acq On : 09 Dec 2022 14:23
 Operator : SY/MD
 Sample : N5920-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	241446	242037	15.35%	1.946%
2	1.564	155	163	179	rVB	187425	210272	13.33%	1.690%
3	2.105	320	331	344	rBV	361473	524586	33.26%	4.217%
4	2.407	422	425	427	rBV	276	165	0.01%	0.001%
5	2.503	447	455	462	rVB3	1212	1820	0.12%	0.015%
6	2.696	512	515	519	rVB	206	153	0.01%	0.001%
7	2.728	522	525	528	rBV2	228	145	0.01%	0.001%
8	2.760	532	535	536	rBV2	334	203	0.01%	0.002%
9	2.815	547	552	557	rBV3	355	315	0.02%	0.003%
10	2.960	594	597	601	rBV	226	177	0.01%	0.001%
11	2.995	606	608	611	rBV	195	120	0.01%	0.001%
12	3.085	632	636	638	rBV3	335	198	0.01%	0.002%
13	3.178	662	665	667	rBV	143	104	0.01%	0.001%
14	3.227	677	680	686	rBV	178	231	0.01%	0.002%
15	3.275	692	695	698	rBV	141	88	0.01%	0.001%
16	3.609	795	799	800	rBV	149	107	0.01%	0.001%
17	3.706	826	829	832	rBV2	211	152	0.01%	0.001%
18	3.805	855	860	863	rBV2	152	166	0.01%	0.001%
19	3.866	869	879	909	rBV	114364	304641	19.32%	2.449%
20	4.339	1010	1026	1059	rBV	239870	605017	38.36%	4.864%
21	4.632	1116	1117	1120	rBV2	373	225	0.01%	0.002%
22	4.725	1144	1146	1147	rBV	220	92	0.01%	0.001%
23	4.757	1154	1156	1158	rBV	139	101	0.01%	0.001%
24	4.789	1161	1166	1172	rVB3	270	310	0.02%	0.002%
25	4.825	1172	1177	1182	rBV	341	306	0.02%	0.002%
26	5.040	1226	1244	1295	rBV2	596675	1577199	100.00%	12.679%
27	5.529	1391	1396	1398	rBV3	175	165	0.01%	0.001%
28	5.542	1398	1400	1406	rVB2	466	274	0.02%	0.002%
29	5.609	1407	1421	1451	rBV	522386	1060045	67.21%	8.521%
30	5.911	1503	1515	1536	rBV5	24829	56009	3.55%	0.450%
31	6.063	1548	1562	1598	rBV	326771	685227	43.45%	5.508%
32	6.272	1625	1627	1629	rVB	289	110	0.01%	0.001%
33	6.284	1629	1631	1633	rVB	280	113	0.01%	0.001%
34	6.458	1683	1685	1689	rVB	312	174	0.01%	0.001%
35	6.490	1693	1695	1698	rVB	231	85	0.01%	0.001%
36	6.532	1706	1708	1711	rVB	197	130	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029519.D
 Acq On : 09 Dec 2022 14:23
 Operator : SY/MD
 Sample : N5920-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.567	1716	1719	1722	rBV2	231	149	0.01%	0.001%
38	6.599	1726	1729	1730	rBV2	232	119	0.01%	0.001%
39	6.638	1730	1741	1744	rBV4	1180	1849	0.12%	0.015%
40	6.690	1755	1757	1759	rBV	301	173	0.01%	0.001%
41	6.731	1768	1770	1777	rVB2	304	278	0.02%	0.002%
42	6.760	1777	1779	1781	rBV	302	135	0.01%	0.001%
43	6.773	1781	1783	1784	rBV	280	125	0.01%	0.001%
44	6.937	1832	1834	1836	rBV2	186	93	0.01%	0.001%
45	6.979	1836	1847	1878	rBV	161998	300042	19.02%	2.412%
46	7.307	1936	1949	1982	rBV	744036	1315673	83.42%	10.576%
47	7.612	2034	2044	2066	rBV	111281	199040	12.62%	1.600%
48	8.082	2180	2190	2226	rBV	408184	727002	46.09%	5.844%
49	8.609	2351	2354	2355	rBV2	352	212	0.01%	0.002%
50	8.670	2369	2373	2375	rBV3	201	154	0.01%	0.001%
51	8.709	2383	2385	2387	rBV	270	113	0.01%	0.001%
52	8.747	2395	2397	2401	rBV2	345	222	0.01%	0.002%
53	8.844	2415	2427	2472	rBV	767240	1257474	79.73%	10.108%
54	9.117	2505	2512	2513	rBV4	540	569	0.04%	0.005%
55	9.217	2538	2543	2544	rBV2	156	139	0.01%	0.001%
56	9.226	2544	2546	2549	rVV	246	127	0.01%	0.001%
57	9.246	2549	2552	2555	rVB2	270	179	0.01%	0.001%
58	9.265	2555	2558	2559	rBV	199	98	0.01%	0.001%
59	9.284	2562	2564	2566	rBV	340	142	0.01%	0.001%
60	9.300	2566	2569	2576	rVV3	177	194	0.01%	0.002%
61	9.387	2593	2596	2599	rVB	183	94	0.01%	0.001%
62	9.426	2603	2608	2612	rBV2	285	300	0.02%	0.002%
63	9.442	2612	2613	2617	rBV	237	144	0.01%	0.001%
64	9.535	2637	2642	2645	rBV2	809	923	0.06%	0.007%
65	9.609	2662	2665	2667	rBV2	215	133	0.01%	0.001%
66	9.638	2670	2674	2679	rVB3	369	331	0.02%	0.003%
67	9.664	2679	2682	2686	rVB3	235	141	0.01%	0.001%
68	9.702	2686	2694	2695	rBV3	347	383	0.02%	0.003%
69	9.741	2703	2706	2709	rVB3	230	165	0.01%	0.001%
70	9.760	2709	2712	2716	rVB2	256	217	0.01%	0.002%
71	9.786	2716	2720	2724	rBV2	180	155	0.01%	0.001%
72	9.860	2739	2743	2746	rBV2	309	242	0.02%	0.002%
73	9.918	2757	2761	2763	rBV2	394	305	0.02%	0.002%
74	9.972	2775	2778	2780	rBV3	238	135	0.01%	0.001%
75	10.021	2791	2793	2796	rVB2	178	112	0.01%	0.001%
76	10.120	2820	2824	2825	rBV2	148	91	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029519.D
 Acq On : 09 Dec 2022 14:23
 Operator : SY/MD
 Sample : N5920-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.162	2826	2837	2841	rBV2	27963	41037	2.60%	0.330%
78	10.207	2842	2851	2872	rVB	481940	766252	48.58%	6.160%
79	10.374	2892	2903	2916	rVB4	5015	8802	0.56%	0.071%
80	10.439	2917	2923	2927	rVB3	413	477	0.03%	0.004%
81	10.461	2927	2930	2932	rBV	410	217	0.01%	0.002%
82	10.506	2941	2944	2945	rBV2	315	181	0.01%	0.001%
83	10.522	2945	2949	2953	rVV4	712	747	0.05%	0.006%
84	10.567	2954	2963	2974	rVB2	12989	20975	1.33%	0.169%
85	10.651	2986	2989	2990	rBV2	168	90	0.01%	0.001%
86	10.786	3028	3031	3034	rBV	388	316	0.02%	0.003%
87	10.828	3041	3044	3046	rBV2	242	165	0.01%	0.001%
88	10.844	3046	3049	3055	rVV3	402	387	0.02%	0.003%
89	10.908	3064	3069	3078	rVB4	1234	1582	0.10%	0.013%
90	11.123	3134	3136	3139	rBV	207	97	0.01%	0.001%
91	11.178	3145	3153	3158	rBV4	1243	1766	0.11%	0.014%
92	11.236	3158	3171	3195	rBV	844783	1305377	82.77%	10.494%
93	11.394	3218	3220	3222	rBV	354	193	0.01%	0.002%
94	11.612	3276	3288	3318	rVB	769426	1207898	76.59%	9.710%
95	11.860	3363	3365	3373	rVB4	498	384	0.02%	0.003%
96	11.918	3380	3383	3388	rBV3	451	348	0.02%	0.003%
97	12.011	3409	3412	3416	rVB3	353	260	0.02%	0.002%
98	12.570	3584	3586	3587	rBV	340	155	0.01%	0.001%
99	12.635	3604	3606	3613	rVB4	1231	964	0.06%	0.008%
100	13.255	3793	3799	3805	rVB7	1379	1734	0.11%	0.014%




Sum of corrected areas: 12439838

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029519.D
Acq On : 09 Dec 2022 14:23
Operator : SY/MD
Sample : N5920-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

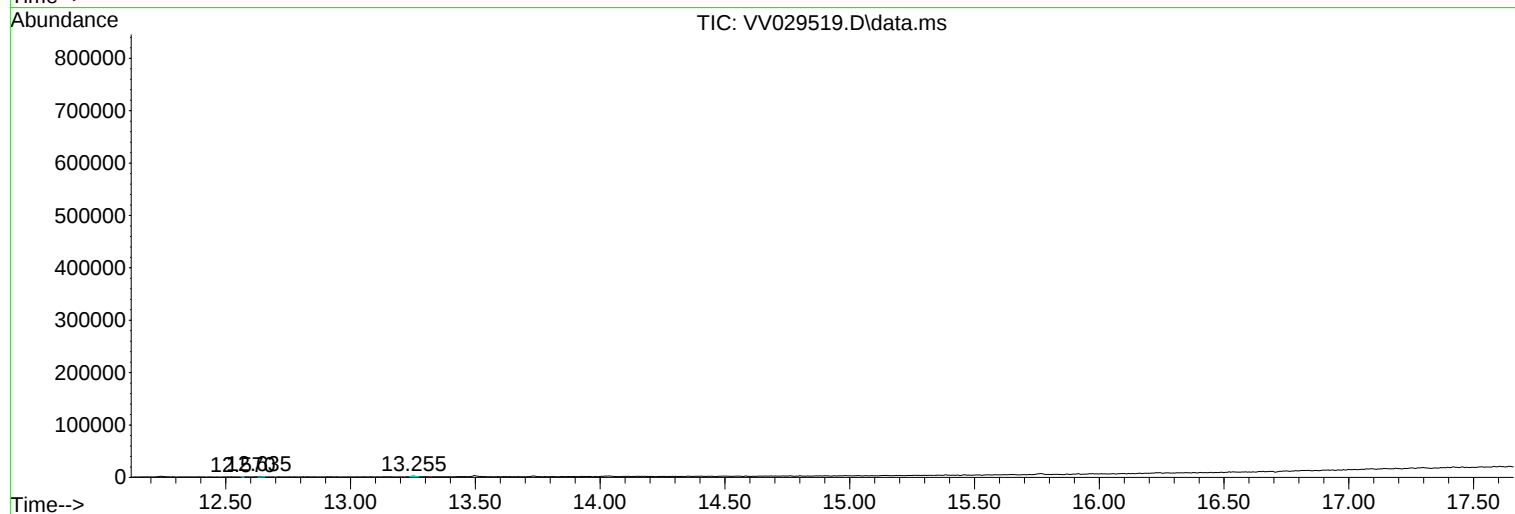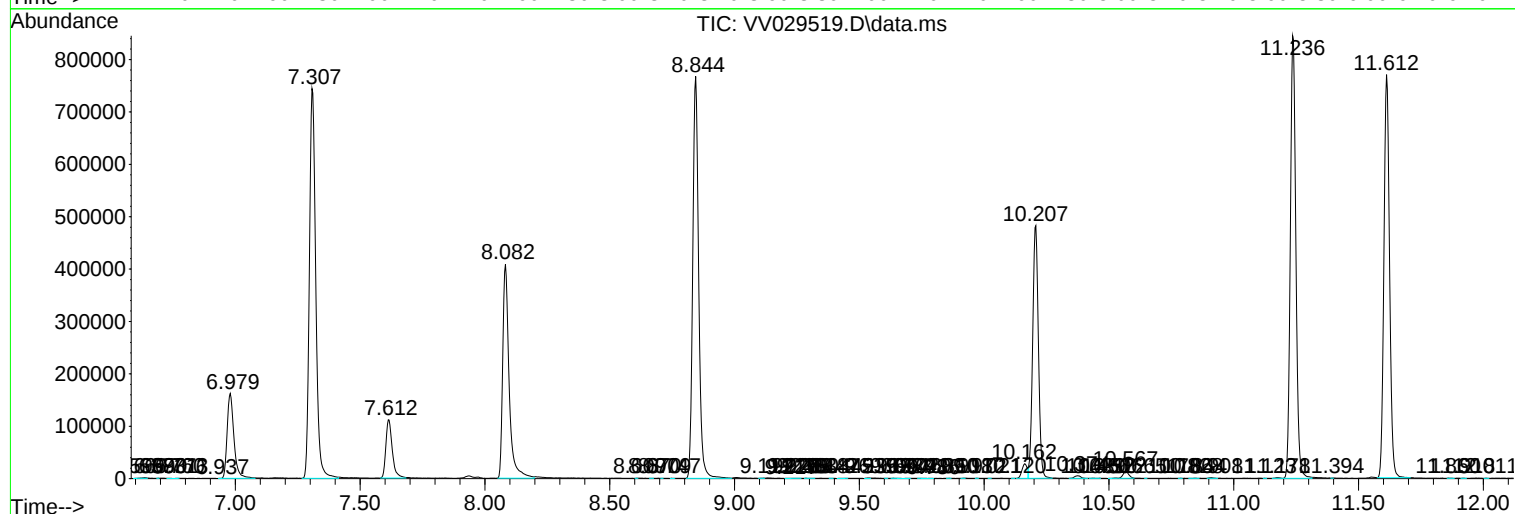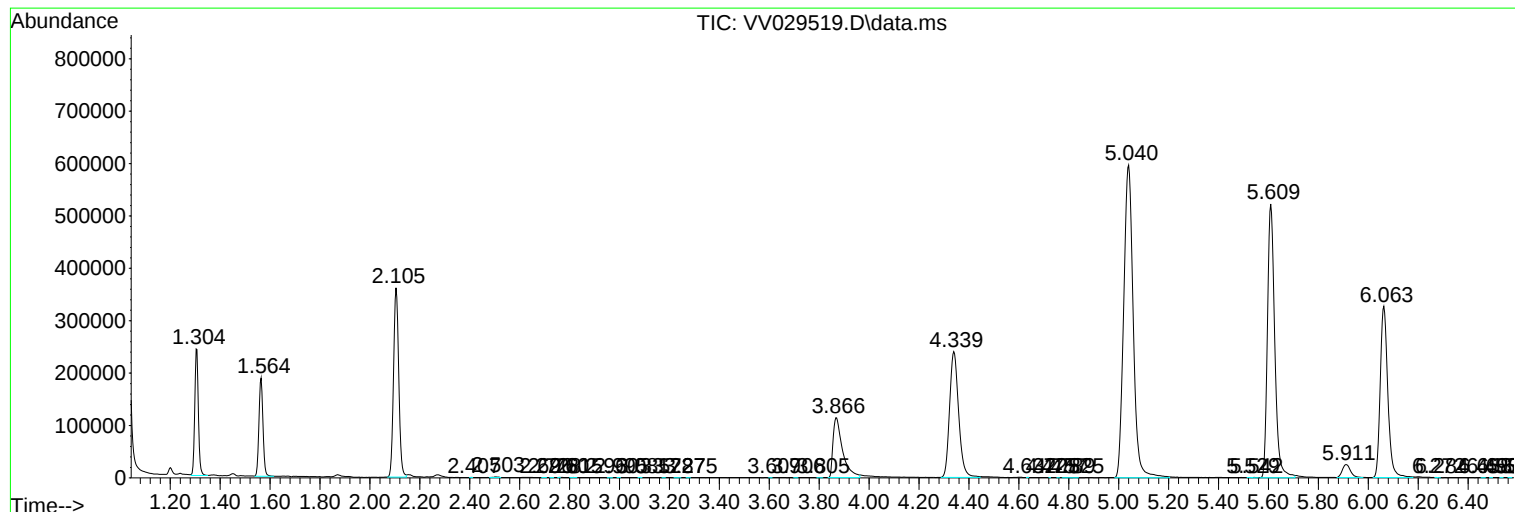

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029519.D
Acq On : 09 Dec 2022 14:23
Operator : SY/MD
Sample : N5920-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029519.D
Acq On : 09 Dec 2022 14:23
Operator : SY/MD
Sample : N5920-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------