

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029520.D
 Acq On : 09 Dec 2022 14:47
 Operator : SY/MD
 Sample : N5920-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	248135	246889	14.38%	1.843%
2	1.564	156	163	175	rVB	203617	225933	13.16%	1.686%
3	2.105	321	331	346	rBV	390632	564798	32.90%	4.215%
4	2.503	449	455	462	rVB2	1137	1647	0.10%	0.012%
5	2.629	488	494	504	rVB4	1280	1992	0.12%	0.015%
6	2.699	514	516	522	rVB3	204	163	0.01%	0.001%
7	2.732	523	526	529	rBV	263	212	0.01%	0.002%
8	2.902	576	579	582	rBV2	194	176	0.01%	0.001%
9	2.941	588	591	594	rBV3	248	163	0.01%	0.001%
10	3.031	616	619	623	rBV3	305	221	0.01%	0.002%
11	3.092	634	638	639	rBV	261	180	0.01%	0.001%
12	3.172	661	663	665	rBV	171	96	0.01%	0.001%
13	3.201	670	672	676	rVB	264	147	0.01%	0.001%
14	3.230	676	681	684	rBV2	174	171	0.01%	0.001%
15	3.314	705	707	710	rVV	169	87	0.01%	0.001%
16	3.375	722	726	728	rBV2	160	102	0.01%	0.001%
17	3.404	733	735	739	rVB	359	164	0.01%	0.001%
18	3.426	739	742	744	rBV2	179	131	0.01%	0.001%
19	3.462	748	753	757	rVV3	219	228	0.01%	0.002%
20	3.548	777	780	783	rBV	175	126	0.01%	0.001%
21	3.590	790	793	796	rBV	173	150	0.01%	0.001%
22	3.642	804	809	815	rVB2	168	208	0.01%	0.002%
23	3.680	815	821	823	rBV	258	202	0.01%	0.002%
24	3.719	830	833	837	rVB2	159	104	0.01%	0.001%
25	3.748	839	842	845	rVB	184	118	0.01%	0.001%
26	3.870	867	880	920	rBV	121856	336222	19.59%	2.509%
27	4.339	1008	1026	1058	rBV	264469	671882	39.14%	5.015%
28	4.728	1144	1147	1150	rVV2	304	218	0.01%	0.002%
29	4.793	1165	1167	1172	rVB	194	92	0.01%	0.001%
30	4.828	1176	1178	1181	rBV	229	157	0.01%	0.001%
31	4.863	1185	1189	1190	rBV	213	119	0.01%	0.001%
32	4.902	1198	1201	1203	rBV	207	119	0.01%	0.001%
33	4.918	1203	1206	1212	rBV2	201	190	0.01%	0.001%
34	5.040	1226	1244	1274	rBV2	654385	1716698	100.00%	12.812%
35	5.394	1351	1354	1357	rBV2	432	385	0.02%	0.003%
36	5.429	1363	1365	1367	rBV2	214	112	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029520.D
 Acq On : 09 Dec 2022 14:47
 Operator : SY/MD
 Sample : N5920-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COEN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.609	1407	1421	1465	rVV	542892	1103942	64.31%	8.239%
38	5.912	1503	1515	1530	rBV7	6301	14263	0.83%	0.106%
39	6.002	1539	1543	1545	rBV3	185	164	0.01%	0.001%
40	6.063	1548	1562	1599	rBV	364376	755735	44.02%	5.640%
41	6.342	1647	1649	1652	rVB	235	126	0.01%	0.001%
42	6.362	1652	1655	1661	rBV2	234	210	0.01%	0.002%
43	6.391	1661	1664	1668	rBV3	253	206	0.01%	0.002%
44	6.445	1679	1681	1686	rVB2	401	264	0.02%	0.002%
45	6.513	1697	1702	1706	rVB3	366	346	0.02%	0.003%
46	6.548	1711	1713	1719	rVV2	251	141	0.01%	0.001%
47	6.590	1724	1726	1729	rBV2	337	160	0.01%	0.001%
48	6.629	1730	1738	1739	rBV2	1123	1304	0.08%	0.010%
49	6.767	1779	1781	1785	rVB	182	135	0.01%	0.001%
50	6.879	1814	1816	1819	rVB2	199	107	0.01%	0.001%
51	6.899	1819	1822	1827	rBV3	258	233	0.01%	0.002%
52	6.979	1836	1847	1879	rBV	181215	334510	19.49%	2.497%
53	7.239	1926	1928	1932	rBV2	478	237	0.01%	0.002%
54	7.307	1937	1949	1984	rBV	799122	1435892	83.64%	10.717%
55	7.612	2034	2044	2065	rBV	126064	222833	12.98%	1.663%
56	7.802	2101	2103	2107	rBV2	384	273	0.02%	0.002%
57	8.082	2180	2190	2225	rBV	458340	811846	47.29%	6.059%
58	8.548	2333	2335	2338	rBV3	348	176	0.01%	0.001%
59	8.641	2361	2364	2368	rVB2	367	300	0.02%	0.002%
60	8.796	2409	2412	2414	rBV	254	174	0.01%	0.001%
61	8.844	2414	2427	2456	rBV	793368	1305266	76.03%	9.742%
62	9.095	2502	2505	2507	rBV	277	162	0.01%	0.001%
63	9.127	2511	2515	2517	rBV4	855	659	0.04%	0.005%
64	9.188	2530	2534	2539	rVB2	344	239	0.01%	0.002%
65	9.227	2541	2546	2548	rBV2	288	256	0.01%	0.002%
66	9.249	2548	2553	2555	rBV2	309	278	0.02%	0.002%
67	9.281	2560	2563	2566	rVB2	273	205	0.01%	0.002%
68	9.301	2566	2569	2571	rVB2	211	113	0.01%	0.001%
69	9.320	2571	2575	2580	rBV2	266	333	0.02%	0.002%
70	9.419	2604	2606	2609	rVB2	375	197	0.01%	0.001%
71	9.452	2612	2616	2618	rVB2	325	259	0.02%	0.002%
72	9.538	2636	2643	2644	rBV4	642	607	0.04%	0.005%
73	9.738	2703	2705	2709	rVB2	249	187	0.01%	0.001%
74	9.773	2709	2716	2719	rBV3	267	322	0.02%	0.002%
75	9.792	2719	2722	2729	rVB2	356	292	0.02%	0.002%
76	9.915	2756	2760	2762	rBV2	478	343	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029520.D
 Acq On : 09 Dec 2022 14:47
 Operator : SY/MD
 Sample : N5920-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.969	2774	2777	2779	rBV2	282	177	0.01%	0.001%
78	10.075	2807	2810	2812	rBV	207	148	0.01%	0.001%
79	10.162	2827	2837	2841	rBV2	28320	40999	2.39%	0.306%
80	10.204	2842	2850	2878	rVB	543483	852075	49.63%	6.359%
81	10.342	2891	2893	2895	rBV	351	227	0.01%	0.002%
82	10.374	2895	2903	2914	rVB3	6527	10920	0.64%	0.082%
83	10.419	2914	2917	2920	rBV	347	263	0.02%	0.002%
84	10.436	2920	2922	2929	rVB3	439	451	0.03%	0.003%
85	10.464	2929	2931	2933	rBV	304	149	0.01%	0.001%
86	10.481	2933	2936	2944	rVB4	465	443	0.03%	0.003%
87	10.529	2945	2951	2954	rBV4	973	1055	0.06%	0.008%
88	10.567	2955	2963	2975	rVB2	13275	20924	1.22%	0.156%
89	10.690	2997	3001	3003	rBV3	208	151	0.01%	0.001%
90	10.706	3003	3006	3008	rBV2	334	195	0.01%	0.001%
91	10.738	3014	3016	3019	rBV2	356	214	0.01%	0.002%
92	10.754	3019	3021	3024	rVB2	303	96	0.01%	0.001%
93	10.905	3063	3068	3076	rBV5	1161	1605	0.09%	0.012%
94	11.053	3110	3114	3116	rBV2	154	110	0.01%	0.001%
95	11.104	3127	3130	3132	rBV2	271	182	0.01%	0.001%
96	11.153	3142	3145	3146	rBV	312	168	0.01%	0.001%
97	11.172	3147	3151	3152	rBV2	1054	649	0.04%	0.005%
98	11.239	3159	3172	3195	rBV	868986	1361967	79.34%	10.165%
99	11.554	3262	3270	3276	rBV5	2072	3740	0.22%	0.028%
100	11.612	3276	3288	3314	rVV	848391	1337816	77.93%	9.985%




Sum of corrected areas: 13398621

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029520.D
Acq On : 09 Dec 2022 14:47
Operator : SY/MD
Sample : N5920-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

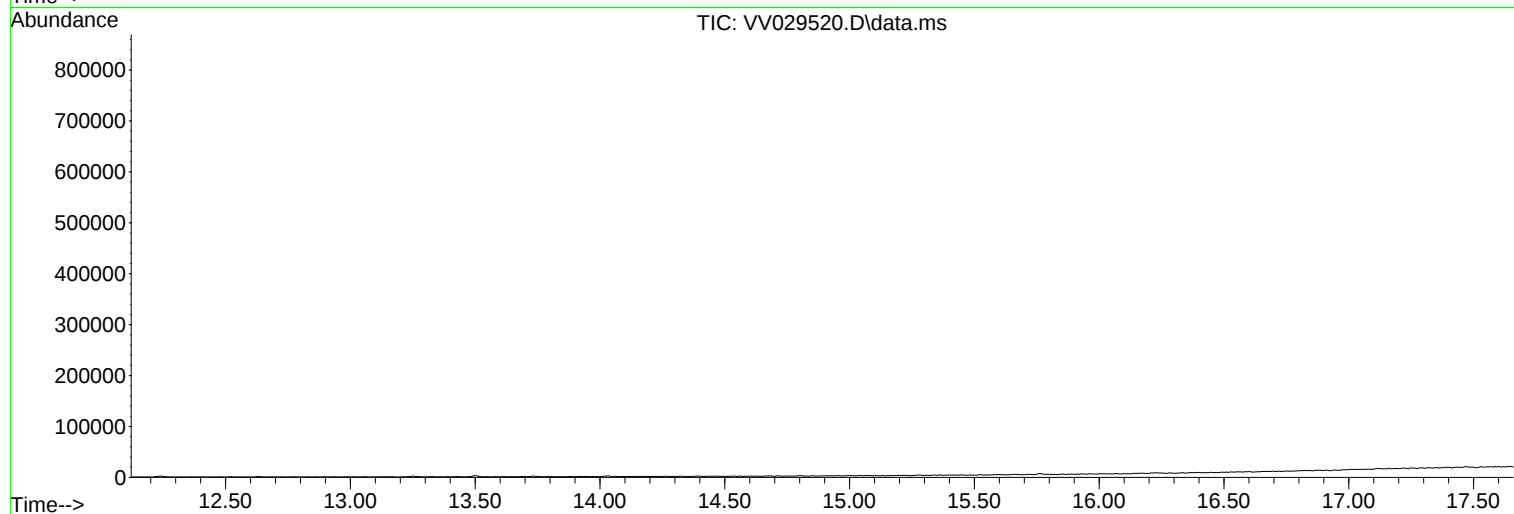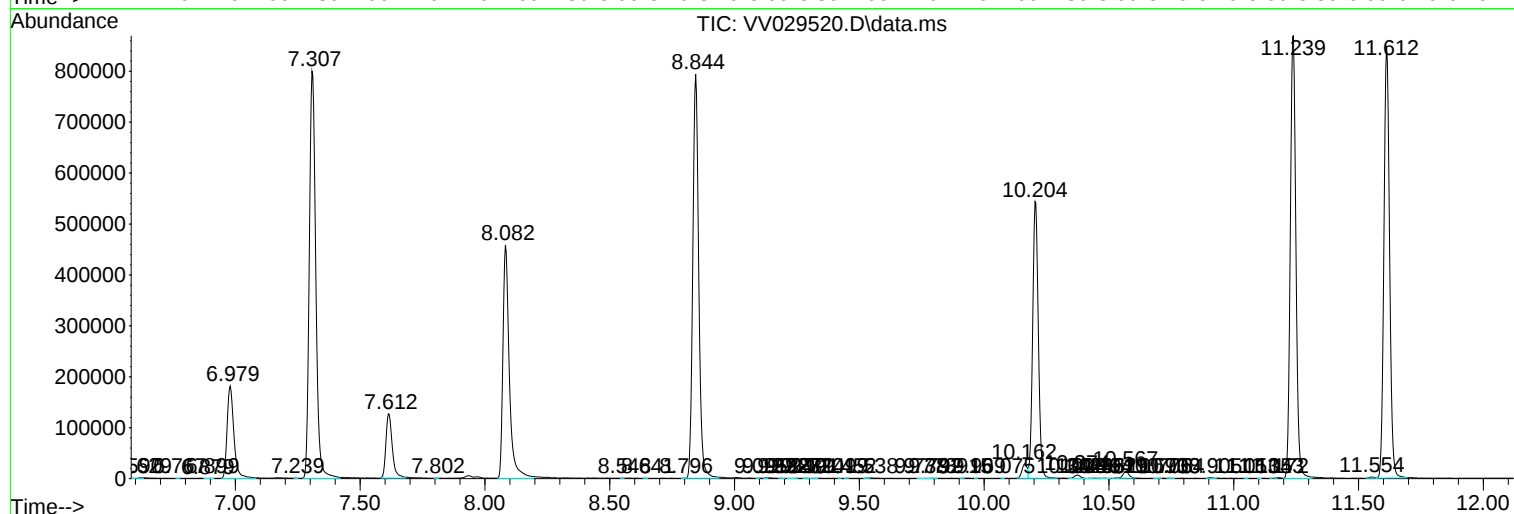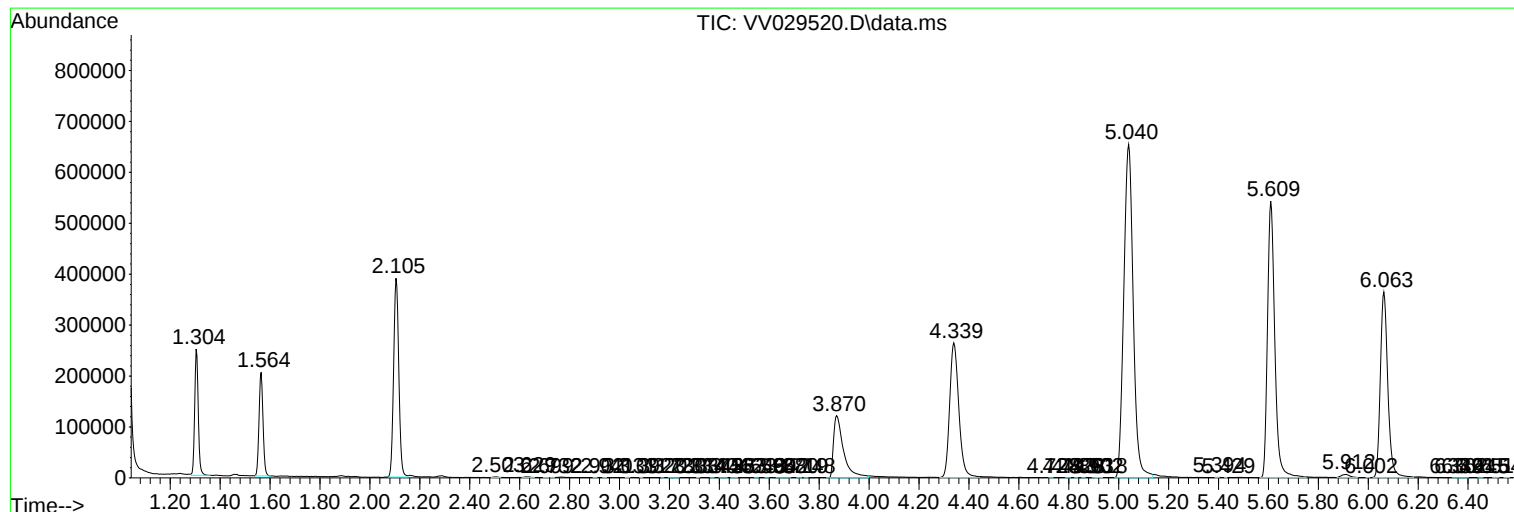

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029520.D
Acq On : 09 Dec 2022 14:47
Operator : SY/MD
Sample : N5920-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029520.D
Acq On : 09 Dec 2022 14:47
Operator : SY/MD
Sample : N5920-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc