

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
 Data File : VV029521.D
 Acq On : 09 Dec 2022 15:10
 Operator : SY/MD
 Sample : N5920-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	209525	207034	14.46%	1.877%
2	1.564	155	163	180	rVB	169172	191735	13.40%	1.738%
3	2.105	320	331	344	rBV	328040	468920	32.76%	4.250%
4	2.507	448	456	460	rBV3	1003	1200	0.08%	0.011%
5	2.542	465	467	468	rBV3	189	90	0.01%	0.001%
6	2.613	487	489	493	rBV2	326	206	0.01%	0.002%
7	2.754	527	533	537	rBV5	886	1106	0.08%	0.010%
8	2.825	551	555	559	rVB3	246	196	0.01%	0.002%
9	2.870	565	569	572	rBV	141	122	0.01%	0.001%
10	2.889	573	575	578	rVV	213	105	0.01%	0.001%
11	3.050	623	625	626	rBV	236	97	0.01%	0.001%
12	3.204	670	673	680	rVB2	159	164	0.01%	0.001%
13	3.275	693	695	698	rVB	177	75	0.01%	0.001%
14	3.320	706	709	715	rVB2	185	133	0.01%	0.001%
15	3.381	725	728	729	rBV	187	85	0.01%	0.001%
16	3.433	741	744	748	rVB	154	95	0.01%	0.001%
17	3.455	748	751	752	rBV	135	77	0.01%	0.001%
18	3.542	776	778	779	rBV	161	75	0.01%	0.001%
19	3.580	785	790	793	rBV2	271	183	0.01%	0.002%
20	3.642	808	809	813	rVB2	199	84	0.01%	0.001%
21	3.664	813	816	818	rBV	130	83	0.01%	0.001%
22	3.799	855	858	862	rVB2	125	76	0.01%	0.001%
23	3.835	866	869	871	rBV	149	94	0.01%	0.001%
24	3.873	871	881	915	rBV	99261	275217	19.23%	2.495%
25	4.339	1010	1026	1065	rBV	217185	556136	38.85%	5.041%
26	4.603	1104	1108	1113	rVB3	253	203	0.01%	0.002%
27	4.661	1122	1126	1127	rBV2	377	288	0.02%	0.003%
28	4.728	1143	1147	1157	rVB2	202	372	0.03%	0.003%
29	4.773	1157	1161	1163	rBV2	191	124	0.01%	0.001%
30	4.844	1179	1183	1187	rBV2	217	228	0.02%	0.002%
31	4.879	1191	1194	1196	rBV2	244	124	0.01%	0.001%
32	4.934	1208	1211	1213	rVB2	202	110	0.01%	0.001%
33	5.040	1226	1244	1283	rBV2	541543	1431332	100.00%	12.974%
34	5.391	1350	1353	1359	rBV4	441	428	0.03%	0.004%
35	5.416	1359	1361	1365	rVB2	430	186	0.01%	0.002%
36	5.436	1365	1367	1370	rVB2	281	145	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029521.D
 Acq On : 09 Dec 2022 15:10
 Operator : SY/MD
 Sample : N5920-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.455	1370	1373	1375	rBV3	281	210	0.01%	0.002%
38	5.523	1389	1394	1397	rBV2	220	211	0.01%	0.002%
39	5.609	1407	1421	1448	rBV	429533	881345	61.58%	7.989%
40	5.912	1503	1515	1533	rVB7	11252	26110	1.82%	0.237%
41	5.992	1538	1540	1545	rVB2	398	193	0.01%	0.002%
42	6.063	1548	1562	1597	rBV	304500	631964	44.15%	5.728%
43	6.278	1624	1629	1630	rBV2	295	236	0.02%	0.002%
44	6.429	1673	1676	1679	rVB2	257	188	0.01%	0.002%
45	6.449	1679	1682	1685	rBV2	211	144	0.01%	0.001%
46	6.513	1698	1702	1705	rBV2	463	279	0.02%	0.003%
47	6.535	1705	1709	1713	rBV3	249	298	0.02%	0.003%
48	6.587	1722	1725	1729	rBV2	101	75	0.01%	0.001%
49	6.629	1729	1738	1739	rBV3	999	1213	0.08%	0.011%
50	6.677	1751	1753	1758	rVB	366	259	0.02%	0.002%
51	6.741	1771	1773	1778	rVB2	166	93	0.01%	0.001%
52	6.780	1778	1785	1788	rBV3	392	448	0.03%	0.004%
53	6.802	1789	1792	1794	rBV2	224	128	0.01%	0.001%
54	6.850	1804	1807	1809	rBV2	128	84	0.01%	0.001%
55	6.892	1816	1820	1823	rBV2	265	191	0.01%	0.002%
56	6.912	1823	1826	1828	rBV	143	90	0.01%	0.001%
57	6.979	1836	1847	1877	rBV	149719	277215	19.37%	2.513%
58	7.140	1895	1897	1898	rBV	309	142	0.01%	0.001%
59	7.227	1921	1924	1926	rBV2	344	224	0.02%	0.002%
60	7.307	1936	1949	1977	rBV	669764	1194773	83.47%	10.830%
61	7.616	2034	2045	2071	rBV	102332	182904	12.78%	1.658%
62	7.934	2135	2144	2152	rBV4	3707	7034	0.49%	0.064%
63	8.082	2180	2190	2225	rBV	362316	664305	46.41%	6.021%
64	8.384	2281	2284	2287	rBV4	450	356	0.02%	0.003%
65	8.616	2350	2356	2357	rBV3	391	330	0.02%	0.003%
66	8.657	2365	2369	2377	rVB3	799	796	0.06%	0.007%
67	8.699	2379	2382	2384	rBV	261	166	0.01%	0.002%
68	8.757	2398	2400	2403	rBV2	340	224	0.02%	0.002%
69	8.844	2414	2427	2459	rBV	636967	1051669	73.47%	9.532%
70	9.185	2530	2533	2536	rBV	426	261	0.02%	0.002%
71	9.252	2551	2554	2555	rBV	346	213	0.01%	0.002%
72	9.323	2573	2576	2584	rVB3	355	417	0.03%	0.004%
73	9.355	2584	2586	2587	rBV3	221	98	0.01%	0.001%
74	9.391	2594	2597	2599	rVB	153	105	0.01%	0.001%
75	9.413	2599	2604	2605	rBV2	321	204	0.01%	0.002%
76	9.513	2631	2635	2638	rBV	339	320	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW120922\
 Data File : VW029521.D
 Acq On : 09 Dec 2022 15:10
 Operator : SY/MD
 Sample : N5920-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EN7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.606	2657	2664	2667	rBV2	301	259	0.02%	0.002%
78	9.628	2667	2671	2674	rBV2	181	137	0.01%	0.001%
79	9.645	2674	2676	2677	rBV	178	98	0.01%	0.001%
80	9.702	2691	2694	2697	rBV2	211	160	0.01%	0.001%
81	9.786	2716	2720	2725	rBV2	304	314	0.02%	0.003%
82	9.899	2752	2755	2758	rBV3	172	157	0.01%	0.001%
83	9.953	2770	2772	2775	rBV	376	246	0.02%	0.002%
84	10.108	2817	2820	2821	rBV	166	79	0.01%	0.001%
85	10.162	2828	2837	2841	rBV	23529	34050	2.38%	0.309%
86	10.207	2842	2851	2873	rVB	443101	704176	49.20%	6.383%
87	10.378	2892	2904	2918	rBV4	4446	7872	0.55%	0.071%
88	10.452	2925	2927	2931	rVB2	460	313	0.02%	0.003%
89	10.567	2956	2963	2977	rVB	10626	17665	1.23%	0.160%
90	10.664	2990	2993	2995	rBV	256	174	0.01%	0.002%
91	10.702	3004	3005	3007	rBV	183	97	0.01%	0.001%
92	10.728	3011	3013	3014	rBV	206	86	0.01%	0.001%
93	10.908	3062	3069	3078	rBV3	1134	1818	0.13%	0.016%
94	11.011	3099	3101	3104	rBV2	259	161	0.01%	0.001%
95	11.085	3121	3124	3126	rBV	342	208	0.01%	0.002%
96	11.127	3134	3137	3141	rBV2	327	315	0.02%	0.003%
97	11.175	3148	3152	3160	rVB3	1008	1205	0.08%	0.011%
98	11.236	3160	3171	3196	rBV	707166	1091960	76.29%	9.898%
99	11.612	3276	3288	3310	rBV	706819	1108417	77.44%	10.047%
100	11.963	3395	3397	3399	rBV	253	121	0.01%	0.001%




Sum of corrected areas: 11032531

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029521.D
Acq On : 09 Dec 2022 15:10
Operator : SY/MD
Sample : N5920-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

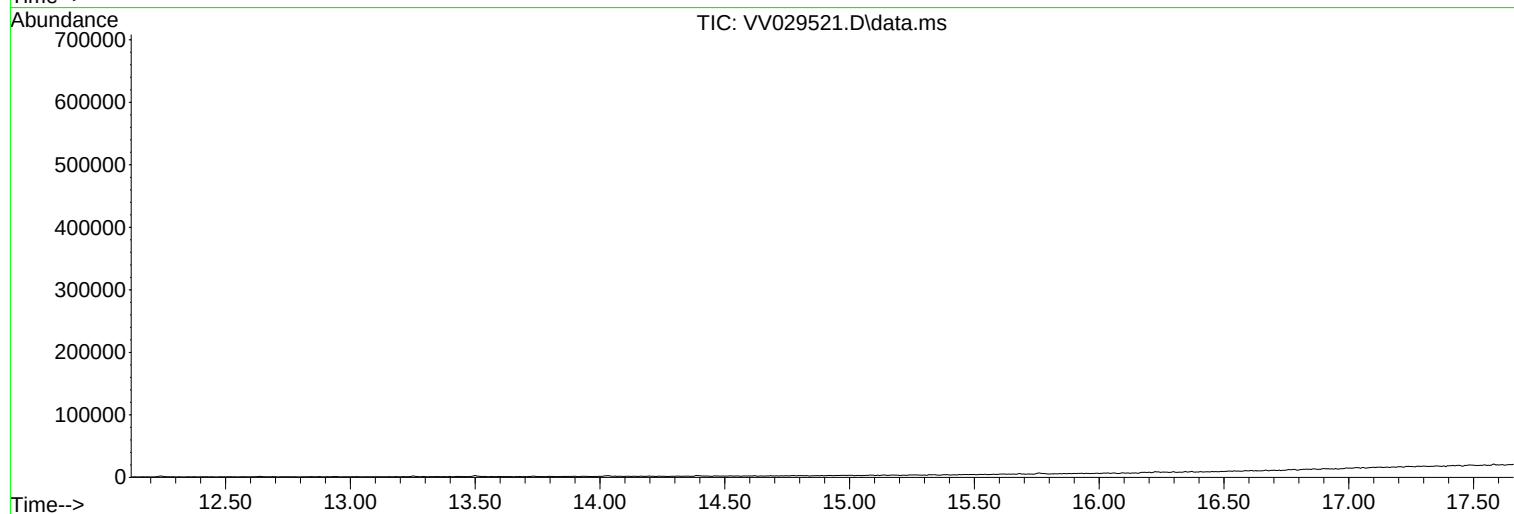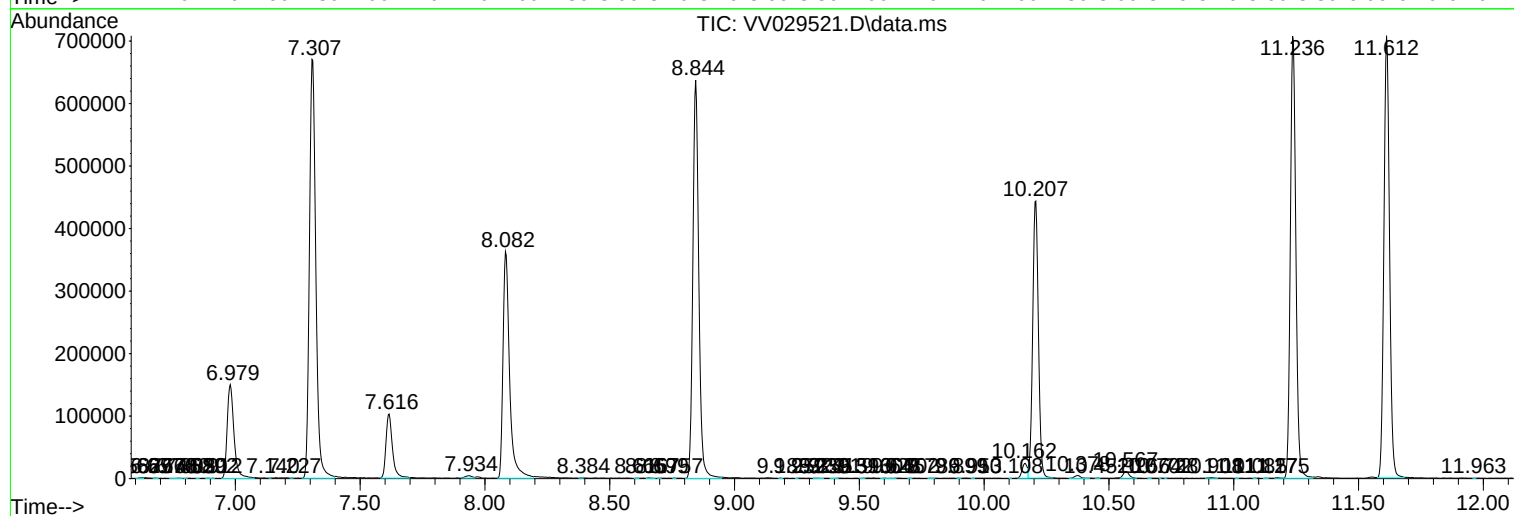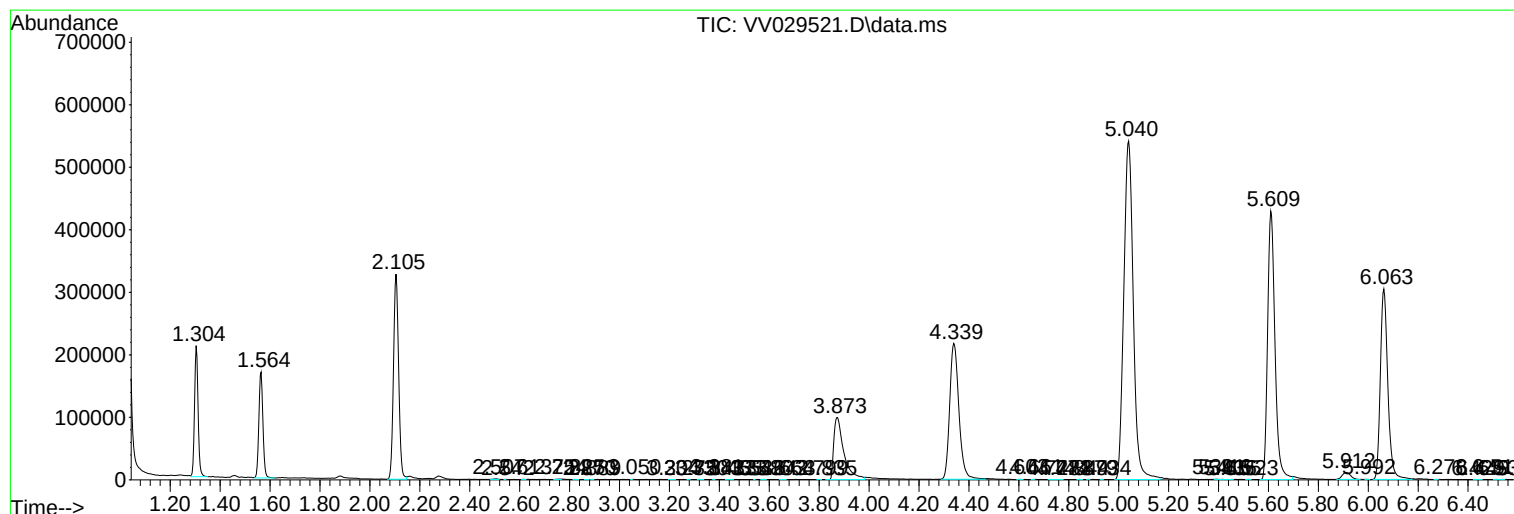

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029521.D
Acq On : 09 Dec 2022 15:10
Operator : SY/MD
Sample : N5920-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV120922\
Data File : VV029521.D
Acq On : 09 Dec 2022 15:10
Operator : SY/MD
Sample : N5920-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EN7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------